

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056742.D
 Acq On : 11 Dec 2023 19:18
 Operator : MD/SY
 Sample : 05677-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AD4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rVB	138530	158812	3.29%	1.067%
2	1.908	184	192	211	rVB	100132	139835	2.90%	0.939%
3	2.451	349	361	373	rVB2	58091	95025	1.97%	0.638%
4	2.567	383	397	412	rBV3	292563	587929	12.20%	3.948%
5	4.621	1022	1036	1042	rBV	119601	252720	5.24%	1.697%
6	5.055	1155	1171	1210	rVB	188511	462186	9.59%	3.104%
7	5.721	1355	1378	1409	rBV2	362173	950637	19.72%	6.384%
8	6.245	1527	1541	1566	rBV	286055	573354	11.90%	3.850%
9	6.534	1617	1631	1660	rBV	1175065	2252527	46.73%	15.127%
10	6.685	1665	1678	1702	rVB2	220885	438020	9.09%	2.942%
11	7.560	1937	1950	1971	rBV	92461	169725	3.52%	1.140%
12	7.894	2041	2054	2074	rBV	416602	760562	15.78%	5.108%
13	8.177	2131	2142	2156	rBV	54139	93915	1.95%	0.631%
14	8.547	2243	2257	2273	rBV	2805360	4820104	100.00%	32.370%
15	8.631	2273	2283	2320	rVB2	436917	886064	18.38%	5.950%
16	9.412	2511	2526	2563	rBV	422132	753384	15.63%	5.059%
17	10.753	2929	2943	2965	rVB	148672	244004	5.06%	1.639%
18	11.807	3258	3271	3292	rBV	383618	640255	13.28%	4.300%
19	12.187	3377	3389	3413	rBV	361377	611668	12.69%	4.108%




Sum of corrected areas: 14890726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056742.D
Acq On : 11 Dec 2023 19:18
Operator : MD/SY
Sample : 05677-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

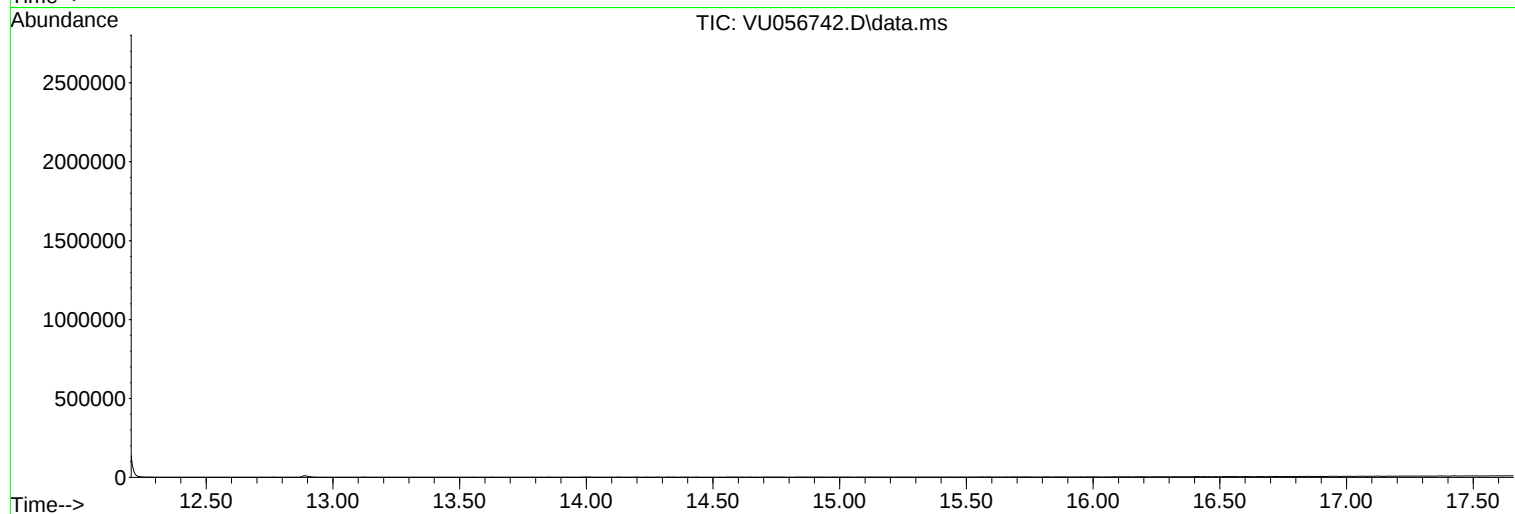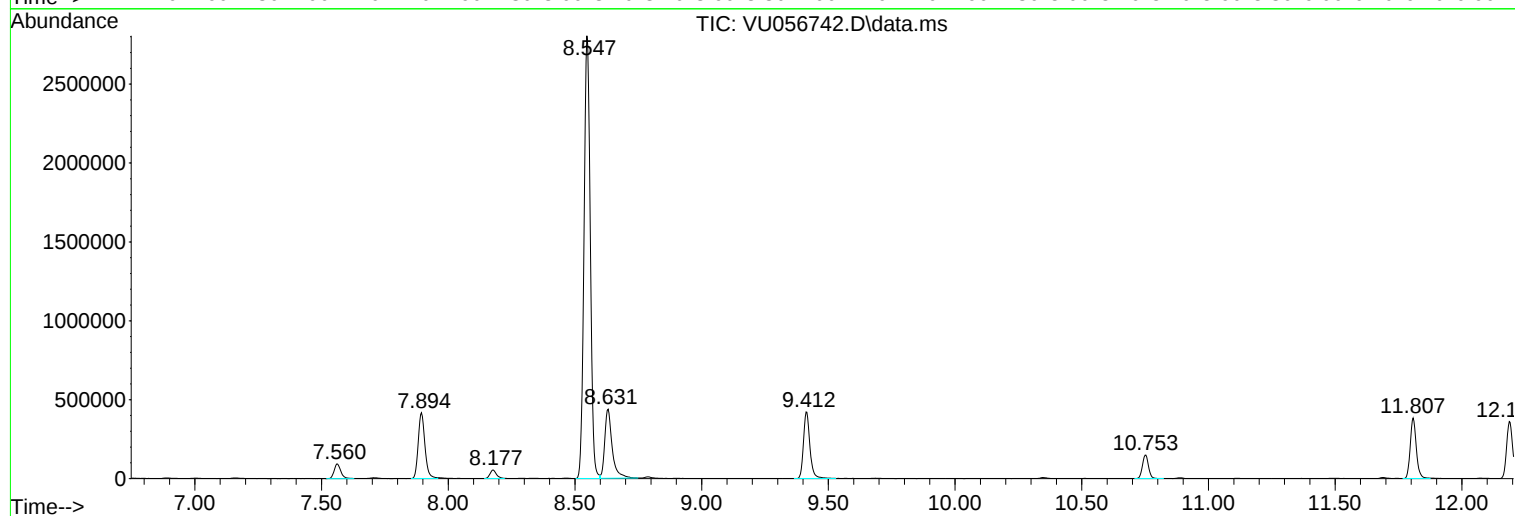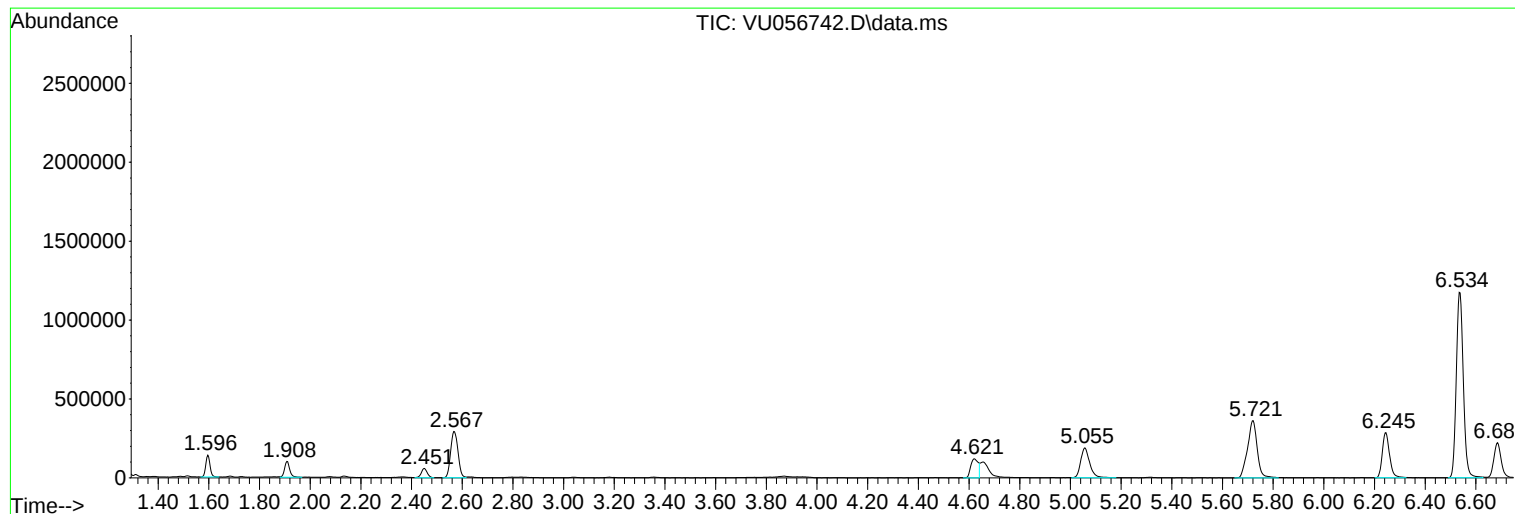

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056742.D
Acq On : 11 Dec 2023 19:18
Operator : MD/SY
Sample : 05677-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.451	0.83 ug/L	95025	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	59
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	58
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	53
4	2-Chloroethanol			80	C2H5ClO	000107-07-3	5
5	Acetyl chloride			78	C2H3ClO	000075-36-5	4

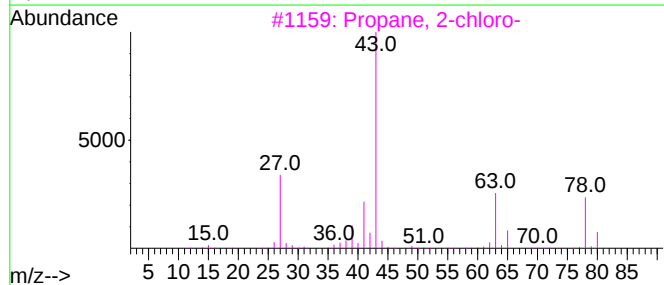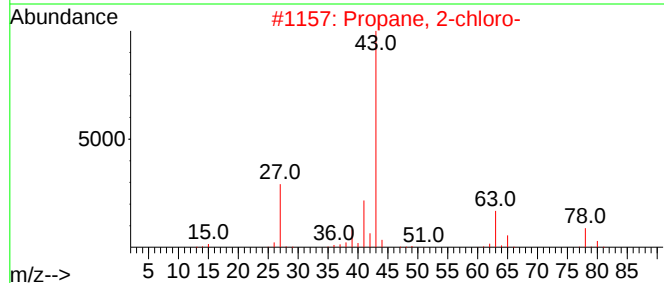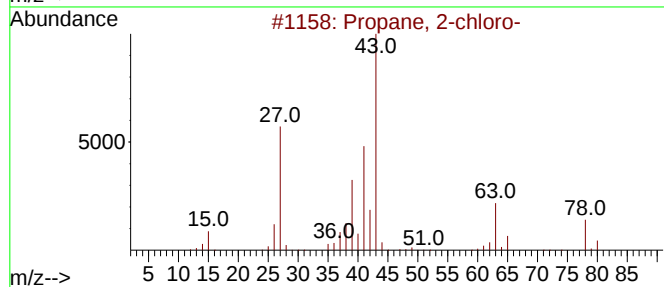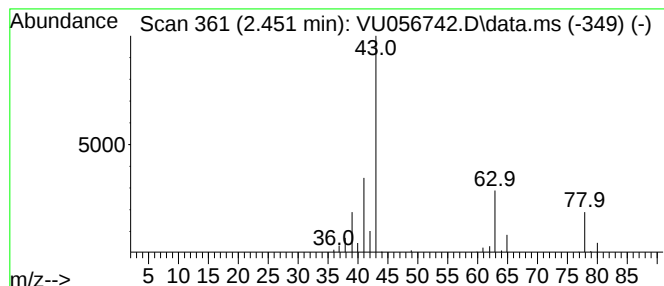

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056742.D
Acq On : 11 Dec 2023 19:18
Operator : MD/SY
Sample : 05677-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.451	0.8	ug/L	95025	1	6.245	573354	5.0