

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056761.D
 Acq On : 12 Dec 2023 03:23
 Operator : MD/SY
 Sample : 05675-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	106	rBV	138442	156729	2.97%	0.999%
2	1.907	184	192	207	rVB	101964	140485	2.66%	0.896%
3	2.451	350	361	376	rVB	34665	57602	1.09%	0.367%
4	2.567	380	397	412	rBV3	306680	596980	11.32%	3.806%
5	4.621	1024	1036	1067	rBV	135234	444069	8.42%	2.831%
6	5.055	1155	1171	1204	rVB	207185	490249	9.29%	3.126%
7	5.721	1355	1378	1411	rBV2	400004	1066684	20.22%	6.801%
8	6.245	1524	1541	1563	rBV	300487	597088	11.32%	3.807%
9	6.537	1618	1632	1659	rBV	858657	1639487	31.08%	10.454%
10	6.685	1664	1678	1697	rVV	246913	488024	9.25%	3.112%
11	7.560	1938	1950	1977	rBV2	126192	229839	4.36%	1.466%
12	7.894	2040	2054	2072	rBV	466886	863511	16.37%	5.506%
13	8.177	2131	2142	2160	rBV2	69476	126559	2.40%	0.807%
14	8.547	2242	2257	2273	rBV	3087921	5275767	100.00%	33.639%
15	8.631	2273	2283	2317	rVB2	524277	1046233	19.83%	6.671%
16	9.412	2513	2526	2546	rBV	422798	765042	14.50%	4.878%
17	10.753	2930	2943	2960	rBV	168897	285128	5.40%	1.818%
18	11.807	3258	3271	3299	rBV2	410077	693761	13.15%	4.424%
19	12.187	3377	3389	3413	rBV	420787	720068	13.65%	4.591%




Sum of corrected areas: 15683305

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056761.D
Acq On : 12 Dec 2023 03:23
Operator : MD/SY
Sample : 05675-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

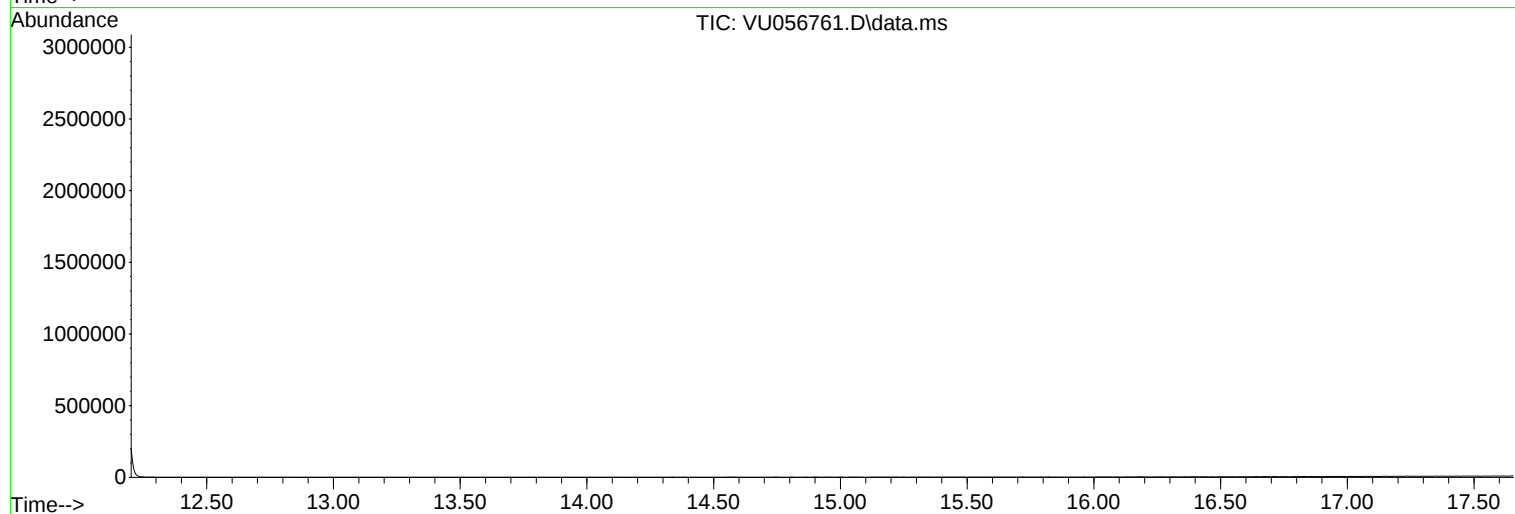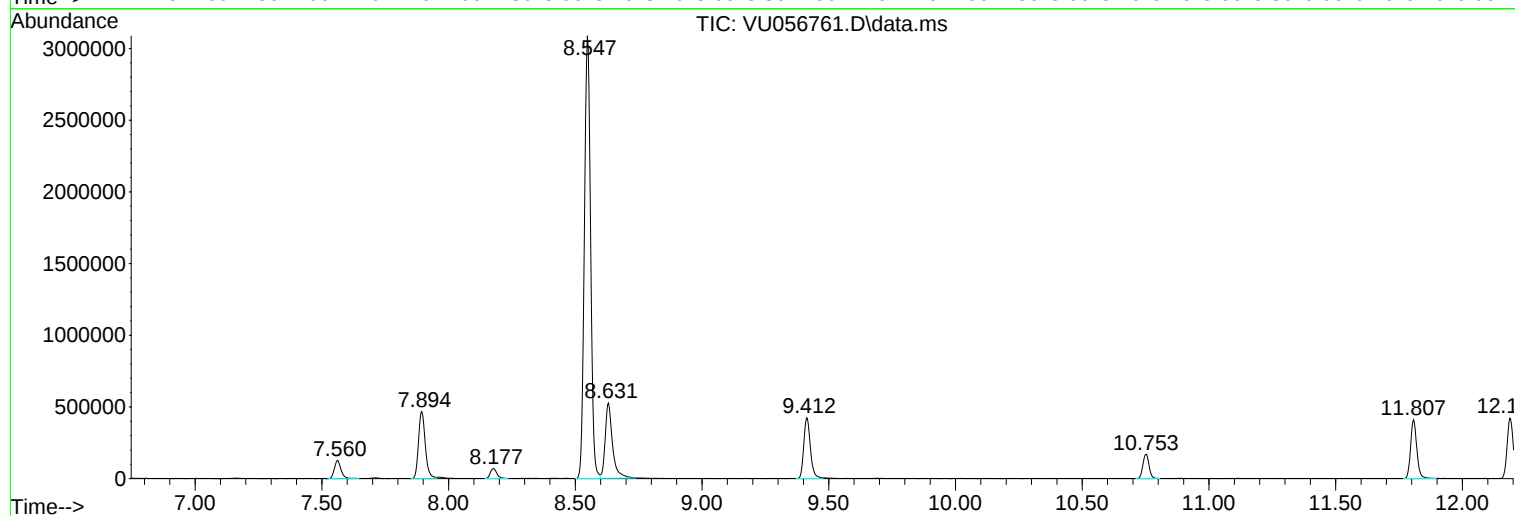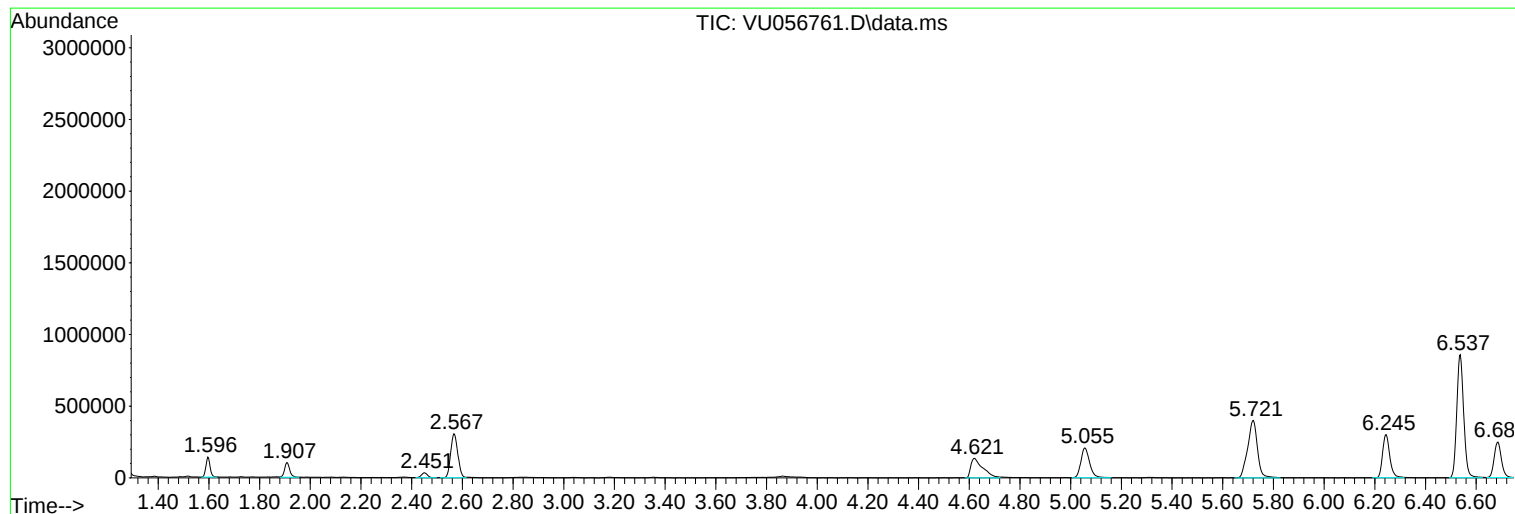

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056761.D
Acq On : 12 Dec 2023 03:23
Operator : MD/SY
Sample : 05675-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056761.D
Acq On : 12 Dec 2023 03:23
Operator : MD/SY
Sample : 05675-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
