

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056763.D
 Acq On : 12 Dec 2023 04:11
 Operator : MD/SY
 Sample : 05675-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	112	rVB	143903	165666	15.32%	1.838%
2	1.908	183	192	207	rVB	112428	155146	14.35%	1.721%
3	2.136	251	263	278	rVB	368717	555040	51.34%	6.159%
4	2.451	350	361	376	rVB	28465	50000	4.63%	0.555%
5	2.564	383	396	413	rBV	233903	383846	35.51%	4.259%
6	4.618	1024	1035	1071	rBV	135468	374543	34.65%	4.156%
7	5.055	1156	1171	1203	rBV	219786	529664	48.99%	5.877%
8	5.721	1357	1378	1403	rBV2	412756	1081068	100.00%	11.995%
9	6.245	1525	1541	1566	rBV	260425	518507	47.96%	5.753%
10	6.541	1622	1633	1647	rVB7	6847	14193	1.31%	0.157%
11	6.682	1663	1677	1698	rBV	253159	501403	46.38%	5.564%
12	7.560	1935	1950	1968	rBV	120838	220226	20.37%	2.444%
13	7.895	2040	2054	2072	rBV	470391	862341	79.77%	9.568%
14	8.178	2131	2142	2161	rBV	72543	128538	11.89%	1.426%
15	8.547	2246	2257	2271	rBV	138180	243818	22.55%	2.705%
16	8.628	2271	2282	2314	rVV2	500246	974277	90.12%	10.811%
17	9.412	2514	2526	2560	rBV	390422	700913	64.84%	7.777%
18	10.750	2930	2942	2962	rBV	172553	285032	26.37%	3.163%
19	11.808	3259	3271	3294	rBV2	337919	569874	52.71%	6.323%
20	12.187	3376	3389	3412	rBV	415615	698206	64.58%	7.747%




Sum of corrected areas: 9012301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056763.D
Acq On : 12 Dec 2023 04:11
Operator : MD/SY
Sample : 05675-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

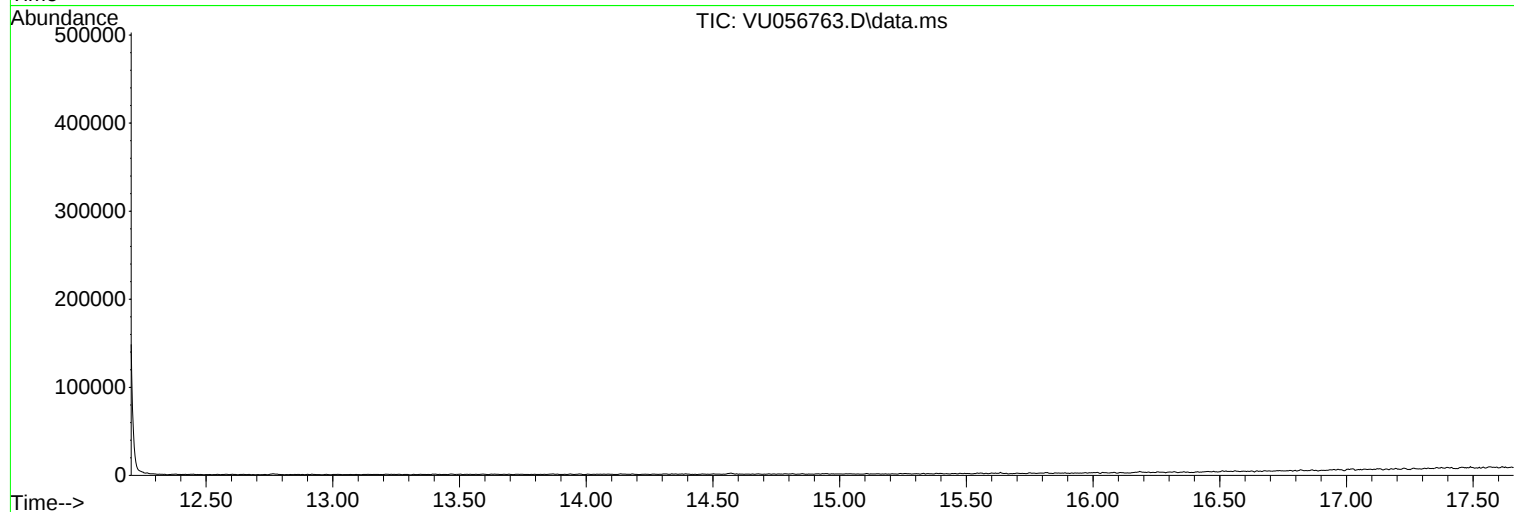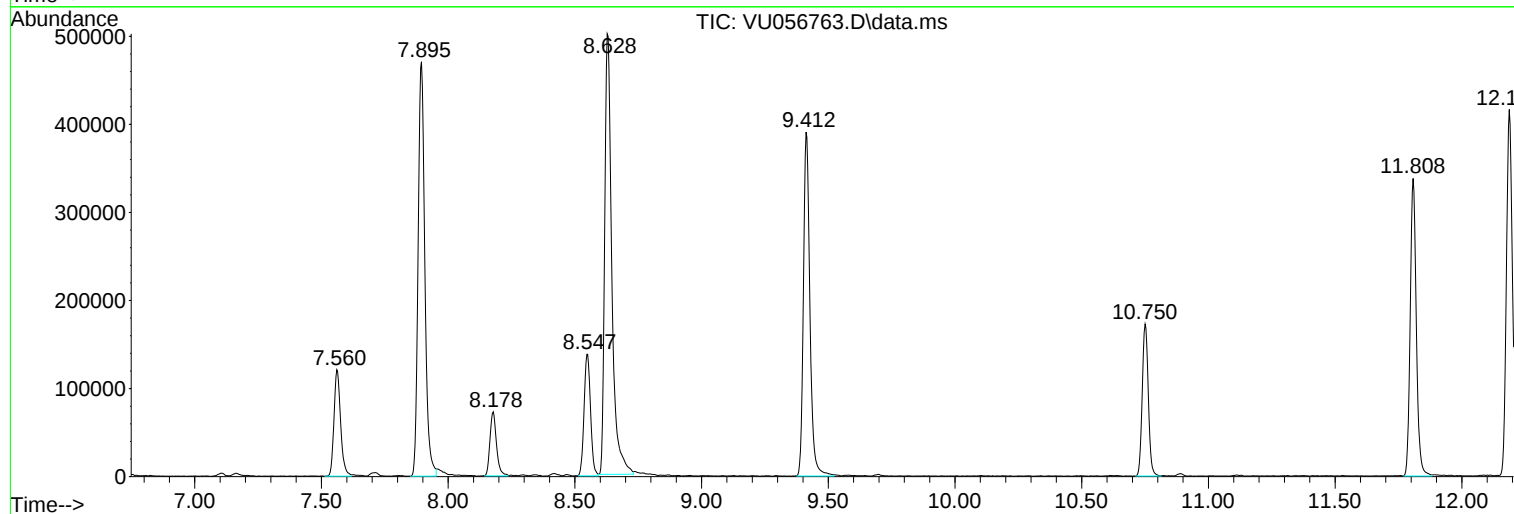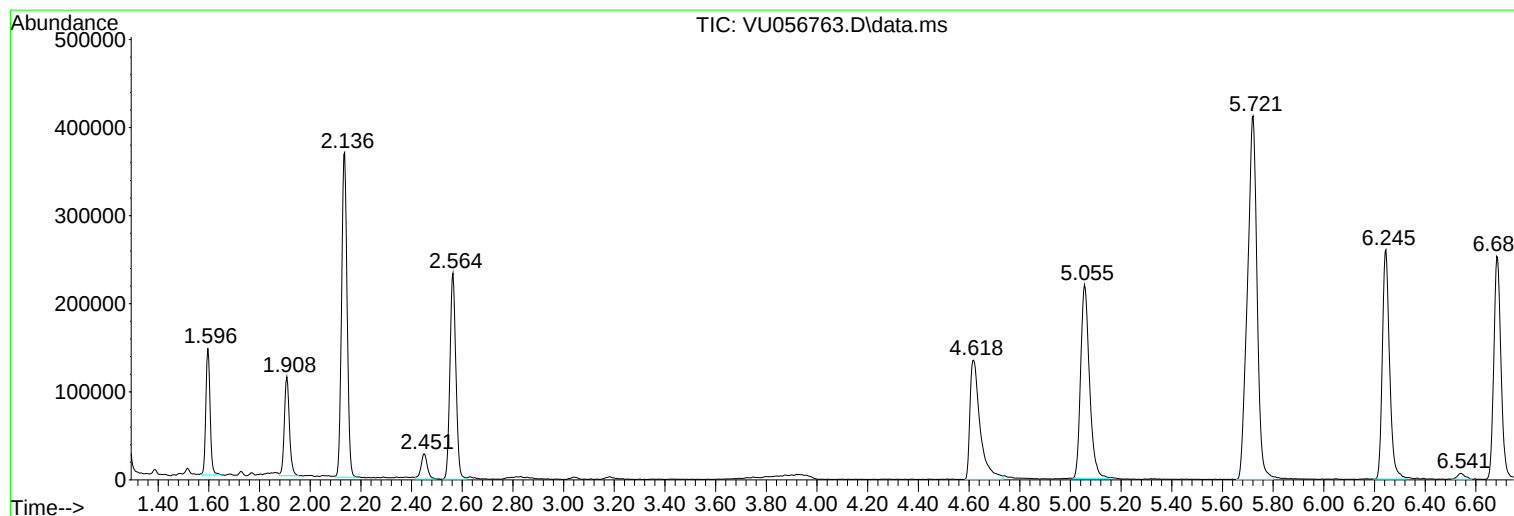

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056763.D
Acq On : 12 Dec 2023 04:11
Operator : MD/SY
Sample : 05675-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056763.D
Acq On : 12 Dec 2023 04:11
Operator : MD/SY
Sample : 05675-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc