

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056767.D
 Acq On : 12 Dec 2023 05:48
 Operator : MD/SY
 Sample : 05675-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rVB	139626	164608	3.01%	1.035%
2	1.908	184	192	207	rVB	109739	153159	2.80%	0.963%
3	2.451	349	361	374	rVB	36557	61489	1.12%	0.387%
4	2.567	383	397	413	rBV3	324740	633123	11.57%	3.981%
5	4.618	1024	1035	1073	rBV2	137177	458782	8.38%	2.885%
6	5.055	1155	1171	1194	rBV	210990	493092	9.01%	3.100%
7	5.721	1358	1378	1407	rBV2	399191	1056168	19.30%	6.641%
8	6.245	1528	1541	1569	rBV	294671	584054	10.67%	3.672%
9	6.534	1618	1631	1664	rBV	905410	1725425	31.52%	10.848%
10	6.682	1664	1677	1703	rVB	249071	496693	9.07%	3.123%
11	7.560	1936	1950	1970	rBV2	117749	219434	4.01%	1.380%
12	7.895	2038	2054	2073	rBV	469070	848933	15.51%	5.338%
13	8.174	2129	2141	2158	rBV2	71196	127461	2.33%	0.801%
14	8.547	2242	2257	2273	rBV	3217794	5473581	100.00%	34.415%
15	8.631	2273	2283	2321	rVB2	508007	1030504	18.83%	6.479%
16	9.412	2513	2526	2549	rBV	429034	753657	13.77%	4.739%
17	10.750	2930	2942	2959	rBV	169038	280019	5.12%	1.761%
18	11.808	3259	3271	3291	rBV	391061	642664	11.74%	4.041%
19	12.187	3376	3389	3411	rBV	409123	702011	12.83%	4.414%




Sum of corrected areas: 15904857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056767.D
Acq On : 12 Dec 2023 05:48
Operator : MD/SY
Sample : 05675-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

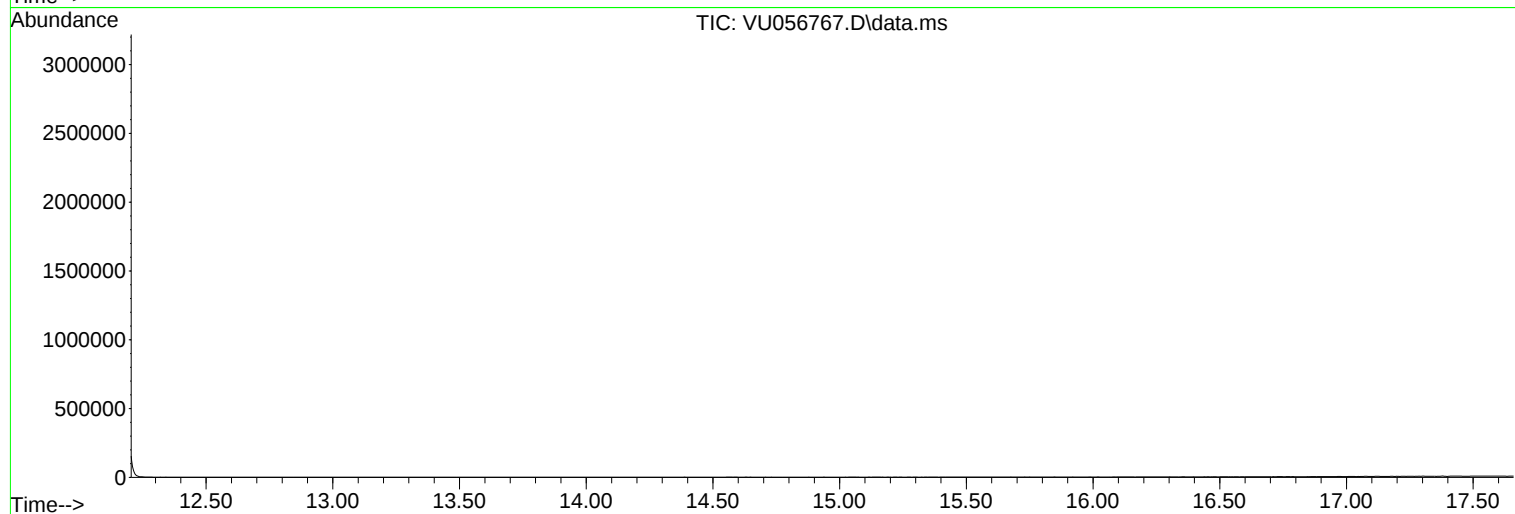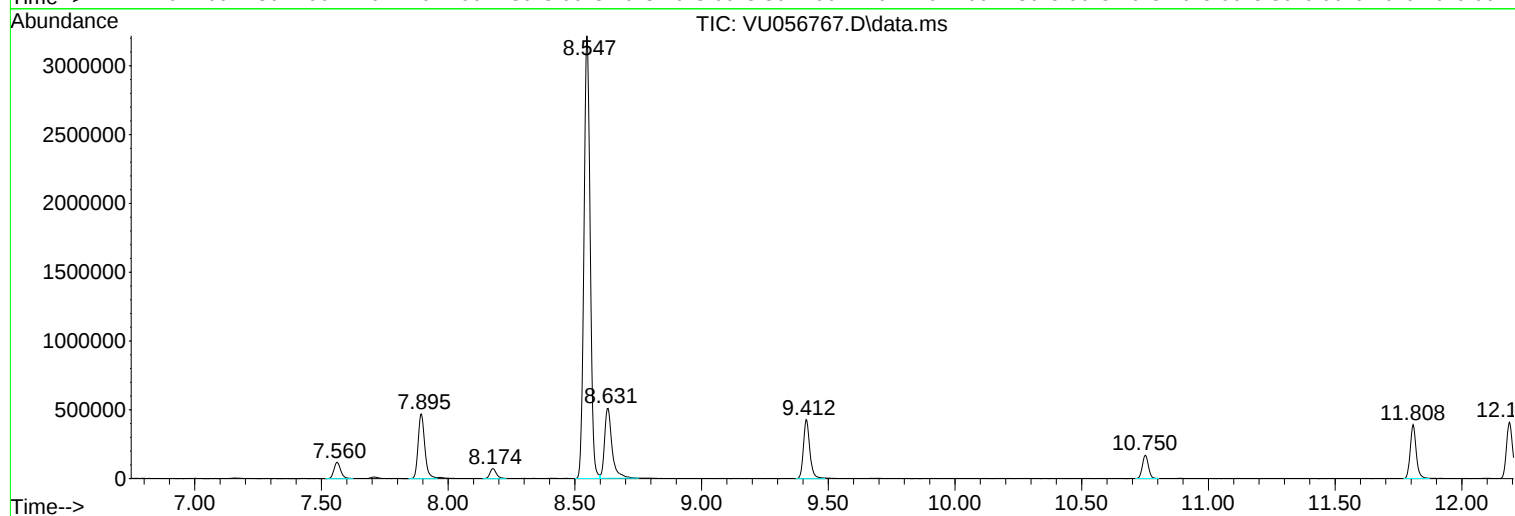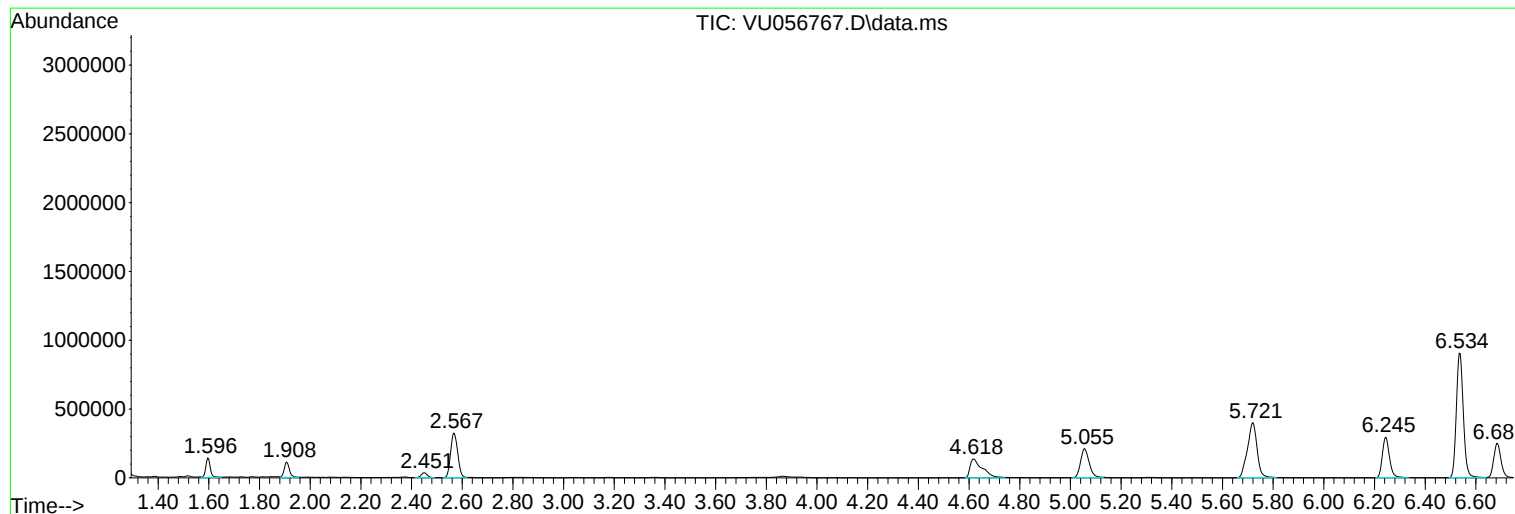

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056767.D
Acq On : 12 Dec 2023 05:48
Operator : MD/SY
Sample : 05675-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.451	0.53 ug/L	61489	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	59
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	Ethene, (methylsulfonyl)-			106	C3H6O2S	003680-02-2	4

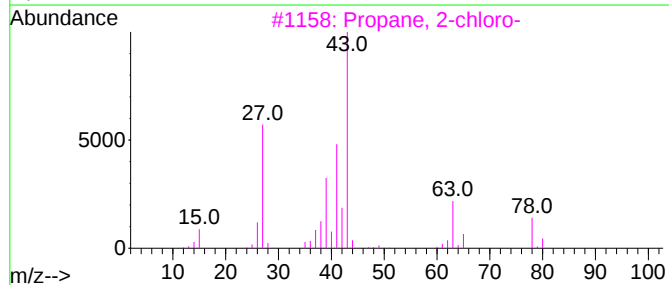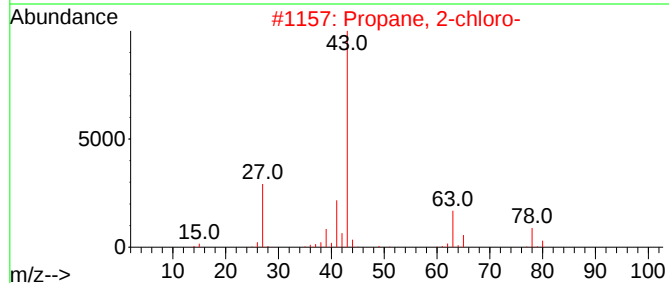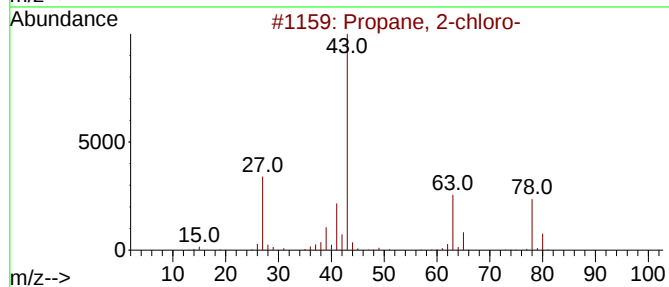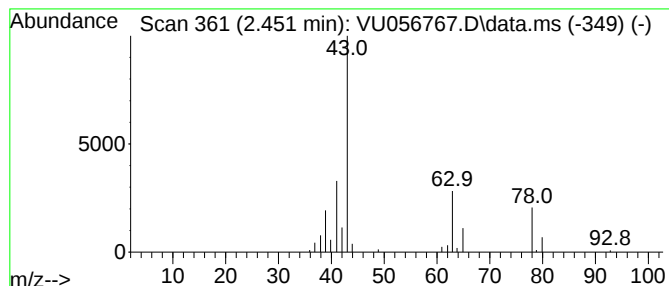

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056767.D
Acq On : 12 Dec 2023 05:48
Operator : MD/SY
Sample : 05675-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.451	0.5	ug/L	61489	1	6.245	584054	5.0