

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056770.D
 Acq On : 12 Dec 2023 07:01
 Operator : MD/SY
 Sample : 05675-20
 Misc : 25.2mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AC3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rVB	141387	164583	2.95%	1.006%
2	1.907	181	192	208	rVB	110609	157168	2.81%	0.961%
3	2.451	350	361	375	rVB	77302	124587	2.23%	0.762%
4	2.570	380	398	415	rBV3	343355	684142	12.25%	4.183%
5	4.615	1024	1034	1045	rBV	139555	342343	6.13%	2.093%
6	5.055	1155	1171	1202	rVB	221151	514557	9.21%	3.146%
7	5.721	1356	1378	1410	rBV2	415676	1080580	19.35%	6.606%
8	6.245	1528	1541	1566	rBV	282344	560632	10.04%	3.427%
9	6.534	1617	1631	1663	rBV	1021735	1986526	35.58%	12.145%
10	6.685	1663	1678	1702	rVB	256736	513166	9.19%	3.137%
11	7.560	1939	1950	1973	rBV	121683	223809	4.01%	1.368%
12	7.894	2041	2054	2074	rBV	476144	875226	15.67%	5.351%
13	8.174	2131	2141	2157	rBV	73568	128118	2.29%	0.783%
14	8.547	2243	2257	2273	rBV	3286672	5583964	100.00%	34.138%
15	8.627	2273	2282	2330	rVB2	521002	1052446	18.85%	6.434%
16	9.412	2513	2526	2551	rBV	404704	727204	13.02%	4.446%
17	10.750	2927	2942	2961	rBV	173979	285042	5.10%	1.743%
18	11.807	3258	3271	3294	rBV	385911	635751	11.39%	3.887%
19	12.187	3376	3389	3408	rBV	425196	717212	12.84%	4.385%




Sum of corrected areas: 16357056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056770.D
Acq On : 12 Dec 2023 07:01
Operator : MD/SY
Sample : 05675-20
Misc : 25.2mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

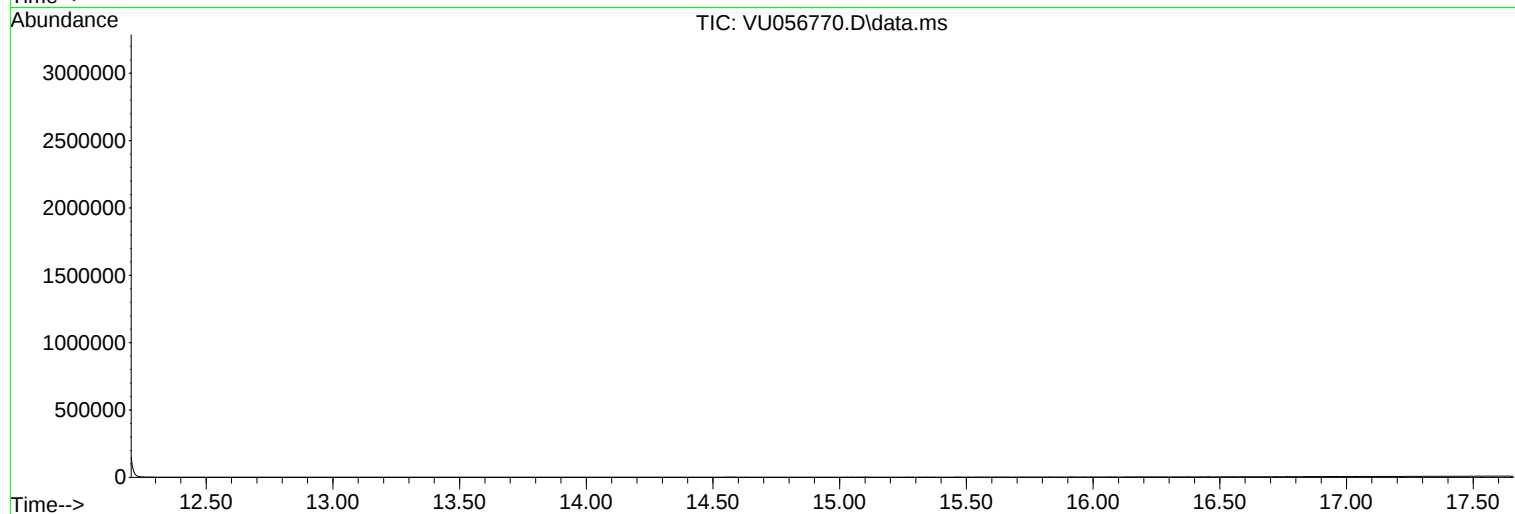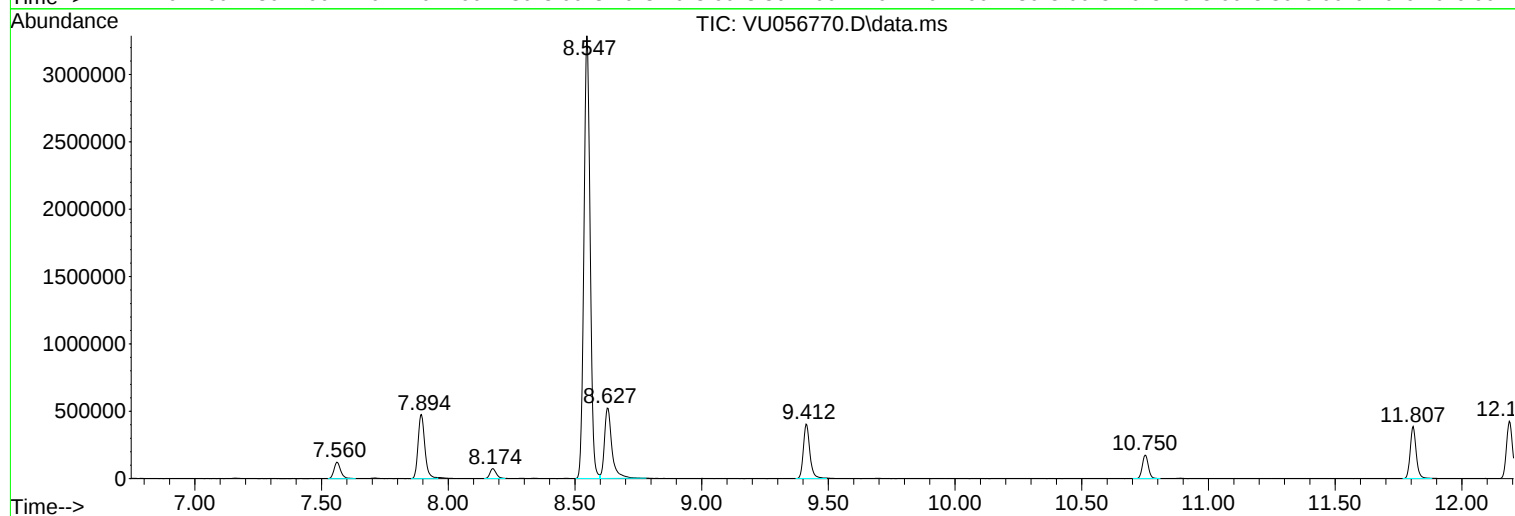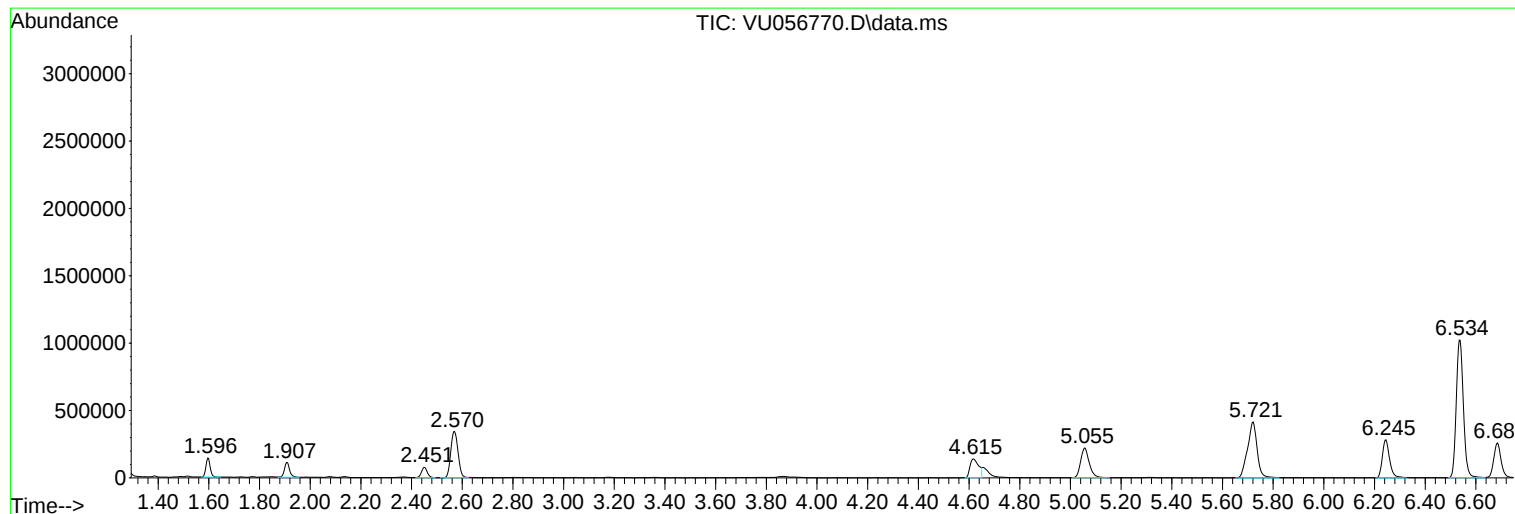

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056770.D
Acq On : 12 Dec 2023 07:01
Operator : MD/SY
Sample : 05675-20
Misc : 25.2mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC3









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.451	1.11 ug/L	124587	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	59
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	58
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	53
4			2-Chloroethanol	80	C2H5ClO	000107-07-3	5
5			2-Propyn-1-ol, acetate	98	C5H6O2	000627-09-8	4

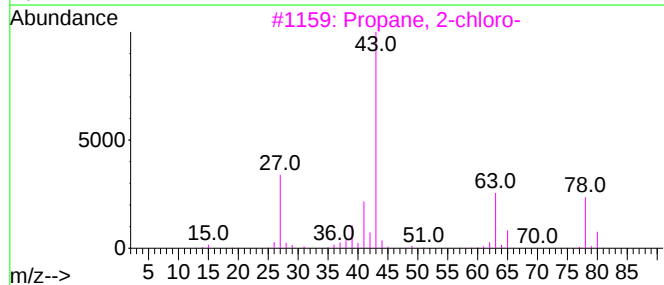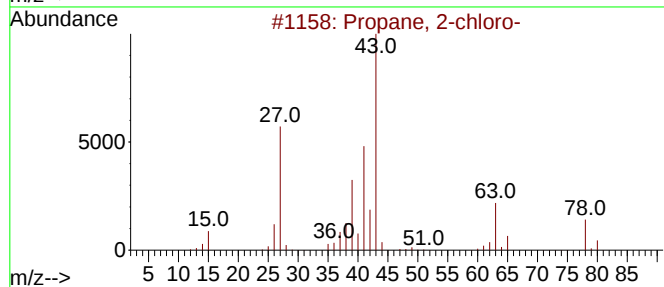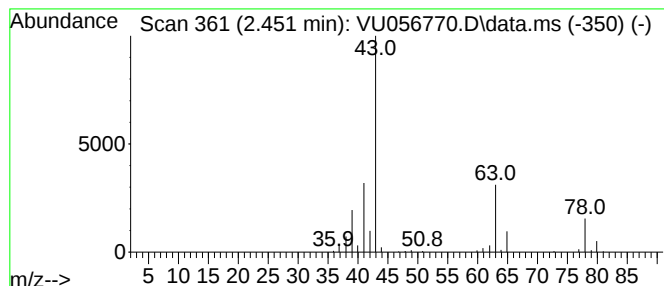

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056770.D
Acq On : 12 Dec 2023 07:01
Operator : MD/SY
Sample : 05675-20
Misc : 25.2mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.451	1.1	ug/L	124587	1	6.245	560632	5.0