


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056719.D
 Acq On : 11 Dec 2023 08:30
 Operator : MD/SY
 Sample : BFB090
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB090

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Dec 12 02:01:50 2023

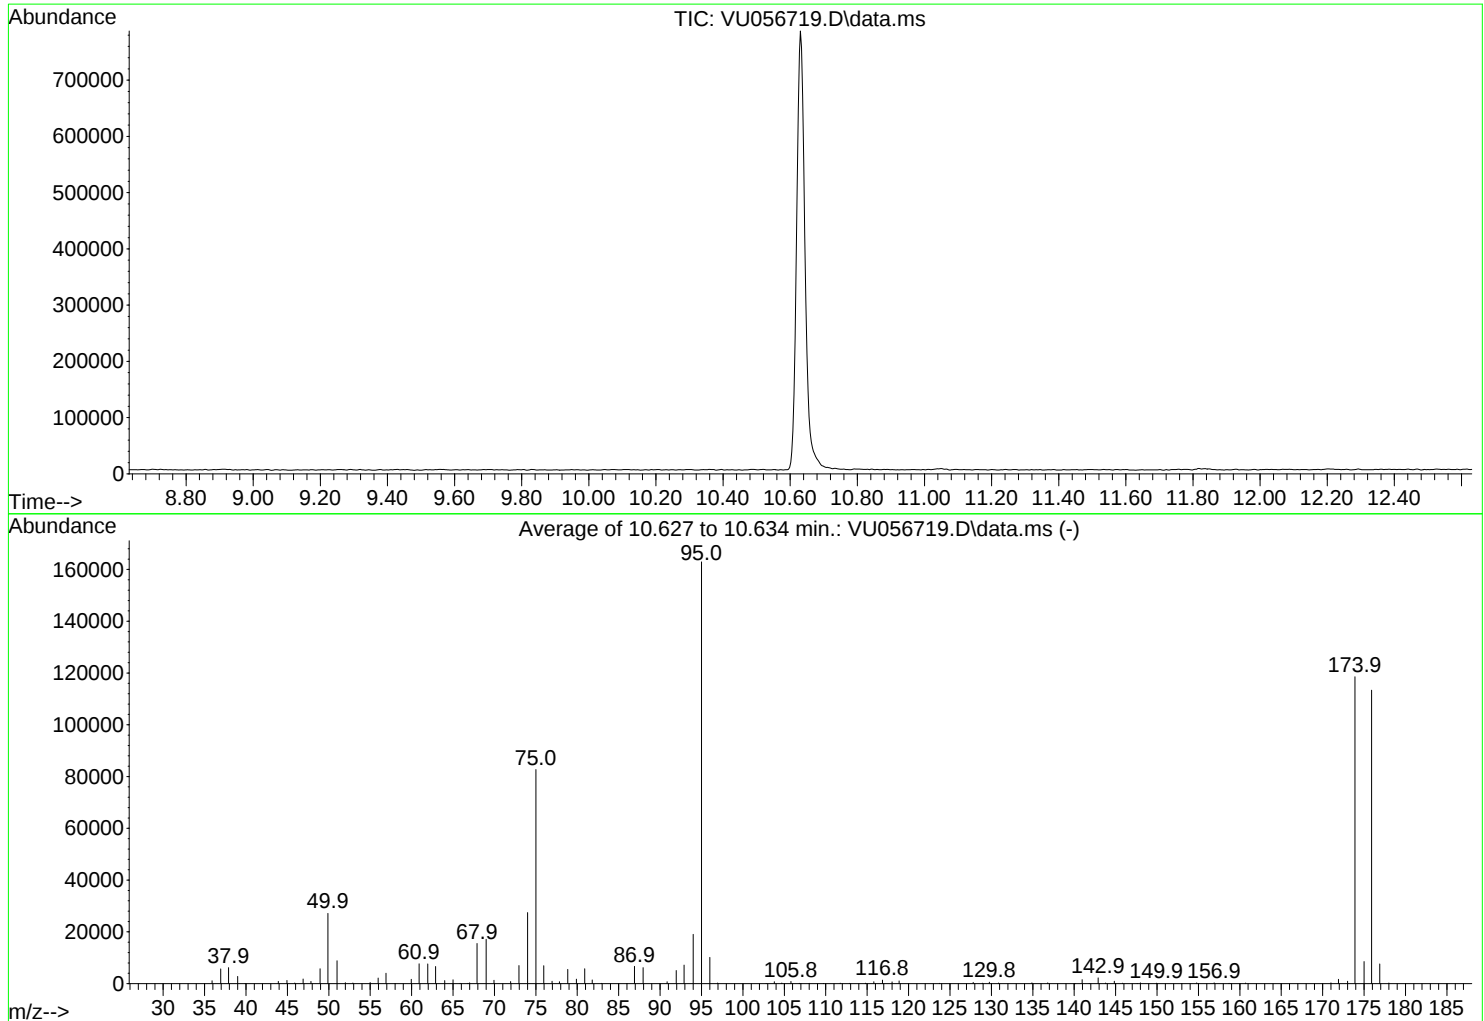

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	27139	PASS
75	95	30	80	50.8	82709	PASS
95	95	100	100	100.0	162944	PASS
96	95	5	9	6.2	10128	PASS
173	174	0.00	2	0.8	935	PASS
174	95	50	120	72.8	118552	PASS
175	174	5	9	7.2	8556	PASS
176	174	95	101	95.6	113349	PASS
177	176	5	9	6.7	7615	PASS

Scan 2890 (10.582 min): VU056719.D\data.ms
BFB090

m/z	Abundance
39.90	6771.0
43.90	409.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	1083.0
36.90	5886.0
37.90	6009.0
39.00	2720.0
39.90	7047.0
44.00	1313.0
44.90	1087.0
45.90	204.0
46.90	1882.0
47.90	904.0
49.00	5865.0
49.90	27128.0
51.00	8804.0
52.00	369.0
52.90	173.0
55.00	411.0
55.90	2280.0
56.90	4286.0
58.00	160.0
60.00	1604.0
60.90	7942.0
62.00	7448.0
62.90	6639.0
64.00	1112.0
65.00	1384.0
65.90	115.0
66.80	413.0
67.90	15482.0
69.00	16616.0
69.90	1428.0
72.00	730.0
72.90	7167.0
74.00	27248.0
75.00	82984.0
76.00	6797.0
77.00	831.0
77.90	814.0
78.80	5417.0
79.90	1741.0
80.90	5888.0
81.80	1476.0
82.90	122.0
86.00	225.0
86.90	6430.0
87.90	6171.0
90.90	782.0
91.90	4761.0
92.90	7204.0
94.00	18448.0
95.00	160256.0
96.00	10584.0
97.00	270.0
103.80	729.0
104.70	270.0
105.80	912.0
106.80	197.0
108.00	133.0
109.80	148.0
111.80	175.0
112.80	125.0
114.90	175.0
115.80	650.0
116.80	1217.0
118.00	654.0
118.80	1069.0
123.80	104.0
127.90	507.0
128.90	189.0
129.80	524.0
130.90	283.0
134.90	317.0
136.80	279.0
140.90	1528.0
142.90	2146.0
143.80	309.0
144.80	837.0
145.80	220.0
148.00	295.0
150.00	145.0
154.80	329.0
156.90	285.0
158.70	187.0
160.70	219.0
171.00	325.0
171.90	1497.0
173.90	112936.0
175.00	8461.0
175.90	107960.0
176.90	7788.0
178.00	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	1116.0
37.00	5719.0
37.90	6354.0
39.00	2915.0
39.90	6908.0
43.90	1319.0
44.90	1241.0
45.90	240.0
46.90	1841.0
47.80	932.0
49.00	5828.0
49.90	27792.0
51.00	9165.0
52.00	418.0
52.90	266.0
55.00	439.0
55.90	2195.0
56.90	4142.0
58.00	119.0
59.90	1710.0
60.90	7854.0
61.90	7843.0
62.90	6735.0
64.00	1209.0
65.00	1535.0
65.80	107.0
67.00	443.0
67.90	16120.0
69.00	17776.0
69.90	1375.0
71.90	806.0
72.90	7196.0
74.00	28288.0
75.00	84864.0
75.90	7082.0
76.90	930.0
77.90	795.0
78.80	5646.0
79.90	1782.0
80.90	6006.0
81.80	1514.0
82.90	149.0
86.90	6842.0
87.90	6378.0
90.90	746.0
92.00	5242.0
92.90	7387.0
94.00	19552.0
95.00	168192.0
96.00	10326.0
96.90	295.0
102.80	105.0
103.80	808.0
104.70	246.0
105.80	912.0
106.80	169.0
108.00	172.0
109.70	136.0
111.70	210.0
112.90	124.0
114.80	164.0
115.80	774.0
116.90	1399.0
118.00	726.0
118.90	1118.0
123.80	114.0
127.80	491.0
128.90	181.0
129.80	564.0
130.90	241.0
134.90	296.0
136.90	308.0
140.90	1604.0
142.90	2201.0
143.80	270.0
144.90	942.0
145.80	186.0
148.00	303.0
149.90	174.0
154.80	329.0
156.90	354.0
158.70	177.0
160.70	275.0
171.00	349.0
171.90	1673.0
173.00	1397.0
173.90	122152.0
175.00	8841.0
175.90	117024.0
176.90	7885.0
178.00	267.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	1184.0
37.00	5533.0
37.90	6182.0
39.00	2770.0
39.90	6623.0
43.90	1175.0
45.00	1349.0
45.90	241.0
46.90	1723.0
47.80	873.0
48.90	5564.0
49.90	26496.0
51.00	8481.0
52.00	360.0
52.90	268.0
55.00	420.0
56.00	2083.0
56.90	3670.0
59.90	1720.0
60.90	7129.0
62.00	7620.0
62.90	6406.0
64.00	1162.0
65.00	1581.0
65.80	154.0
67.00	424.0
67.90	14971.0
69.00	17080.0
70.00	1199.0
71.90	904.0
73.00	6695.0
74.00	26896.0
75.00	80280.0
75.90	6963.0
76.90	987.0
77.80	646.0
78.90	5490.0
79.90	1649.0
80.90	5434.0
81.80	1359.0
82.90	151.0
86.90	6719.0
88.00	6042.0
90.80	711.0
92.00	5212.0
92.90	6927.0
94.00	19176.0
95.00	160384.0
96.00	9473.0
96.90	277.0
102.80	130.0
103.80	784.0
104.70	190.0
105.80	744.0
107.00	184.0
108.00	156.0
111.70	160.0
113.00	102.0
114.70	174.0
115.80	742.0
116.90	1452.0
118.00	676.0
118.90	1018.0
123.70	120.0
127.70	507.0
128.90	225.0
129.70	563.0
130.80	203.0
134.90	251.0
136.70	320.0
140.00	108.0
141.00	1604.0
141.80	184.0
142.90	2259.0
143.80	195.0
144.90	946.0
145.90	187.0
147.60	277.0
148.00	265.0
149.90	192.0
153.00	152.0
154.80	282.0
156.90	371.0
158.90	137.0
160.70	233.0
171.00	245.0
171.90	1778.0
173.00	1407.0
173.90	120568.0
175.00	8365.0
175.90	115064.0
176.90	7171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

178.00

233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090