


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121218\
 Data File : VU028600.D
 Acq On : 11 Dec 2018 11:42
 Operator : MD/SY
 Sample : BFB63
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 12 05:44:10 2018

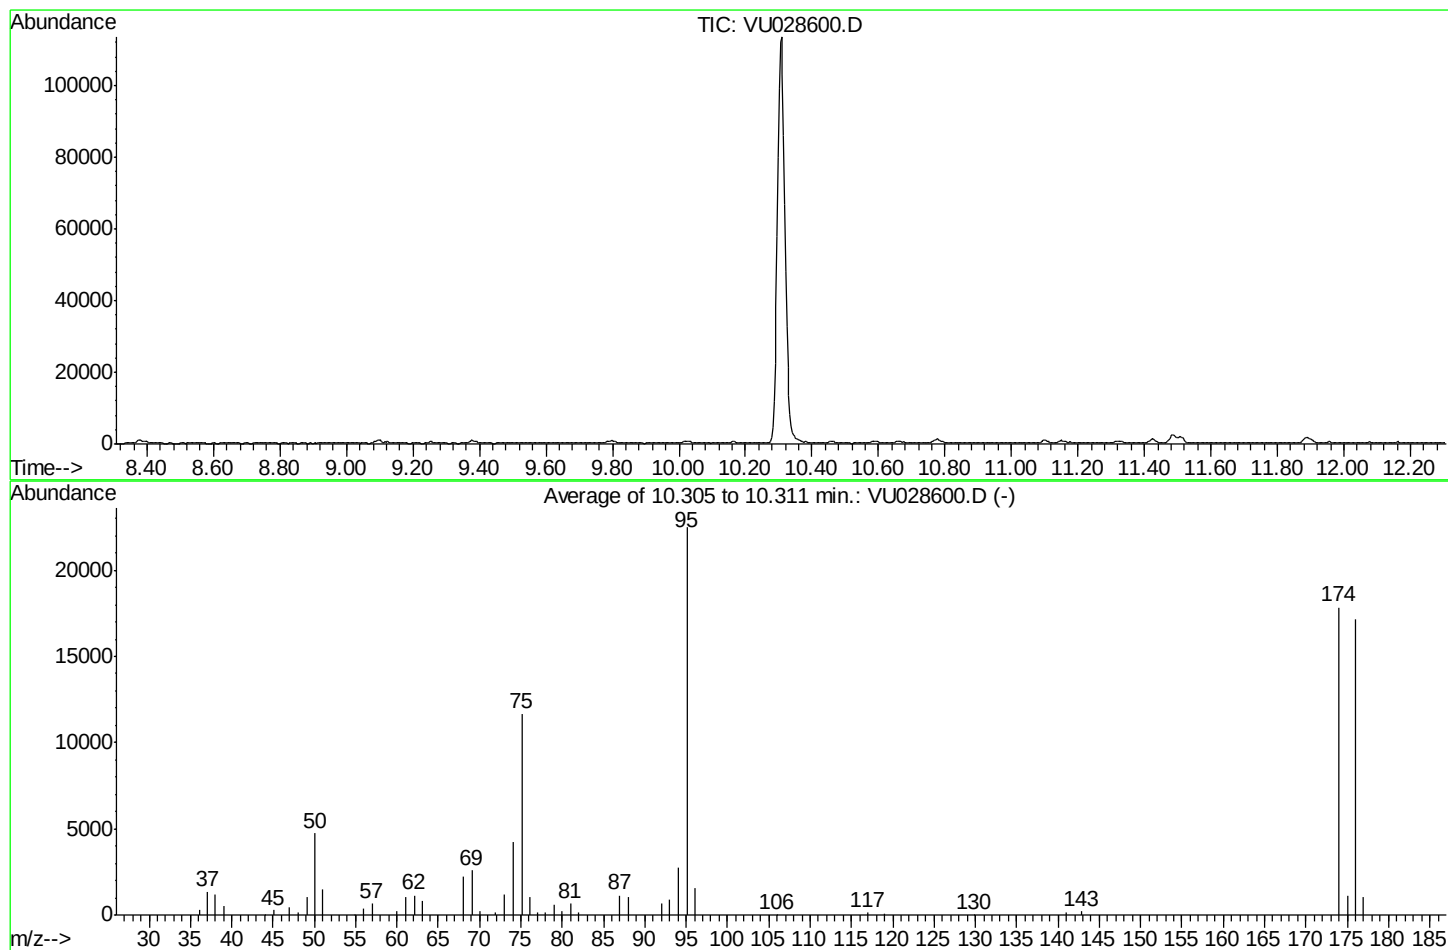

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	4747	PASS
75	95	30	80	51.9	11662	PASS
95	95	100	100	100.0	22485	PASS
96	95	5	9	6.9	1556	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.3	17837	PASS
175	174	5	9	6.4	1146	PASS
176	174	95	101	96.2	17165	PASS
177	176	5	9	6.0	1031	PASS

m/z	Abundance
36.00	358.0
37.10	1464.0
38.00	1214.0
39.00	572.0
44.00	339.0
45.10	295.0
47.00	426.0
48.00	107.0
49.10	1119.0
50.10	4876.0
51.10	1513.0
54.90	113.0
56.00	359.0
57.00	737.0
60.00	231.0
61.00	1082.0
62.10	1217.0
63.10	851.0
68.10	2342.0
69.10	2650.0
70.00	232.0
72.00	167.0
73.00	1263.0
74.10	4412.0
75.10	11974.0
76.10	1188.0
77.00	162.0
77.90	162.0
79.00	583.0
80.00	191.0
81.00	656.0
82.00	107.0
87.00	1239.0
88.00	1058.0
92.00	706.0
93.00	899.0
94.10	2775.0
95.10	22936.0
96.10	1674.0
117.00	121.0
119.00	112.0
141.00	198.0
142.90	224.0
174.00	17776.0
175.00	1160.0
176.00	17144.0
177.00	1046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB63

m/z	Abundance
44.00	320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB63

m/z	Abundance
36.10	268.0
37.10	1164.0
38.10	1085.0
39.00	504.0
44.00	364.0
45.10	253.0
47.00	380.0
48.00	118.0
49.10	924.0
50.10	4463.0
51.00	1350.0
56.00	350.0
57.00	505.0
60.00	207.0
61.00	953.0
62.10	1022.0
63.10	752.0
68.10	2105.0
69.10	2427.0
70.00	172.0
71.90	106.0
73.10	1062.0
74.10	3859.0
75.10	10971.0
76.10	807.0
77.00	192.0
77.90	186.0
79.00	614.0
79.90	232.0
81.00	638.0
82.00	128.0
87.00	965.0
88.00	986.0
92.10	614.0
93.00	793.0
94.10	2597.0
95.10	21312.0
96.10	1392.0
117.00	141.0
119.10	105.0
140.90	149.0
142.90	190.0
174.00	17232.0
175.00	1099.0
176.00	16616.0
177.00	1003.0

Instrument :
MSVOA_U
ClientSampleId :
BFB63

m/z	Abundance
36.00	335.0
37.10	1419.0
38.00	1234.0
39.00	595.0
44.00	359.0
45.10	273.0
47.00	430.0
48.00	126.0
49.10	1088.0
50.10	4903.0
51.00	1495.0
56.00	385.0
57.00	670.0
60.00	227.0
61.00	1064.0
62.10	1213.0
63.10	858.0
68.10	2306.0
69.10	2719.0
70.00	209.0
72.00	146.0
73.10	1221.0
74.10	4391.0
75.10	12041.0
76.10	1077.0
77.00	193.0
77.90	193.0
79.00	638.0
80.00	223.0
81.00	709.0
82.00	113.0
87.00	1179.0
88.00	1068.0
92.00	680.0
93.00	892.0
94.10	2774.0
95.10	23208.0
96.10	1602.0
106.00	104.0
117.00	135.0
119.00	104.0
129.90	100.0
141.00	166.0
142.90	209.0
174.00	18504.0
175.00	1180.0
176.00	17736.0
177.00	1046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB63