
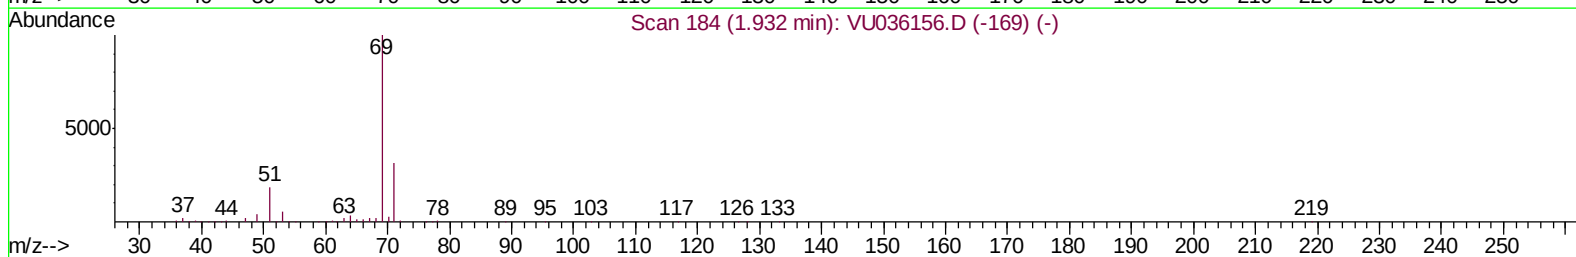
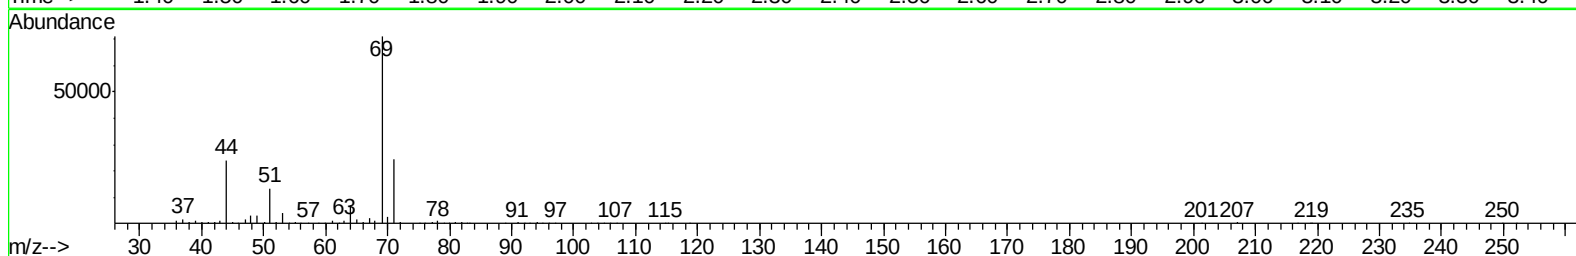


Data File : VU036160.D
Acq On : 12 Dec 2019 19:59
Operator : JC/MD
Sample : K6273-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 13 03:23:02 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 13 02:41:23 2019
Response via : Initial Calibration

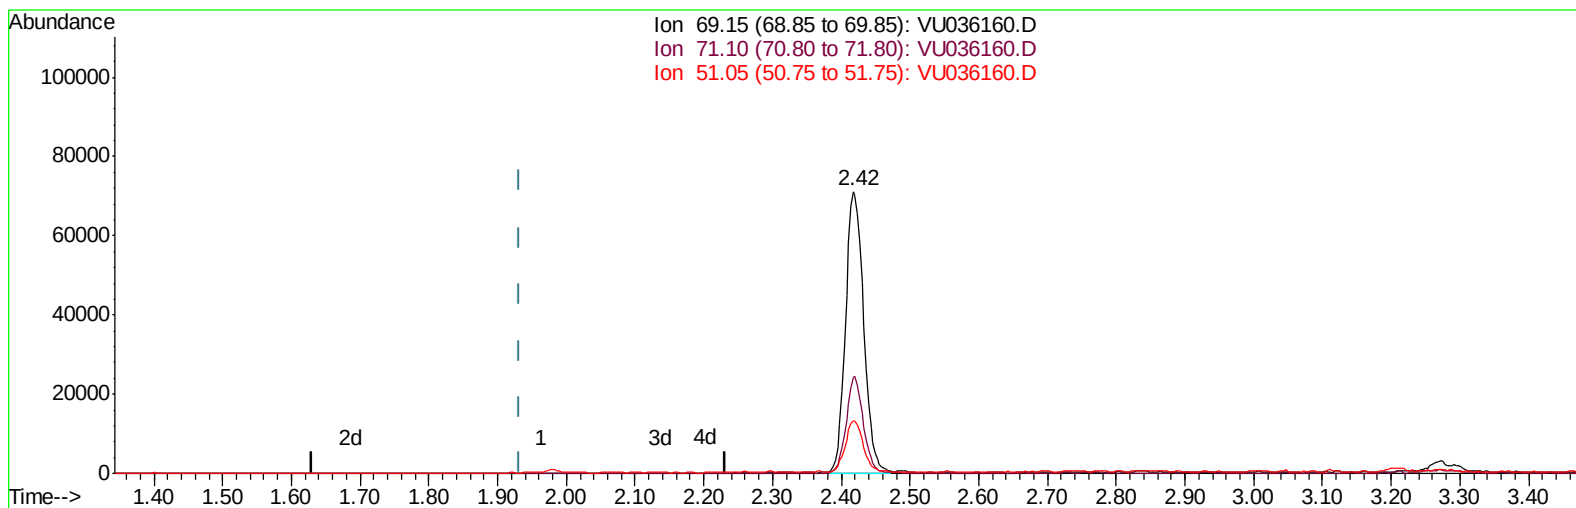

TIC: VU036160.D

(7) Chloroethane-d5 (S)

2.417min (+0.485) 7.34ug/L m

response 130649

Ion	Exp%	Act%
69.15	100	100
71.10	31.40	0.00#
51.05	25.20	1.27#
0.00	0.00	0.00