
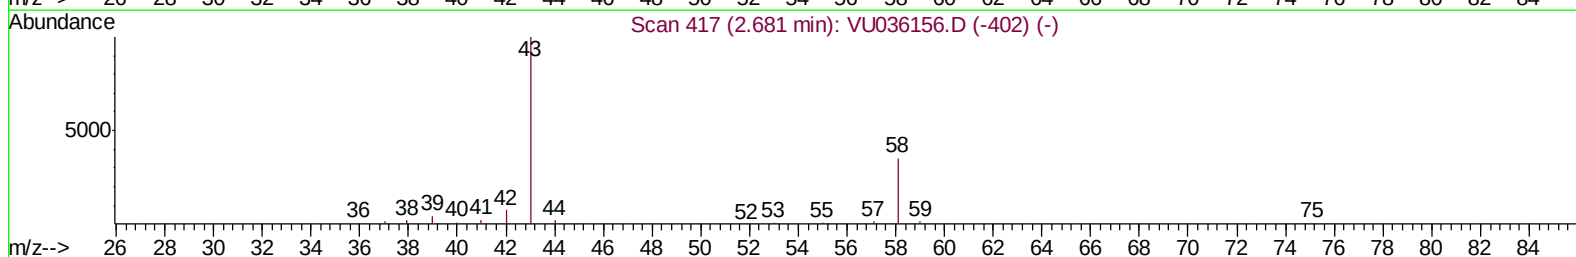
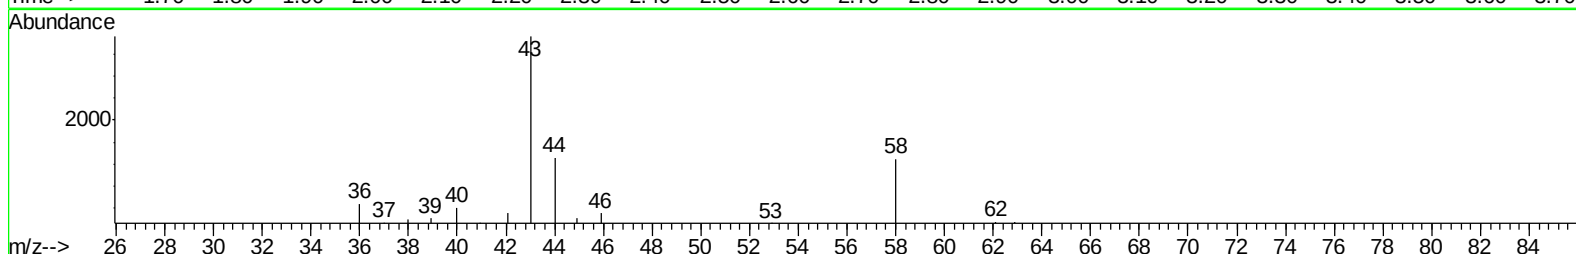


Data File : VU036163.D
Acq On : 12 Dec 2019 21:12
Operator : JC/MD
Sample : K6273-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 13 02:46:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 13 02:41:23 2019
Response via : Initial Calibration

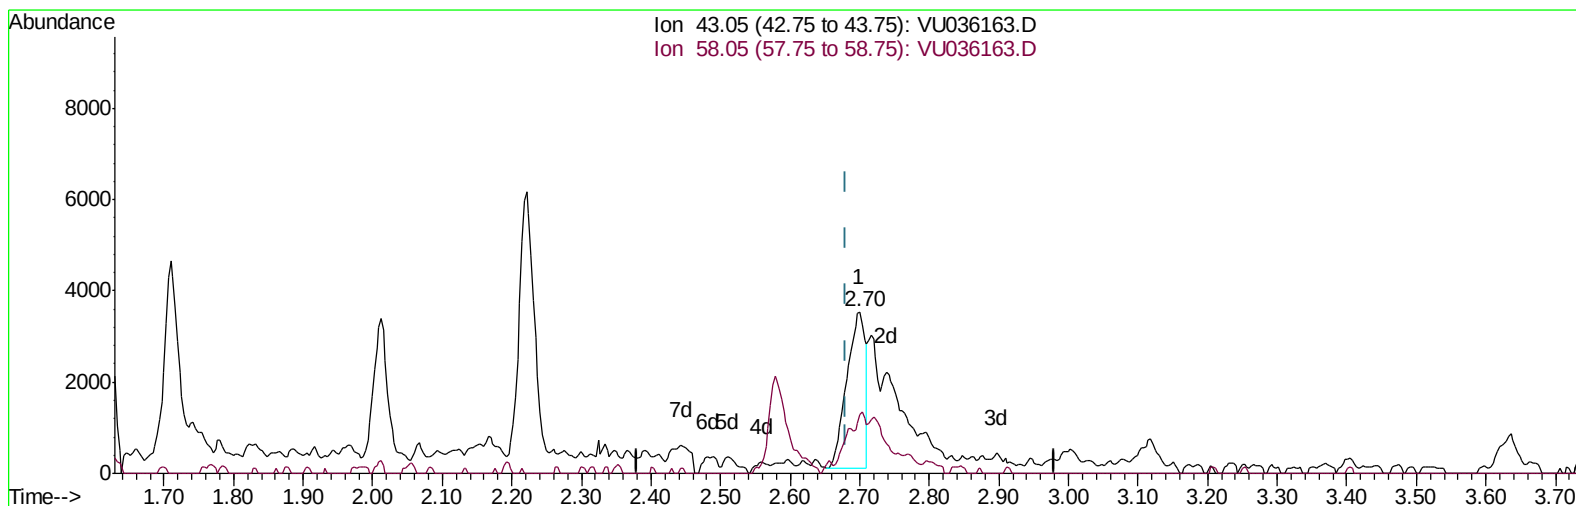

TIC: VU036163.D

(13) Acetone (T)

2.700min (+0.019) 1.82ug/L

response 6419

Ion	Exp%	Act%
43.05	100	100
58.05	35.00	30.97
0.00	0.00	0.00
0.00	0.00	0.00