

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U121219\
 Data File : VU036172.D
 Acq On : 13 Dec 2019 00:50
 Operator : JC/MD
 Sample : K6273-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFDR2

Quant Time: Dec 13 04:13:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 13 02:41:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	215780	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	244334	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	81711	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	102898	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.94	69	99944	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.00%
11) 1,1-Dichloroethene-d2	2.59	63	111605	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.40%
20) 2-Butanone-d5	4.68	46	246773	70.24	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	140.48%#
24) Chloroform-d	5.11	84	159915	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.75	65	94817	5.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.80%
32) Benzene-d6	5.77	84	320602	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.73	67	106744	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	7.93	98	250856	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	8.21	79	39442	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
46) 2-Hexanone-d5	8.68	63	177754	56.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.82%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	107728	5.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	118.80%
64) 1,2-Dichlorobenzene-d4	12.22	152	89990	5.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.00%

Target Compounds


					Ovalue
13) Acetone	2.66	43	31697	10.371 ug/L	98
14) Carbon disulfide	2.83	76	16470	0.305 ug/L	95
22) cis-1,2-Dichloroethene	4.72	96	3212	0.185 ug/L	96
25) Chloroform	5.13	83	16906	0.515 ug/L	100
34) Trichloroethene	6.58	95	27843	1.449 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121219\
Data File : VU036172.D
Acq On : 13 Dec 2019 00:50
Operator : JC/MD
Sample : K6273-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDR2

Quant Time: Dec 13 04:13:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 13 02:41:23 2019
Response via : Initial Calibration

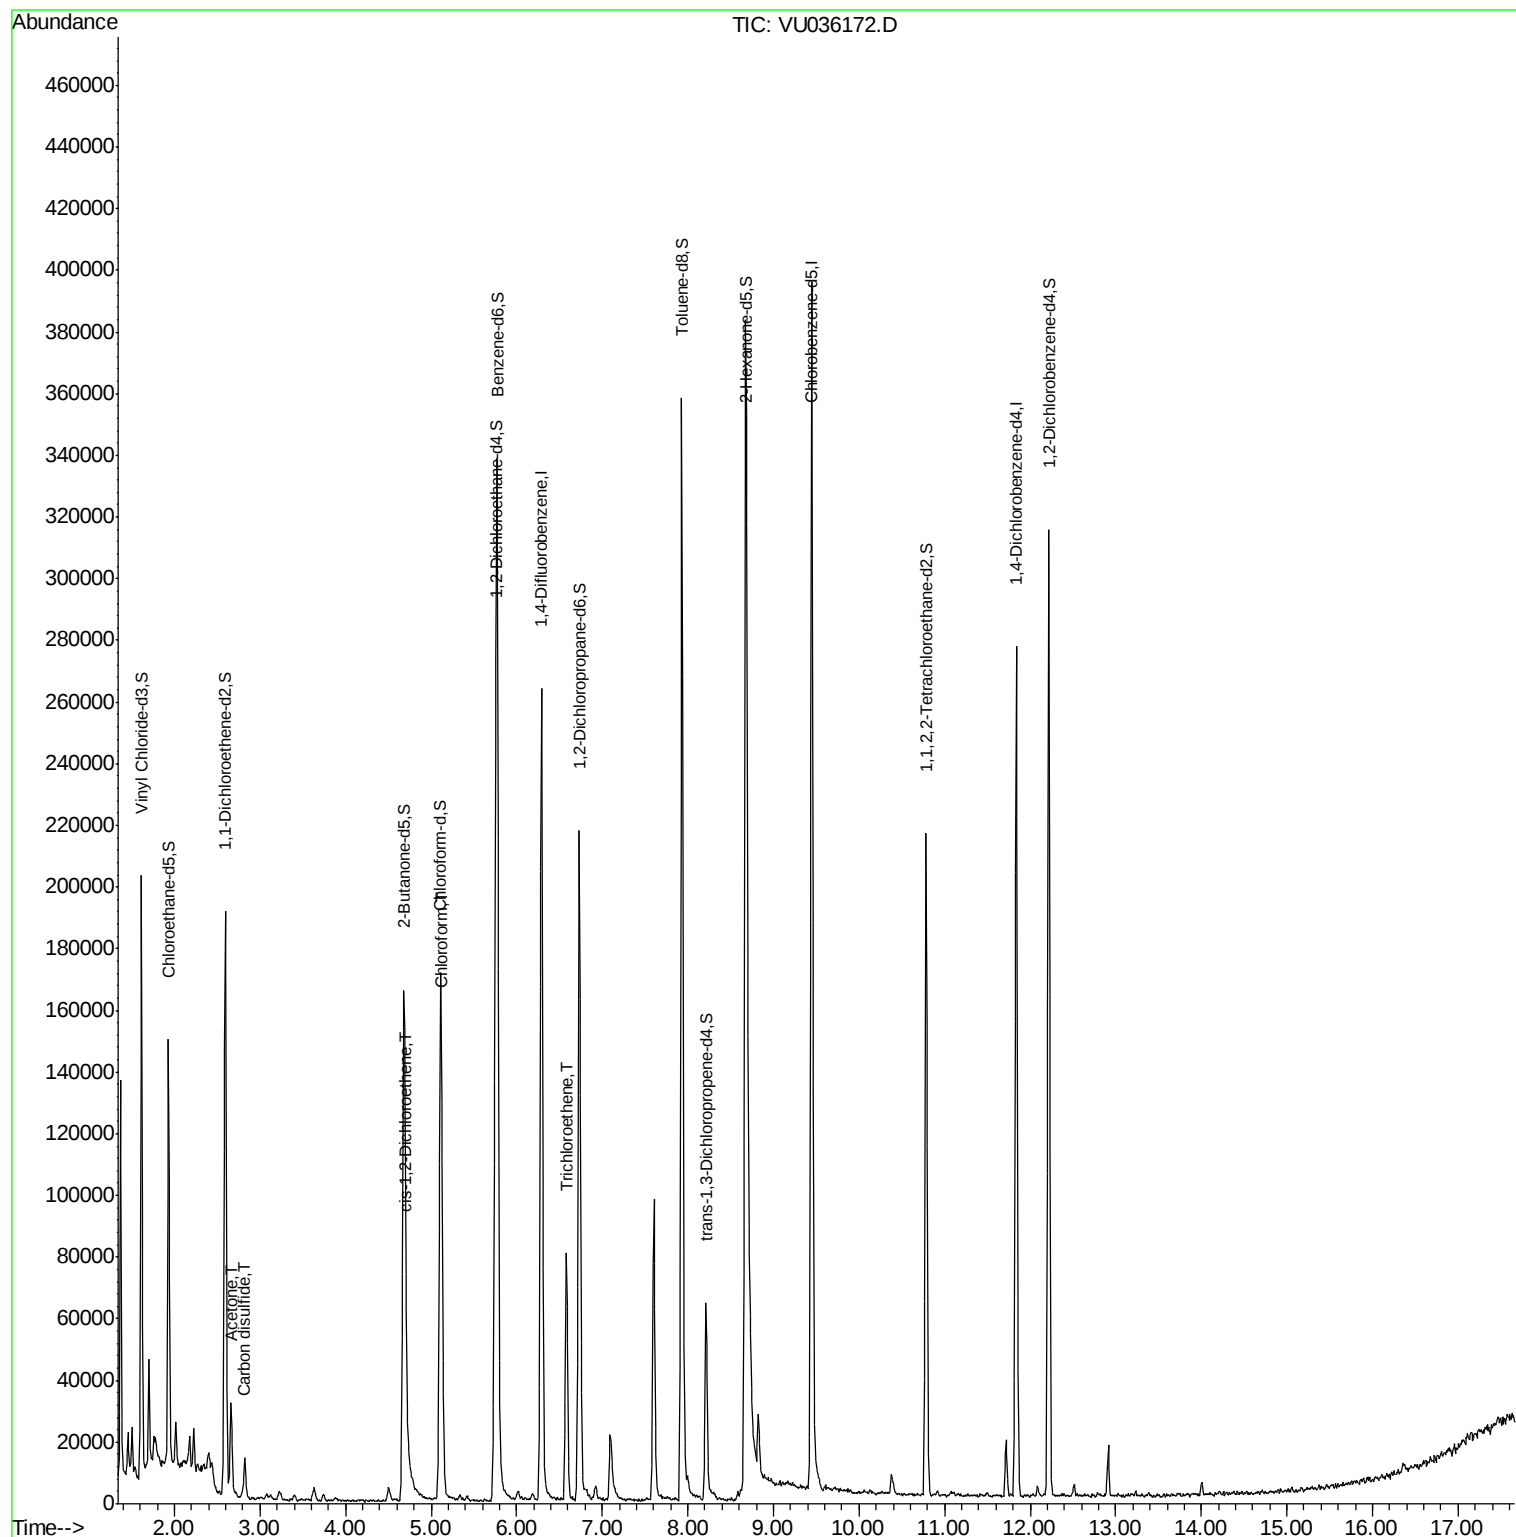

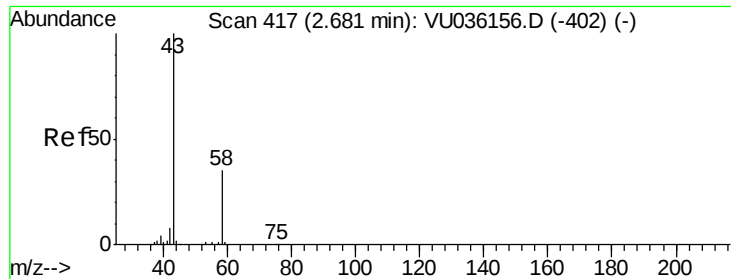

#13

Acetone

Concen: 10.371 ug/L

RT: 2.66 min Scan# 411

Delta R.T. -0.02 min

Lab File: VU036172.D

Acq: 13 Dec 2019 00:50

Instrument :

MSVOA_U

ClientSampleId :


BFDR2

Tot Ion: 43 Resp: 31697




Ion Ratio Lower Upper

43 100

58 36.1 0.0 70.0

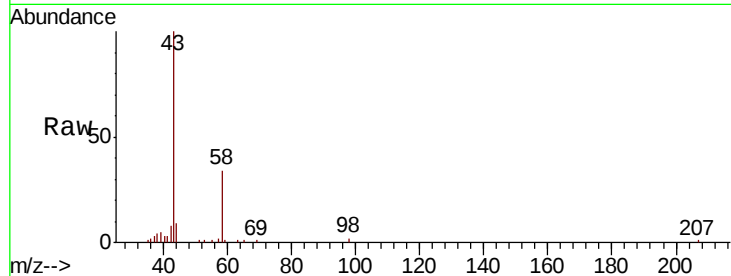

Abundance Ion 43.05 (42.75 to 43.75): VU036172.D (-324) (-)

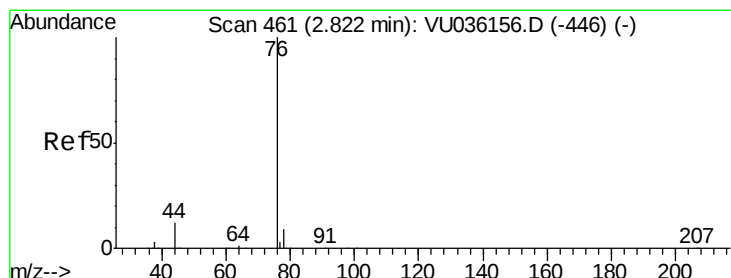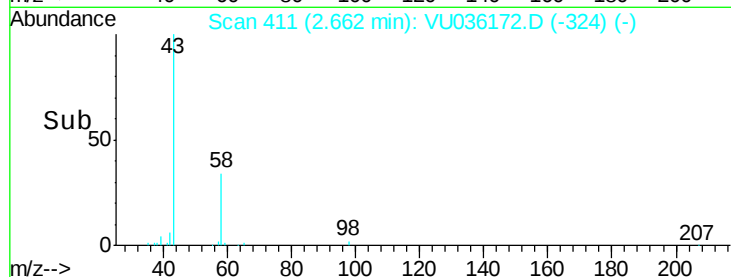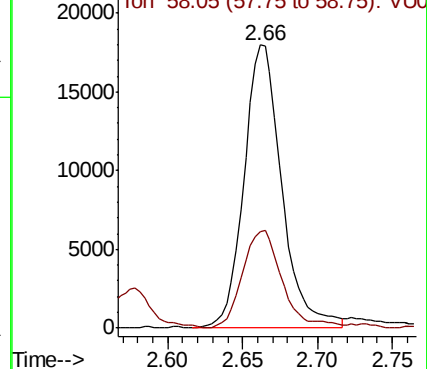

#14

Carbon disulfide

Concen: 0.305 ug/L

RT: 2.83 min Scan# 462

Delta R.T. 0.00 min

Lab File: VU036172.D


Acq: 13 Dec 2019 00:50

Tgt Ion: 76 Resp: 16470



Ion Ratio Lower Upper


76 100

78 7.3 7.2 10.8

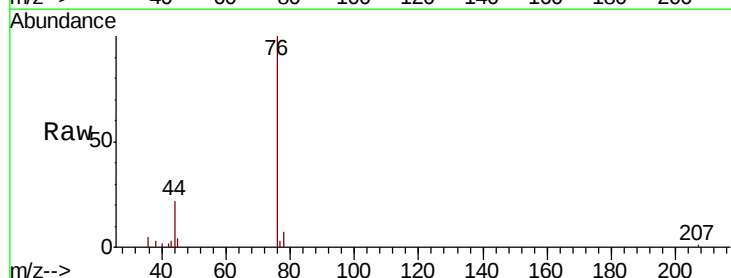

Abundance Ion 76.05 (75.75 to 76.75): VU036172.D (-368) (-)



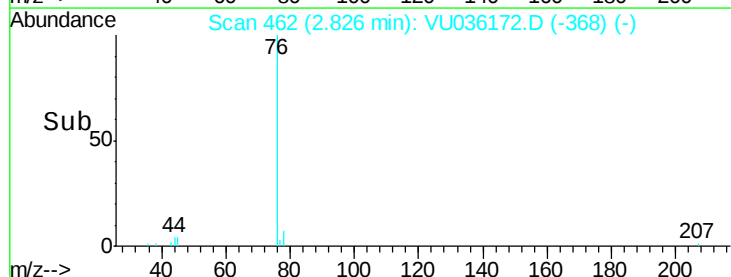
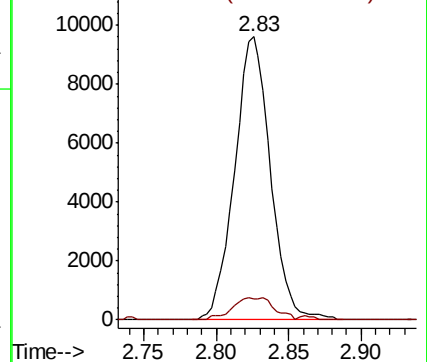


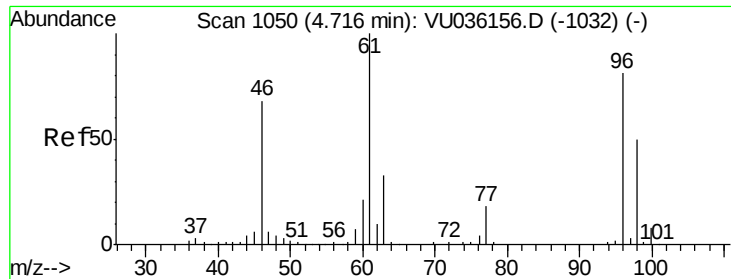

#22
 cis-1,2-Dichloroethene
 Concen: 0.185 ug/L
 RT: 4.72 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VU036172.D
 Acq: 13 Dec 2019 00:50




Instrument :
 MSVOA_U
 ClientSampleId :
 BFDR2


Tot Ion: 96 Resp: 3212
 Ion Ratio Lower Upper
 96 100
 61 115.2 83.8 155.6
 68 0.0 0.0 0.0

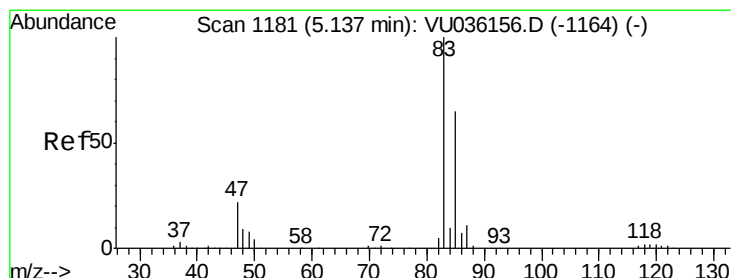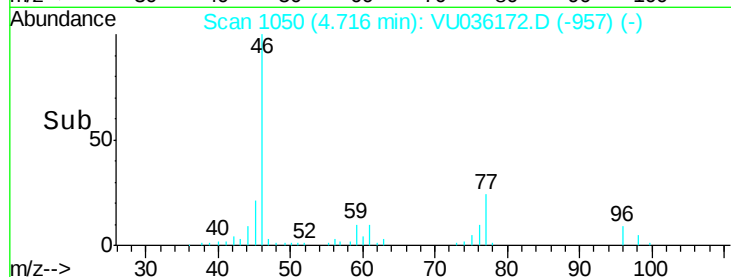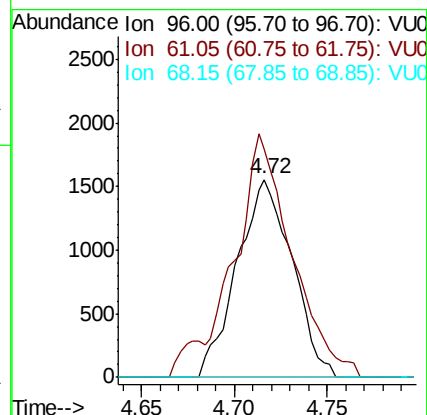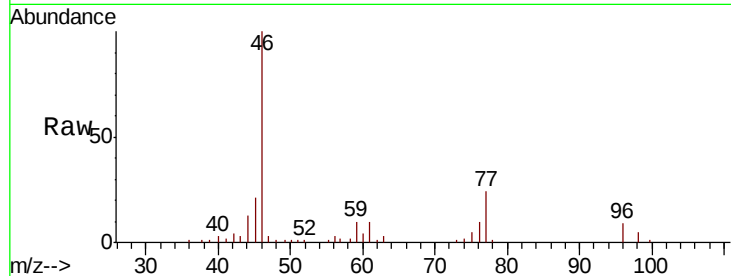

#25
 Chloroform
 Concen: 0.515 ug/L
 RT: 5.13 min Scan# 1179
 Delta R.T. -0.01 min
 Lab File: VU036172.D
 Acq: 13 Dec 2019 00:50

Tgt Ion: 83 Resp: 16906
 Ion Ratio Lower Upper
 83 100
 85 63.2 44.2 82.0

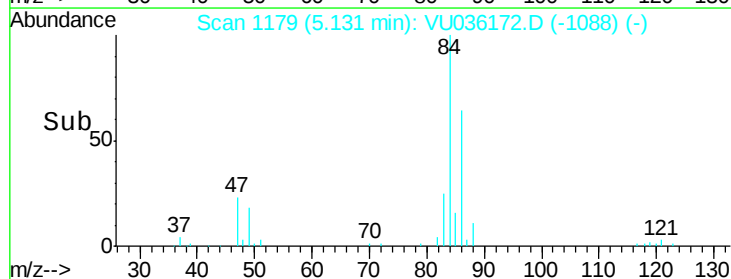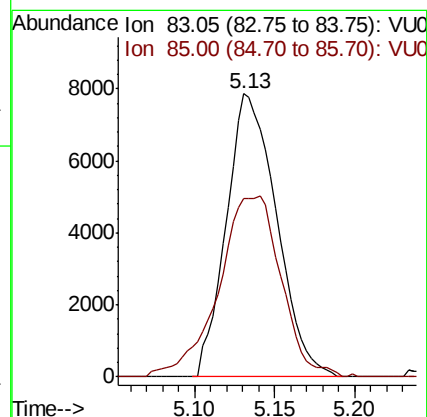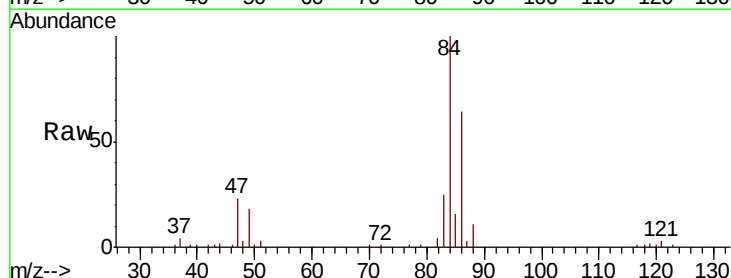

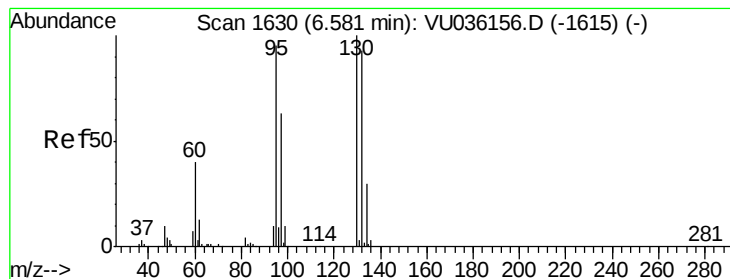

#34

Trichloroethene

Concen: 1.449 ug/L

RT: 6.58 min Scan# 1630

Delta R.T. 0.00 min

Lab File: VU036172.D


Acq: 13 Dec 2019 00:50

Instrument :

MSVOA_U

ClientSampleId :

BFDR2

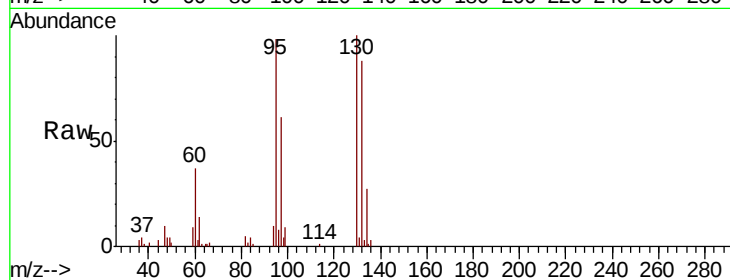

Tot Ion: 95 Resp: 27843


Ion Ratio Lower Upper

95 100

97 62.6 43.7 81.1

132 89.3 71.7 133.3

130 101.9 73.1 135.7

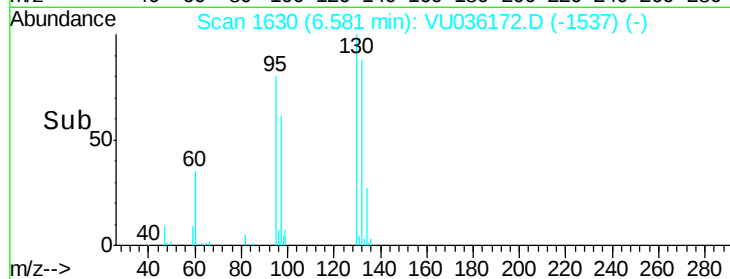

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

