

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U121219\
 Data File : VU036183.D
 Acq On : 13 Dec 2019 05:41
 Operator : JC/MD
 Sample : K6240-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW2

Manual Integrations
 APPROVED

apatel
 12/13/2019 3:58:52 PM

Quant Time: Dec 13 08:14:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 13 04:38:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	254004	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	281275	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	116896	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	106757	4.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.00%
7) Chloroethane-d5	1.93	69	104939	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.80%
11) 1,1-Dichloroethene-d2	2.59	63	111625	3.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.80%
20) 2-Butanone-d5	4.70	46	220060	53.21	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.42%
24) Chloroform-d	5.11	84	178383	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.75	65	91300	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.77	84	329672	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	6.73	67	107825	4.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.20%
41) Toluene-d8	7.93	98	260963	3.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.20%
43) trans-1,3-Dichloropropene-	8.21	79	35232	3.60	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.00%
46) 2-Hexanone-d5	8.68	63	164072	45.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.26%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	96385	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	12.21	152	110587	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.62	62	81648	2.407	ug/L	97
8) Chloroethane	1.95	64	34087	1.632	ug/L	98
13) Acetone	2.68	43	82030	22.801	ug/L	99
15) Methyl Acetate	2.99	43	3157m	0.412	ug/L	
16) Methylene chloride	3.09	84	7336	0.274	ug/L	94
19) 1,1-Dichloroethane	3.92	63	162686	4.454	ug/L	99
21) 2-Butanone	4.78	43	9586	1.999	ug/L	88
22) cis-1,2-Dichloroethene	4.72	96	116448	5.697	ug/L	95
29) 1,1,1-Trichloroethane	5.36	97	62423	1.810	ug/L	98
33) Benzene	5.82	78	105475	1.219	ug/L	100
34) Trichloroethene	6.58	95	10176	0.460	ug/L	93
42) Toluene	8.00	91	45592	0.498	ug/L	96
51) Chlorobenzene	9.48	112	10079	0.169	ug/L	90
52) Ethylbenzene	9.60	91	9226	0.103	ug/L	96
53) m,p-Xylene	9.72	106	10039	0.287	ug/L	82
54) o-Xylene	10.13	106	6932	0.207	ug/L	98
63) 1,4-Dichlorobenzene	11.86	146	5826	0.155	ug/L	97

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121219\
Data File : VU036183.D
Acq On : 13 Dec 2019 05:41
Operator : JC/MD
Sample : K6240-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQW2

Manual Integrations
APPROVED

apatel
12/13/2019 3:58:52 PM

Quant Time: Dec 13 08:14:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 13 04:38:02 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
65) 1,2-Dichlorobenzene	12.24	146	7382	0.200	ug/L #	84
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121219\
Data File : VU036183.D
Acq On : 13 Dec 2019 05:41
Operator : JC/MD
Sample : K6240-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BFQW2

Manual Integrations
APPROVED

apatel
12/13/2019 3:58:52 PM

Quant Time: Dec 13 08:14:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 13 04:38:02 2019
Response via : Initial Calibration

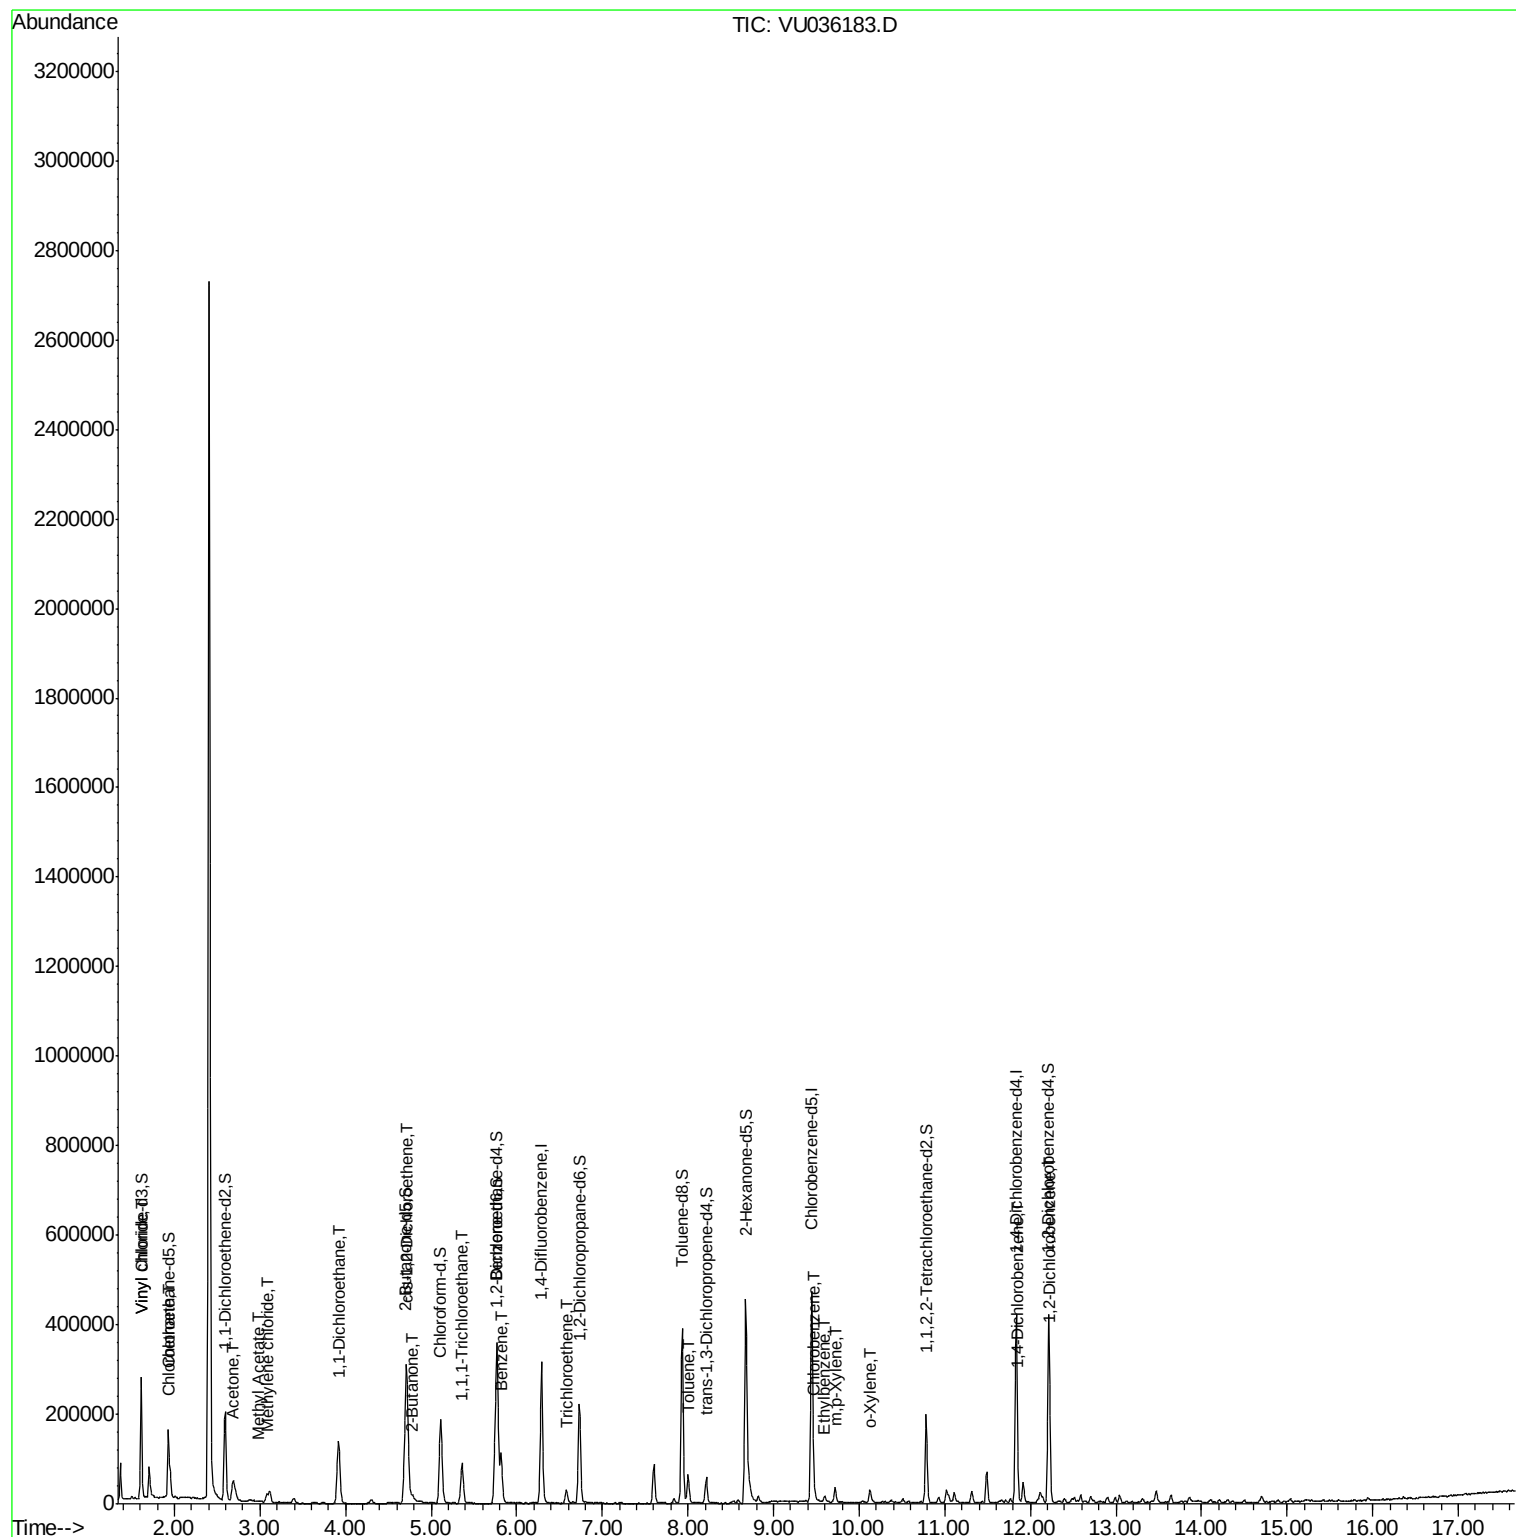

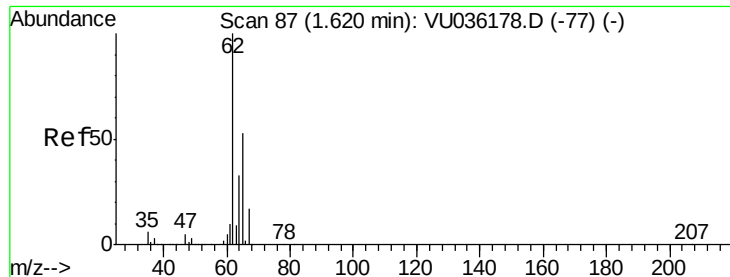

#5

Vinyl chloride

Concen: 2.407 ug/L

RT: 1.62 min Scan# 86

Delta R.T. -0.00 min

Lab File: VU036183.D

Acq: 13 Dec 2019 05:41

Instrument :

MSVOA_U

ClientSampled :

BFQW2

Tot Ion: 62 Resp: 81648

Ion Ratio Lower Upper

62 100


64 32.4 24.0 44.6

Manual Integrations

APPROVED




apatel

12/13/2019 3:58:52 PM

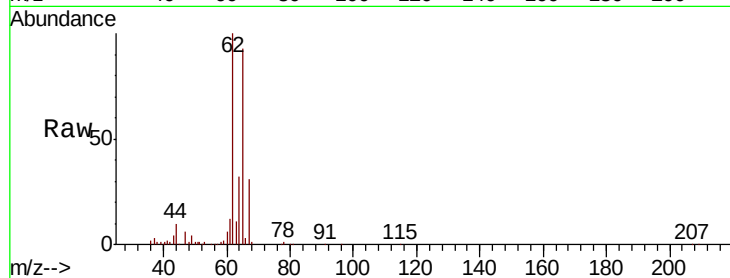

Abundance Ion 62.00 (61.70 to 62.70): VU036183.D (-1) (-)

Ion 64.10 (63.80 to 64.80): VU036183.D (-1) (-)

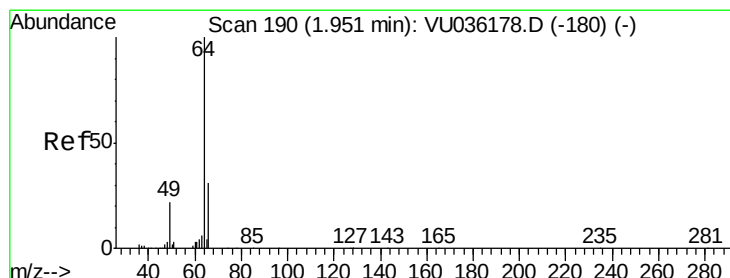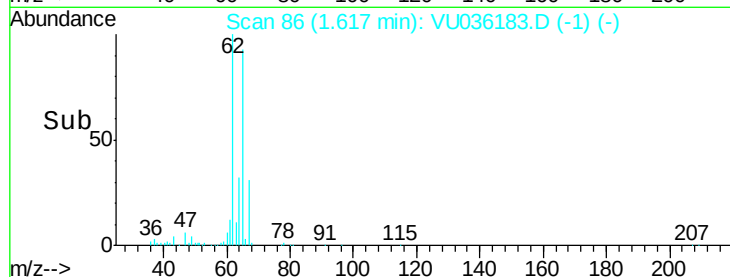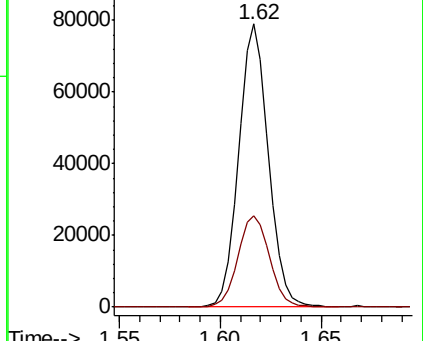

#8

Chloroethane

Concen: 1.632 ug/L

RT: 1.95 min Scan# 190

Delta R.T. -0.00 min

Lab File: VU036183.D


Acq: 13 Dec 2019 05:41

Tgt Ion: 64 Resp: 34087

Ion Ratio Lower Upper



64 100


66 30.2 22.0 41.0

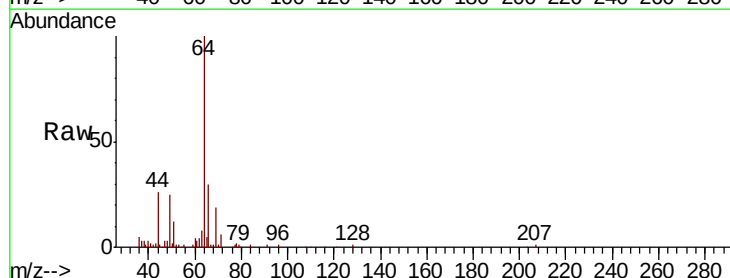

Abundance Ion 64.10 (63.80 to 64.80): VU036183.D (-97) (-)

Ion 66.05 (65.75 to 66.75): VU036183.D (-97) (-)

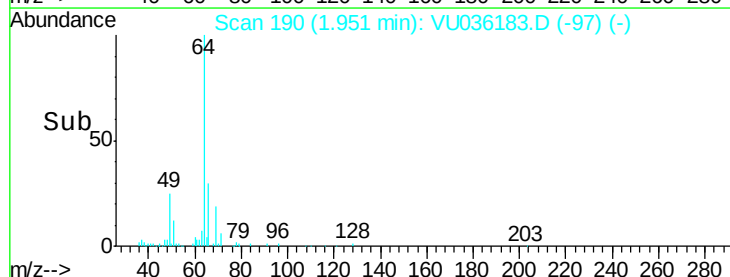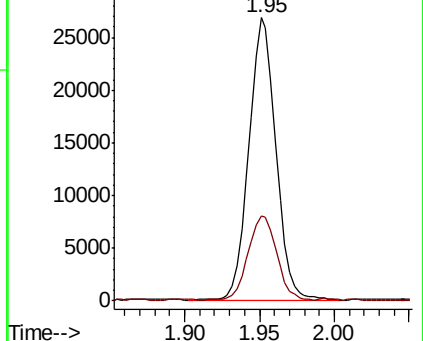

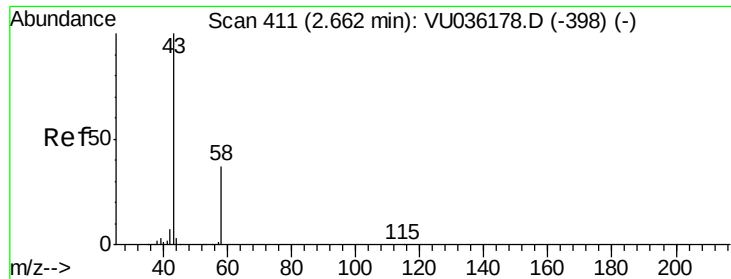





#13
Acetone
Concen: 22.801 ug/L
RT: 2.68 min Scan# 418
Delta R.T. 0.02 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Instrument :
MSVOA_U
ClientSampleId :
BFQW2

Tot Ion: 43 Resp: 82030
Ion Ratio Lower Upper
43 100
58 34.6 0.0 70.0




Manual Integrations
APPROVED


apatel
12/13/2019 3:58:52 PM

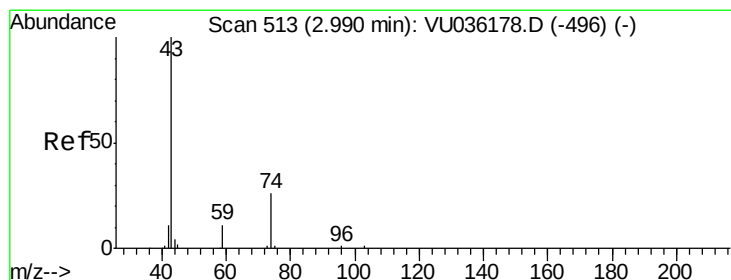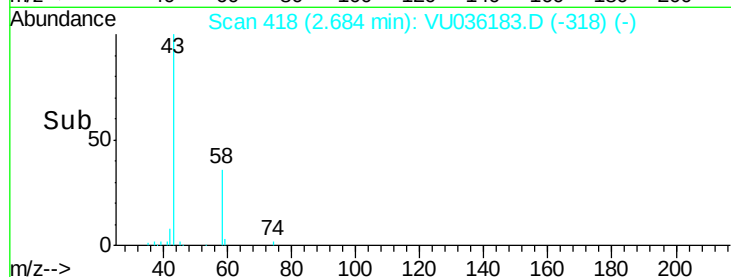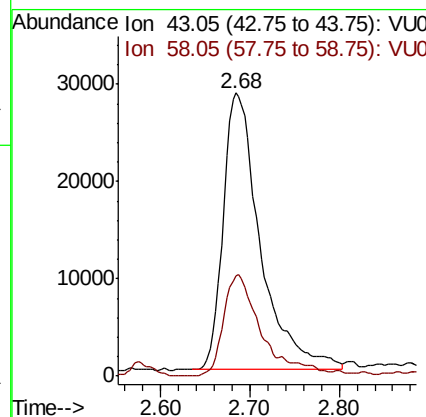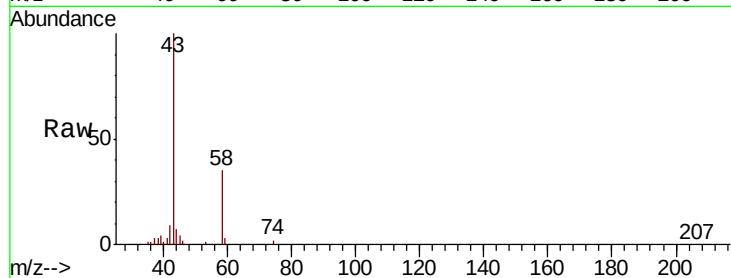

#15
Methyl Acetate
Concen: 0.412 ug/L m
RT: 2.99 min Scan# 513
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Tgt Ion: 43 Resp: 3157
Ion Ratio Lower Upper
43 100
74 23.3 20.6 30.8

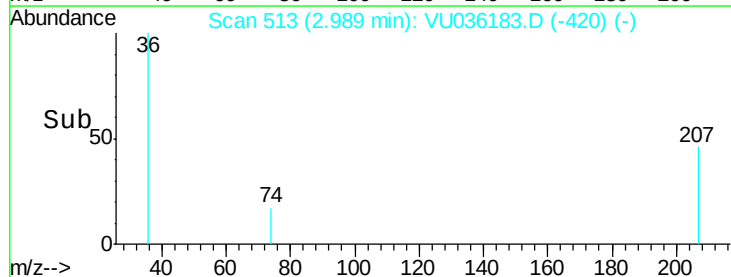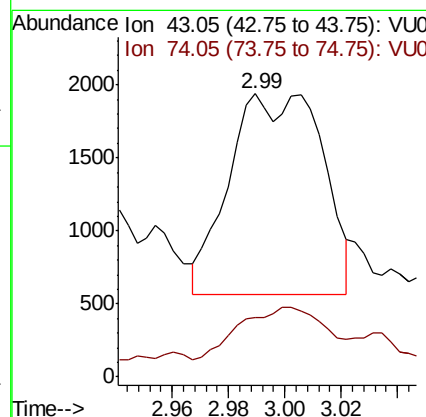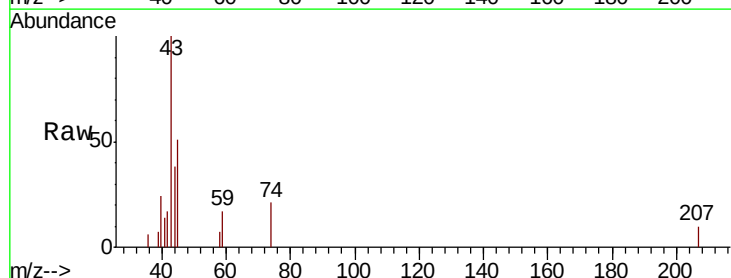

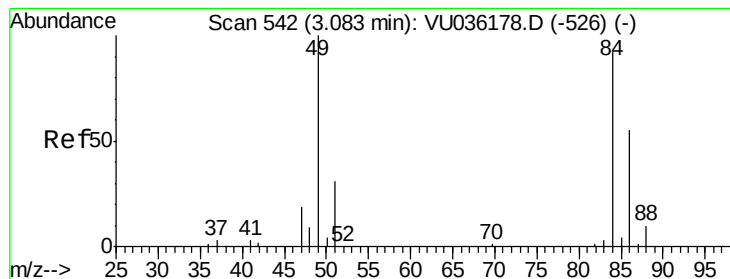

#16

Methylene chloride

Concen: 0.274 ug/L

RT: 3.09 min Scan# 543

Delta R.T. 0.00 min

Lab File: VU036183.D

Acq: 13 Dec 2019 05:41

Instrument :

MSVOA_U





ClientSampled :

BFQW2

Tot Ion:	84	Resp:	7336
Ion	Ratio	Lower	Upper
84	100		
86	68.3	46.1	85.5
49	102.7	77.7	144.3

Manual Integrations
APPROVED

apatel
12/13/2019 3:58:52 PM

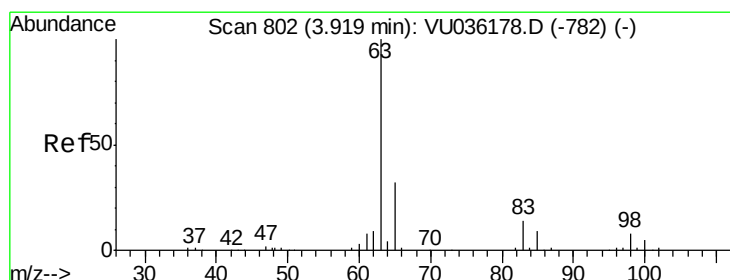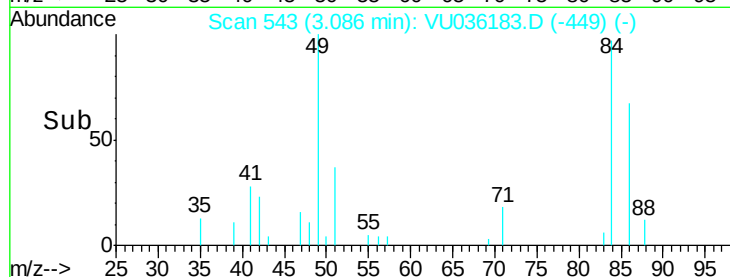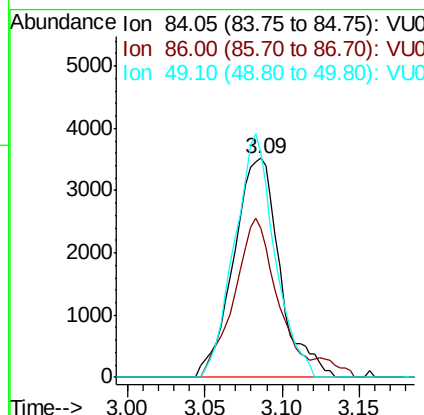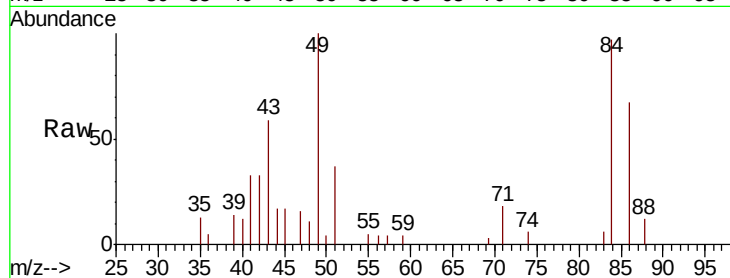

#19

1,1-Dichloroethane

Concen: 4.454 ug/L




RT: 3.92 min Scan# 802


Delta R.T. -0.00 min

Lab File: VU036183.D

Acq: 13 Dec 2019 05:41

Tgt Ion:	63	Resp:	162686
Ion	Ratio	Lower	Upper
63	100		
65	31.8	22.2	41.2
83	13.2	9.8	18.2

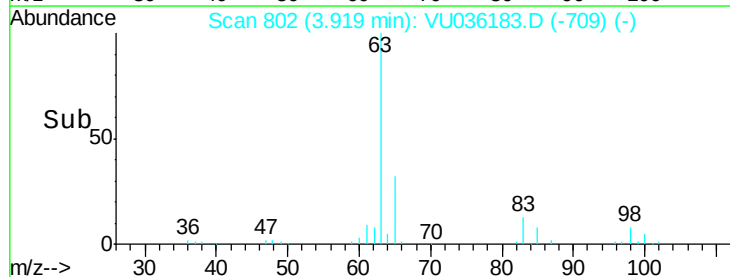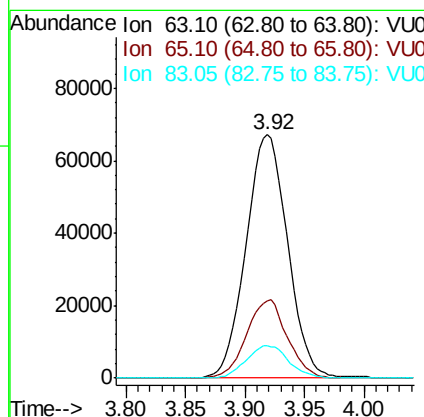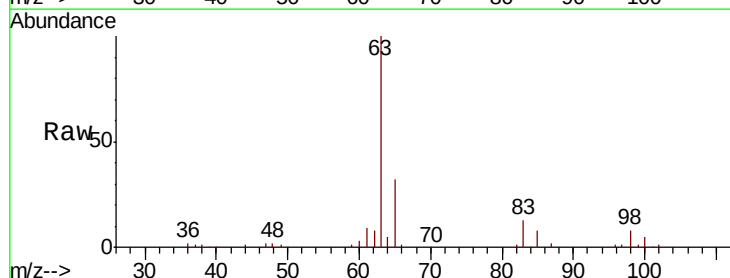

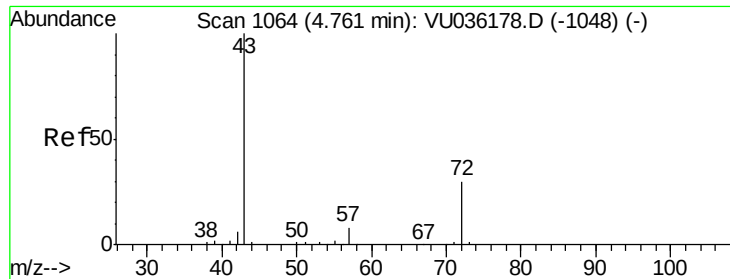

#21

2-Butanone

Concen: 1.999 ug/L

RT: 4.78 min Scan# 1070

Delta R.T. 0.02 min

Lab File: VU036183.D

Acq: 13 Dec 2019 05:41

Instrument :

MSVOA_U

ClientSampled :

BFQW2

Tot Ion: 43 Resp: 9586

Ion Ratio Lower Upper

43 100


72 35.1 14.4 43.2

Manual Integrations




APPROVED

apatel

12/13/2019 3:58:52 PM

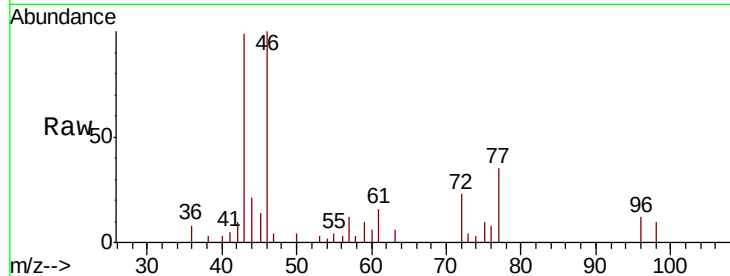

Abundance Ion 43.05 (42.75 to 43.75): VU036183.D (-971) (-)

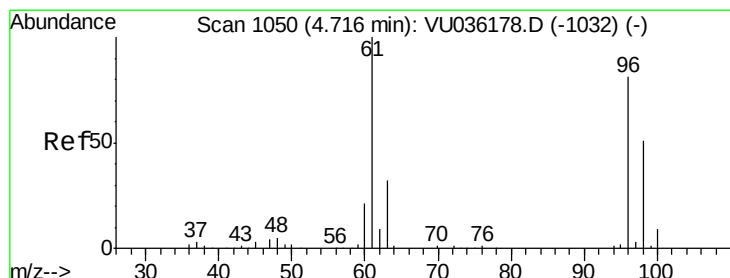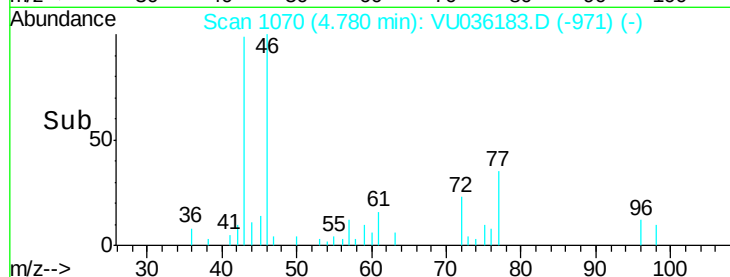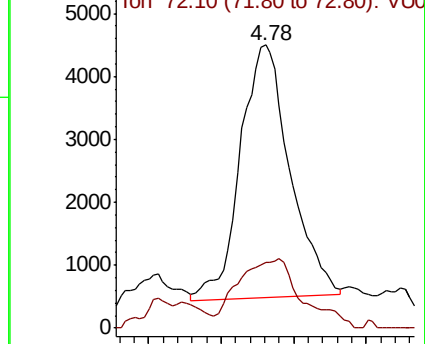

#22

cis-1,2-Dichloroethene

Concen: 5.697 ug/L

RT: 4.72 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VU036183.D

Acq: 13 Dec 2019 05:41


Tgt Ion: 96 Resp: 116448

Ion Ratio Lower Upper



96 100


61 125.3 83.8 155.6

68 0.0 0.0 0.0

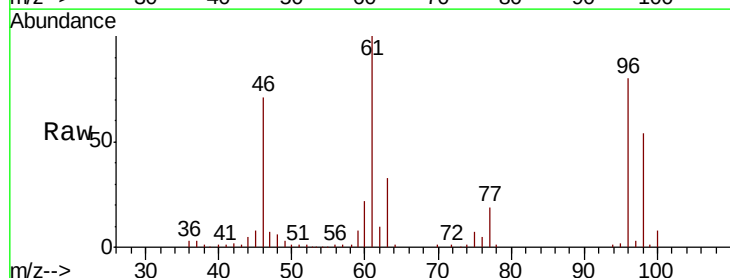

Abundance Ion 96.00 (95.70 to 96.70): VU036183.D (-957) (-)

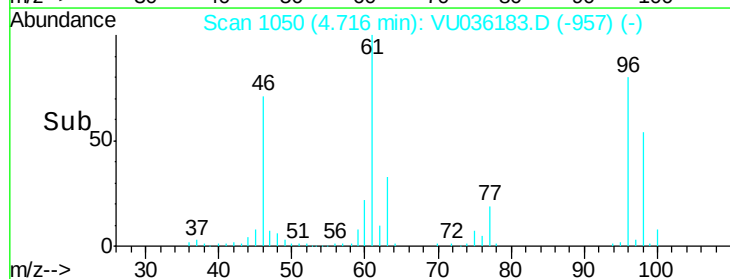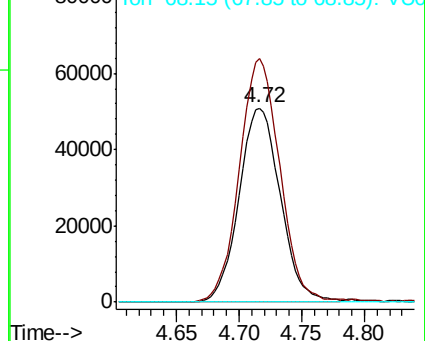

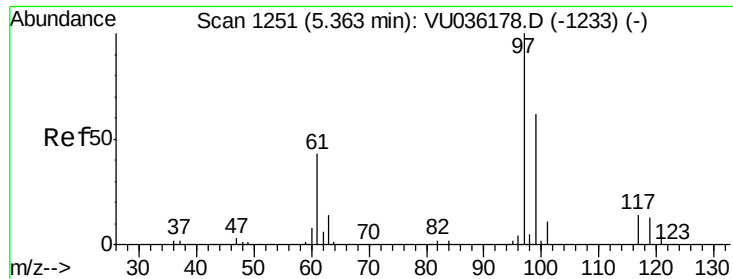


#29
1,1,1-Trichloroethane
Concen: 1.810 ug/L
RT: 5.36 min Scan# 1251
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Instrument :
MSVOA_U
ClientSampleId :
BFQW2




Tot Ion	Ratio	Lower	Upper
97	100		
99	63.9	52.6	79.0
61	45.2	35.4	53.2

Manual Integrations
APPROVED

apatel
12/13/2019 3:58:52 PM

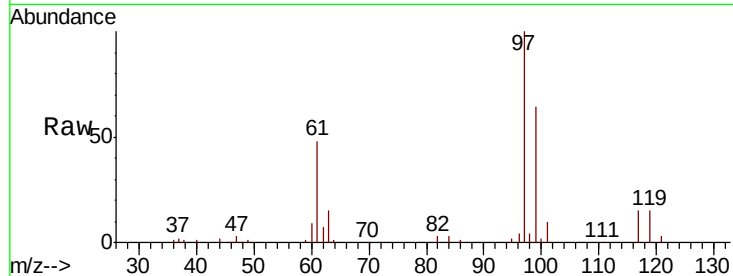


Abundance Ion 96.95 (96.65 to 97.65): VU0
Ion 99.05 (98.75 to 99.75): VU0
Ion 61.05 (60.75 to 61.75): VU0

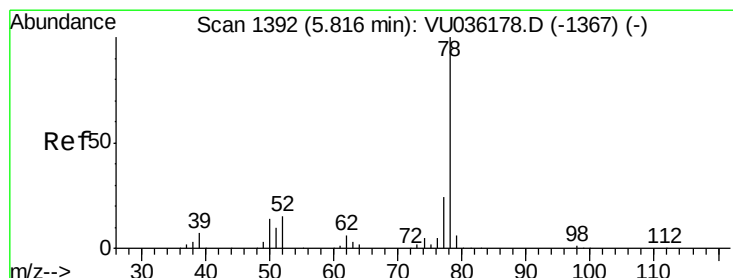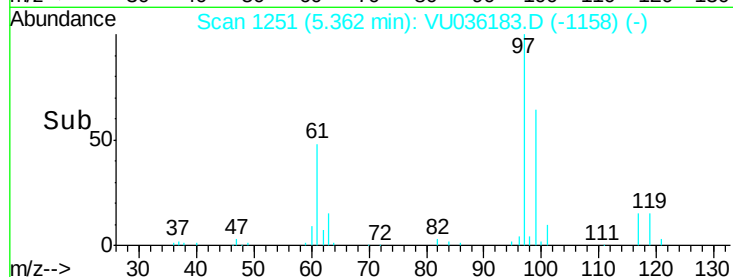
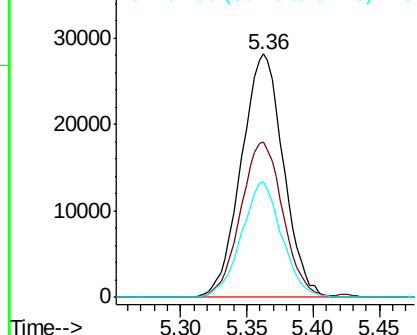



#33
Benzene
Concen: 1.219 ug/L
RT: 5.82 min Scan# 1392
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Tgt Ion: 78 Resp: 105475

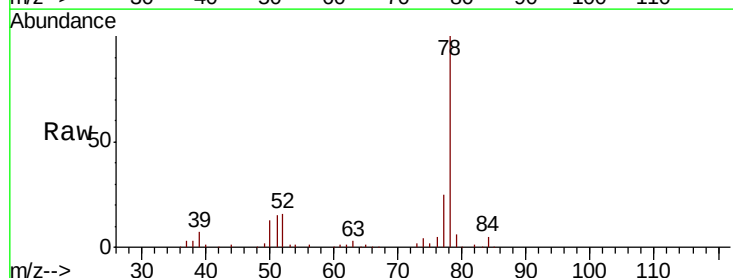

Abundance Ion 78.10 (77.80 to 78.80): VU0

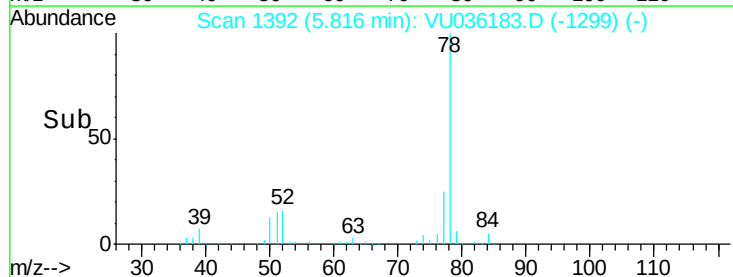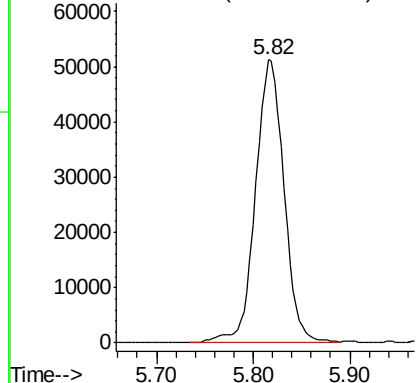

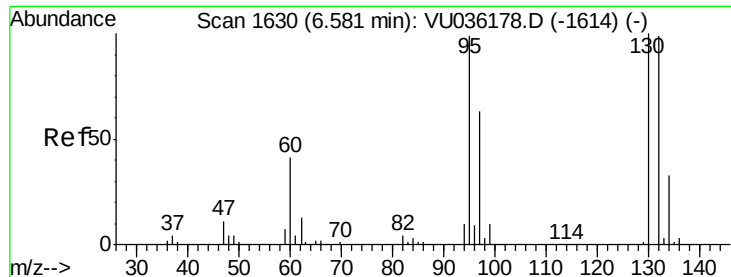


#34
 Trichloroethene
 Concen: 0.460 ug/L
 RT: 6.58 min Scan# 1630
 Delta R.T. -0.00 min
 Lab File: VU036183.D
 Acq: 13 Dec 2019 05:41

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW2

Tot Ion	Ion	Ratio	Lower	Upper
95	100			
97	57.6	43.7	81.1	
132	96.2	71.7	133.3	
130	96.1	73.1	135.7	

Manual Integrations
 APPROVED

apatel
 12/13/2019 3:58:52 PM



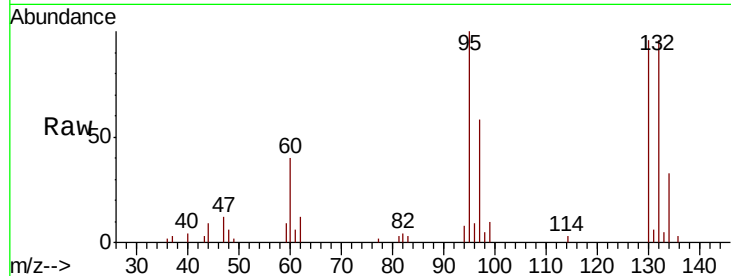


Abundance Ion 95.00 (94.70 to 95.70): VU036183.D (-1537) (-)

Ion 96.95 (96.65 to 97.65): VU036183.D (-1537) (-)


Ion 131.95 (131.65 to 132.65): VU036183.D (-1537) (-)

Ion 129.95 (129.65 to 130.65): VU036183.D (-1537) (-)

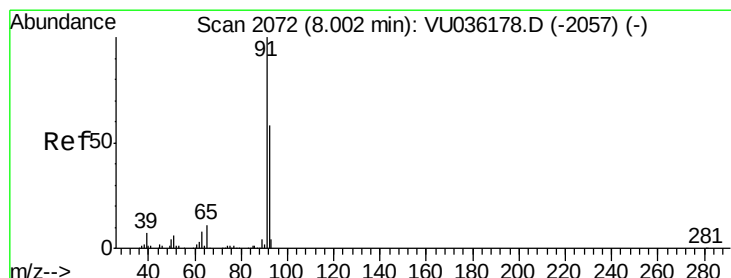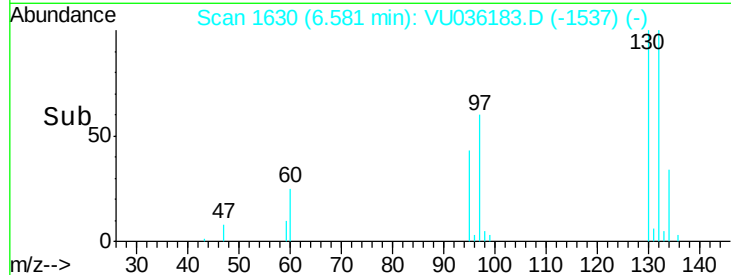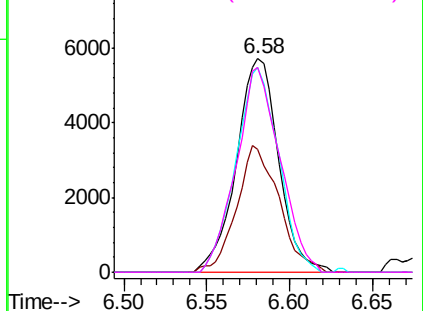



#42
 Toluene
 Concen: 0.498 ug/L
 RT: 8.00 min Scan# 2072
 Delta R.T. -0.00 min
 Lab File: VU036183.D
 Acq: 13 Dec 2019 05:41


Tgt Ion	Ion	Ratio	Lower	Upper
91	100			
92	54.9	40.7	75.7	

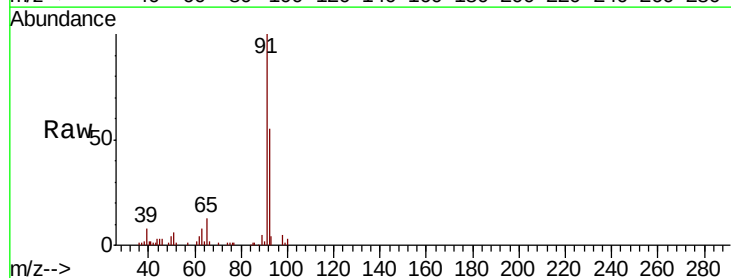

Abundance Ion 91.15 (90.85 to 91.85): VU036183.D (-1979) (-)

Ion 92.15 (91.85 to 92.85): VU036183.D (-1979) (-)

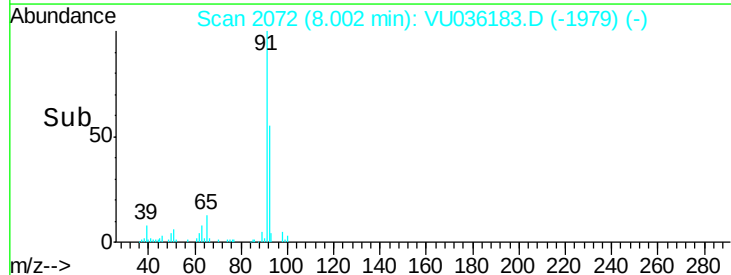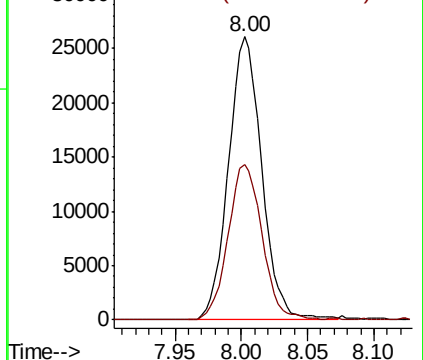

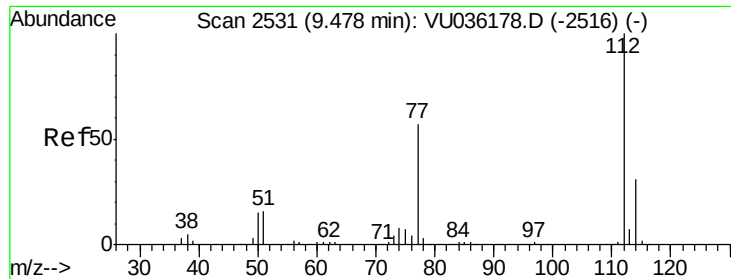


#51
Chlorobenzene
Concen: 0.169 ug/L
RT: 9.48 min Scan# 2531
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Instrument :
MSVOA_U
ClientSampled :
BFQW2




Tot Ion	Ratio	Lower	Upper
112	100		
114	28.5	22.2	41.2
77	48.1	45.7	68.5

Manual Integrations
APPROVED

apatel
12/13/2019 3:58:52 PM

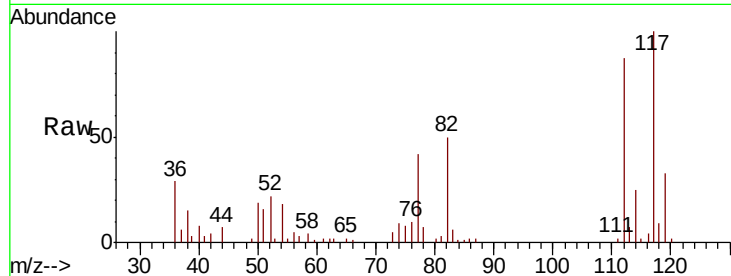


Abundance Ion 112.10 (111.80 to 112.80): V
Ion 114.05 (113.75 to 114.75): V
Ion 77.10 (76.80 to 77.80): V

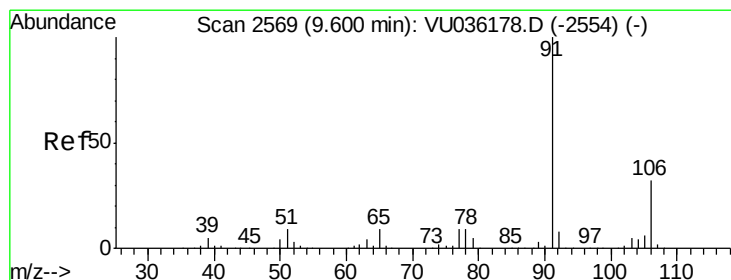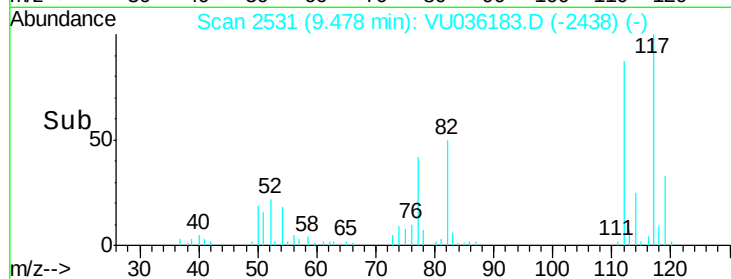
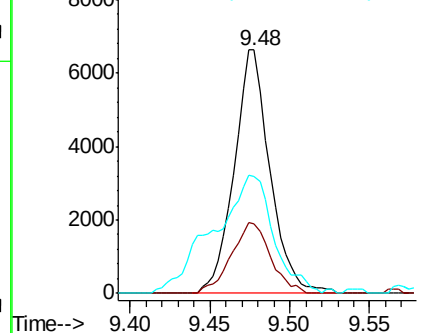



#52
Ethylbenzene
Concen: 0.103 ug/L
RT: 9.60 min Scan# 2568
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Tgt Ion	Ratio	Lower	Upper
91	100		
106	28.7	21.6	40.2

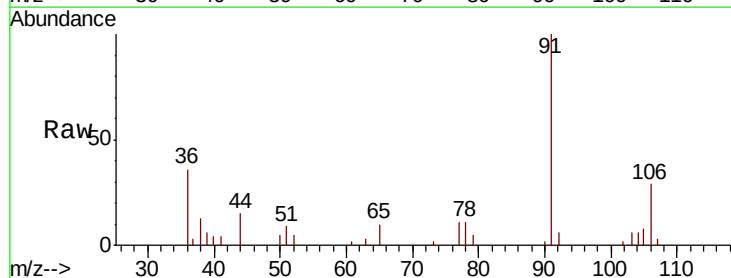

Abundance Ion 91.15 (90.85 to 91.85): V
Ion 106.15 (105.85 to 106.85): V

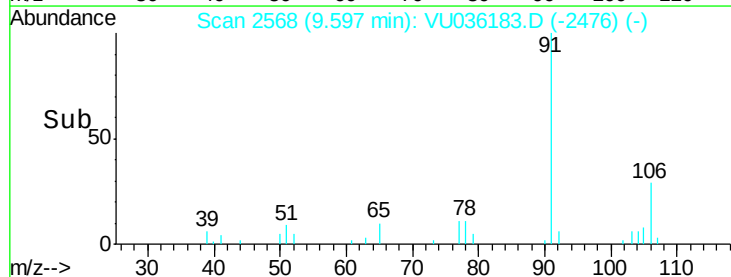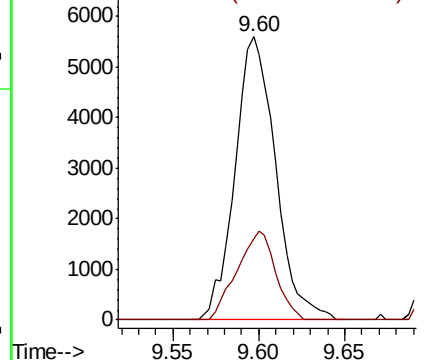

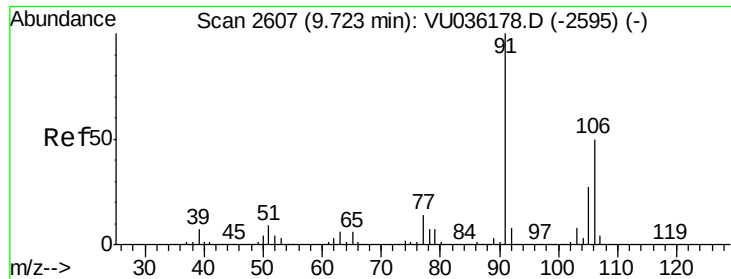

#53

m,p-Xylene

Concen: 0.287 ug/L

RT: 9.72 min Scan# 2606

Delta R.T. -0.00 min

Lab File: VU036183.D

Acq: 13 Dec 2019 05:41

Instrument :

MSVOA_U

ClientSampleId :

BFQW2

Tot Ion:106 Resp: 10039

Ion Ratio Lower Upper

106 100


91 173.1 140.4 260.8

Manual Integrations

APPROVED




apatel

12/13/2019 3:58:52 PM

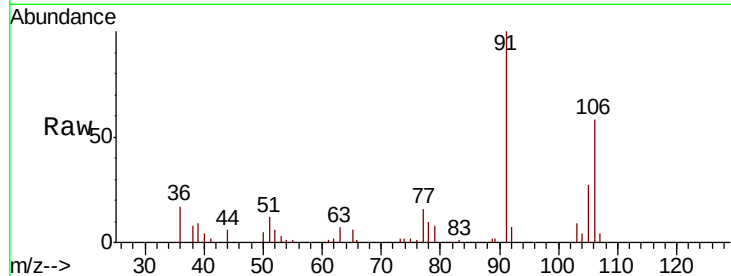

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

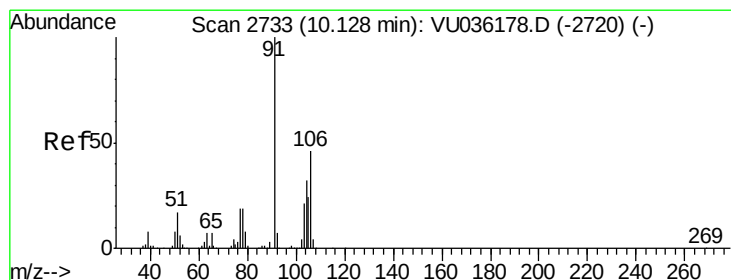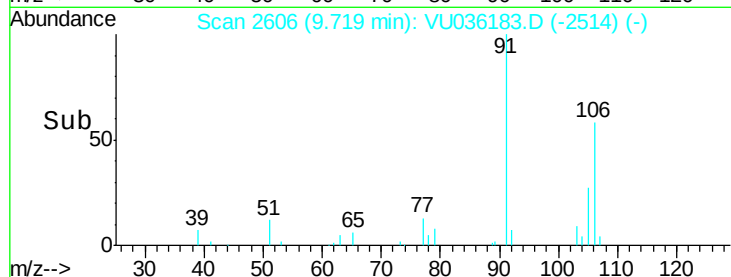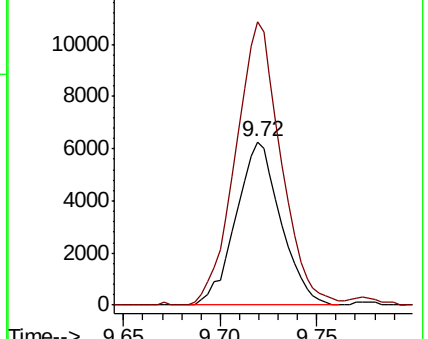

#54

o-Xylene

Concen: 0.207 ug/L

RT: 10.13 min Scan# 2733

Delta R.T. -0.00 min

Lab File: VU036183.D


Acq: 13 Dec 2019 05:41

Tgt Ion:106 Resp: 6932

Ion Ratio Lower Upper



106 100


91 209.6 148.5 275.7

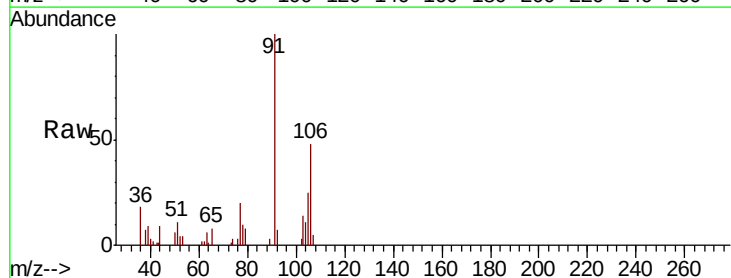

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

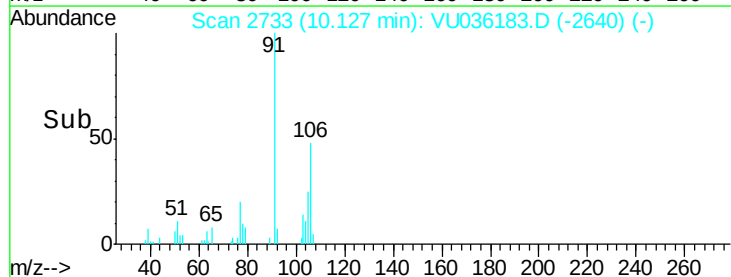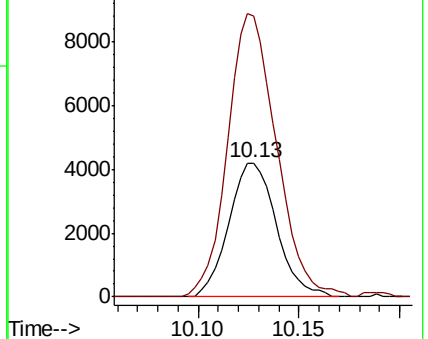

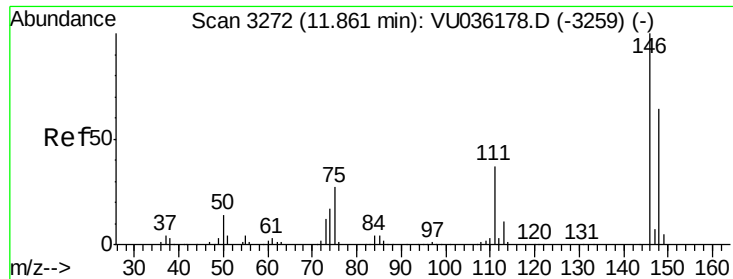





#63
1,4-Dichlorobenzene
Concen: 0.155 ug/L
RT: 11.86 min Scan# 3272
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Instrument :
MSVOA_U
ClientSampleId :
BFQW2

Tot Ion	Ratio	Lower	Upper
146	100		
111	42.7	27.5	51.1
148	65.5	45.4	84.2

Manual Integrations
APPROVED

apatel
12/13/2019 3:58:52 PM

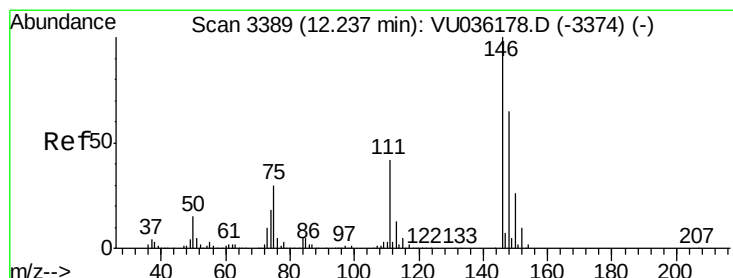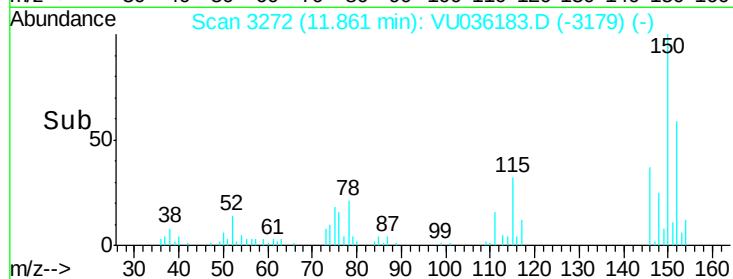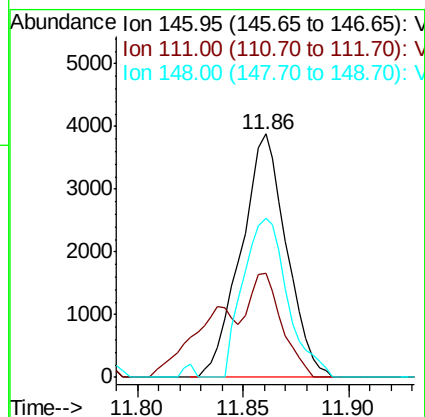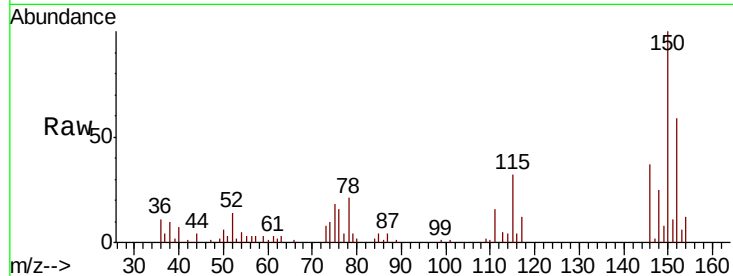

#65
1,2-Dichlorobenzene
Concen: 0.200 ug/L
RT: 12.24 min Scan# 3389
Delta R.T. -0.00 min
Lab File: VU036183.D
Acq: 13 Dec 2019 05:41

Tgt Ion	Ratio	Lower	Upper
146	100		
111	49.4	33.3	49.9
148	80.2	52.2	78.2#

