


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121219\
Data File : VU036147.D
Acq On : 12 Dec 2019 09:34
Operator : JC/MD
Sample : BFB17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB17

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Dec 13 04:38:02 2019

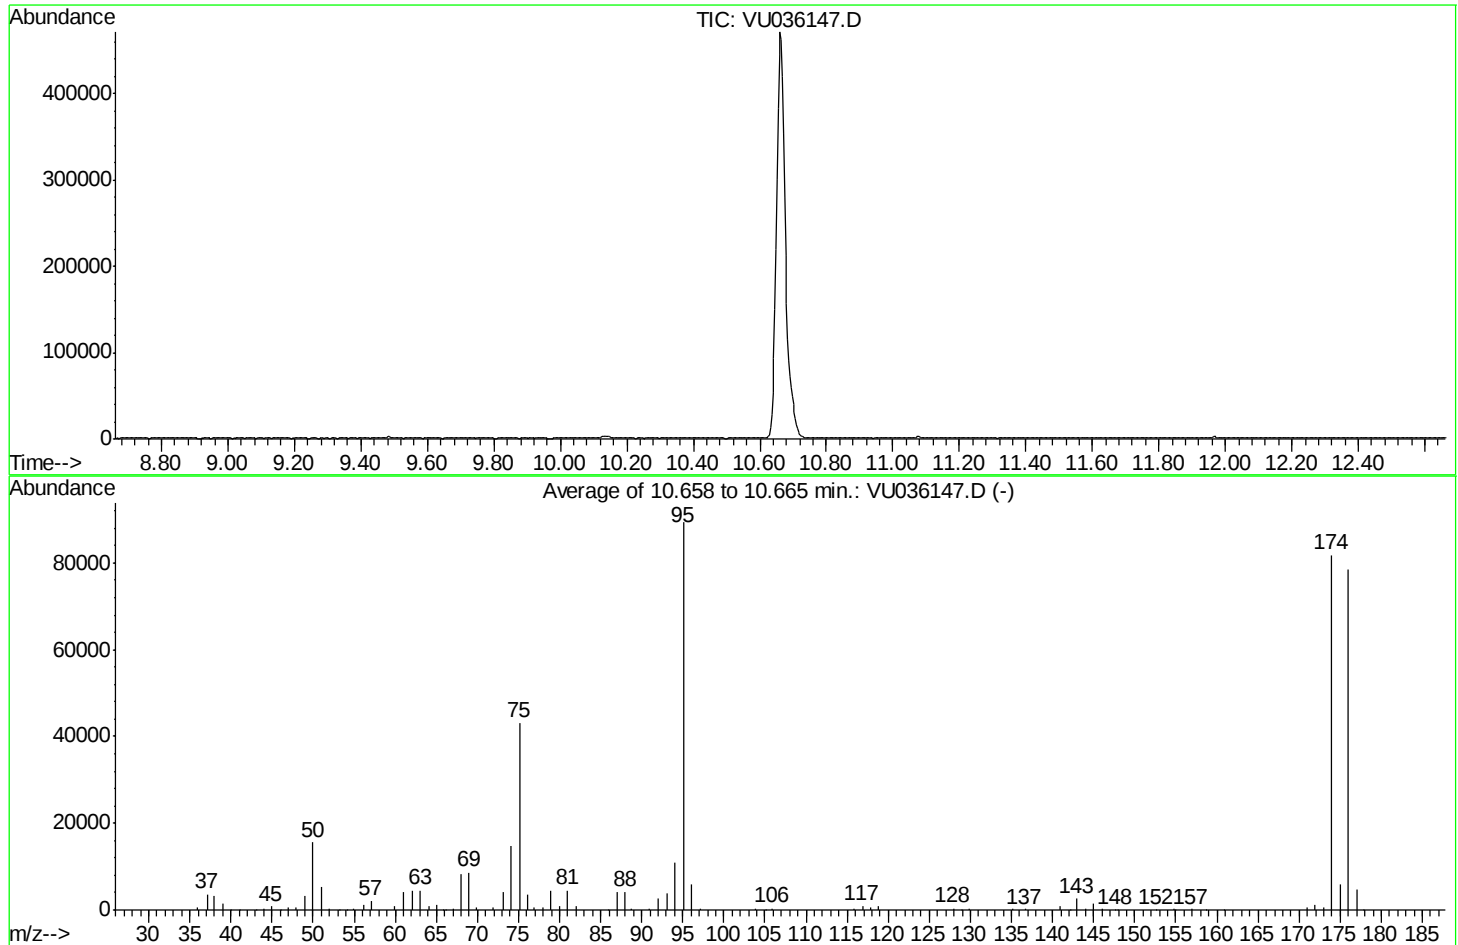

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	15633	PASS
75	95	30	80	48.2	43109	PASS
95	95	100	100	100.0	89360	PASS
96	95	5	9	6.6	5898	PASS
173	174	0.00	2	0.7	595	PASS
174	95	50	120	91.5	81773	PASS
175	174	5	9	7.2	5870	PASS
176	174	95	101	95.8	78378	PASS
177	176	5	9	6.1	4796	PASS

m/z	Abundance
36.00	587.0
37.10	3654.0
38.00	3261.0
39.10	1339.0
39.90	308.0
41.10	144.0
43.10	118.0
44.10	906.0
45.00	851.0
46.00	139.0
47.00	725.0
47.90	545.0
49.10	3336.0
50.00	15151.0
51.10	5372.0
51.90	296.0
53.10	102.0
54.10	140.0
54.90	289.0
56.20	1057.0
57.00	1932.0
59.90	934.0
61.10	4008.0
62.10	4230.0
63.10	4422.0
64.10	894.0
65.10	1021.0
65.80	156.0
67.00	365.0
68.00	8035.0
69.00	8846.0
70.00	555.0
71.90	559.0
73.10	4048.0
74.00	14422.0
75.10	42096.0
76.10	3670.0
77.00	598.0
78.10	468.0
78.90	4478.0
80.00	1027.0
80.90	4433.0
81.90	858.0
85.80	172.0
87.00	3920.0
88.00	4264.0
88.80	282.0
90.90	389.0
91.90	2461.0
93.10	3627.0
94.00	10243.0
95.10	86912.0
96.00	5580.0
97.20	200.0
103.90	440.0
105.00	114.0
105.80	395.0
115.90	254.0
116.90	857.0
117.90	490.0
118.80	946.0
127.90	360.0
129.80	411.0
135.10	157.0
136.70	212.0
140.90	861.0
142.10	153.0
142.90	2479.0
143.90	176.0
144.90	1456.0
146.00	240.0
147.90	125.0
154.70	286.0
157.00	296.0
160.90	106.0
170.90	519.0
171.90	1185.0
173.00	1785.0
173.90	76896.0
175.00	5826.0
176.00	74448.0
177.00	4694.0
177.80	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
36.00	690.0
37.10	3739.0
38.00	3382.0
39.10	1462.0
39.90	397.0
41.10	110.0
43.10	105.0
44.10	1015.0
45.00	836.0
47.00	641.0
48.00	568.0
49.10	3372.0
50.00	16108.0
51.10	5425.0
51.90	326.0
53.20	116.0
54.10	141.0
54.90	281.0
56.10	1200.0
57.10	2147.0
60.00	908.0
61.00	4133.0
62.10	4498.0
63.00	4644.0
64.00	863.0
65.10	1152.0
65.80	121.0
67.00	365.0
68.00	8487.0
69.00	8768.0
69.90	565.0
71.90	536.0
73.10	4352.0
74.10	15124.0
75.10	44496.0
76.10	3809.0
76.90	714.0
78.00	465.0
78.90	4652.0
80.00	1027.0
81.00	4640.0
81.90	1021.0
85.90	116.0
87.00	4148.0
88.00	4331.0
88.80	243.0
90.90	434.0
92.00	2575.0
93.10	4008.0
94.00	11075.0
95.10	91688.0
96.00	5969.0
97.20	178.0
103.80	390.0
105.00	165.0
105.90	432.0
115.90	312.0
116.80	1022.0
117.90	476.0
118.80	957.0
127.90	370.0
128.90	130.0
129.80	354.0
135.10	203.0
136.70	200.0
140.90	823.0
142.90	2749.0
144.00	205.0
144.90	1340.0
146.00	220.0
147.60	179.0
154.80	298.0
157.00	264.0
158.70	106.0
160.90	106.0
170.90	575.0
171.90	1300.0
174.00	84104.0
175.00	6043.0
176.00	80560.0
177.00	4879.0
177.80	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
35.90	734.0
37.10	3631.0
38.00	3364.0
39.00	1552.0
39.90	441.0
44.00	1113.0
44.90	654.0
47.00	736.0
48.00	586.0
49.00	3269.0
50.00	15640.0
51.10	4784.0
51.90	246.0
53.20	141.0
54.10	143.0
54.90	206.0
56.10	1169.0
57.10	2265.0
60.00	913.0
61.00	3956.0
62.10	4395.0
63.00	4617.0
64.00	877.0
65.10	1167.0
66.10	119.0
67.00	255.0
68.00	8276.0
69.00	8161.0
69.90	626.0
72.00	464.0
73.10	4158.0
74.10	14426.0
75.10	42736.0
76.10	3479.0
76.90	757.0
77.90	566.0
78.90	4440.0
80.00	991.0
81.00	4475.0
82.00	1213.0
87.00	4151.0
88.00	3872.0
90.90	441.0
92.00	2595.0
93.10	4178.0
94.10	11143.0
95.00	89480.0
96.00	6146.0
97.20	116.0
103.90	317.0
105.10	186.0
106.00	437.0
115.90	367.0
116.80	1086.0
117.90	403.0
118.90	909.0
128.00	383.0
128.90	122.0
129.80	252.0
135.10	215.0
136.70	174.0
140.90	751.0
143.00	2542.0
144.00	226.0
145.00	1232.0
146.00	174.0
147.70	172.0
152.60	103.0
155.00	328.0
156.90	243.0
170.90	624.0
171.90	1297.0
174.00	84320.0
175.00	5743.0
175.90	80128.0
177.00	4816.0
177.80	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

Scan 2884 (10.613 min): VU036147.D
BFB17

m/z	Abundance
40.00	341.0
44.00	740.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17