

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U121220\
 Data File : VU041581.D
 Acq On : 12 Dec 2020 21:20
 Operator : SY/MD
 Sample : L4995-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AS2

Quant Time: Dec 13 11:27:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Dec 13 11:26:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	152273	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	147548	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	68627	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	37544	3.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.00%
7) Chloroethane-d5	1.92	69	35837	3.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.80%
11) 1,1-Dichloroethene-d2	2.58	63	60892	2.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.60%#
20) 2-Butanone-d5	4.65	46	174442	51.01	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.02%
24) Chloroform-d	5.08	84	87097	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.40%
26) 1,2-Dichloroethane-d4	5.72	65	50942	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
32) Benzene-d6	5.74	84	178168	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.40%
36) 1,2-Dichloropropane-d6	6.70	67	57153	4.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.20%
41) Toluene-d8	7.91	98	157366	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.60%
43) trans-1,3-Dichloropropene-	8.19	79	23036	3.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.40%
46) 2-Hexanone-d5	8.64	63	135370	41.57	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.14%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	56089	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	59887	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Chloromethane	1.52	50	950	0.076	ug/L	98
10) 1,1,2-Trichloro-1,2,2-trif	2.58	101	584	0.056	ug/L #	22
13) Acetone	2.67	43	23340	10.730	ug/L	58
15) Methyl Acetate	2.97	43	2503	0.443	ug/L	97
21) 2-Butanone	4.74	43	7855	2.217	ug/L	100
25) Chloroform	5.11	83	1609	0.080	ug/L	98
33) Benzene	5.79	78	2772	0.059	ug/L	100
34) Trichloroethene	6.27	95	2486	0.210	ug/L #	7
35) Methylcyclohexane	6.70	83	12881	0.672	ug/L #	19
37) 1,2-Dichloropropane	6.70	63	5914	0.490	ug/L #	88
39) cis-1,3-Dichloropropene	7.58	75	1389	0.078	ug/L #	77
42) Toluene	7.98	91	12631	0.259	ug/L	97
44) trans-1,3-Dichloropropene	8.18	75	1039	0.065	ug/L	89
52) Ethylbenzene	9.57	91	2800	0.054	ug/L	100
53) m,p-Xylene	9.69	106	3410	0.176	ug/L	100
54) o-Xylene	10.10	106	1373	0.072	ug/L	87
55) Styrene	10.11	104	10816	0.330	ug/L	97

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121220\
Data File : VU041581.D
Acq On : 12 Dec 2020 21:20
Operator : SY/MD
Sample : L4995-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AS2

Quant Time: Dec 13 11:27:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Dec 13 11:26:38 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
59) 1,2,3-Trichloropropane	11.81	75	8794	0.970	ug/L	97
68) 1,2,4-trichlorobenzene	13.83	180	404	0.030	ug/L #	87
69) Naphthalene	14.07	128	1930	0.070	ug/L #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121220\
Data File : VU041581.D
Acq On : 12 Dec 2020 21:20
Operator : SY/MD
Sample : L4995-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AS2

Quant Time: Dec 13 11:27:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Dec 13 11:26:38 2020
Response via : Initial Calibration




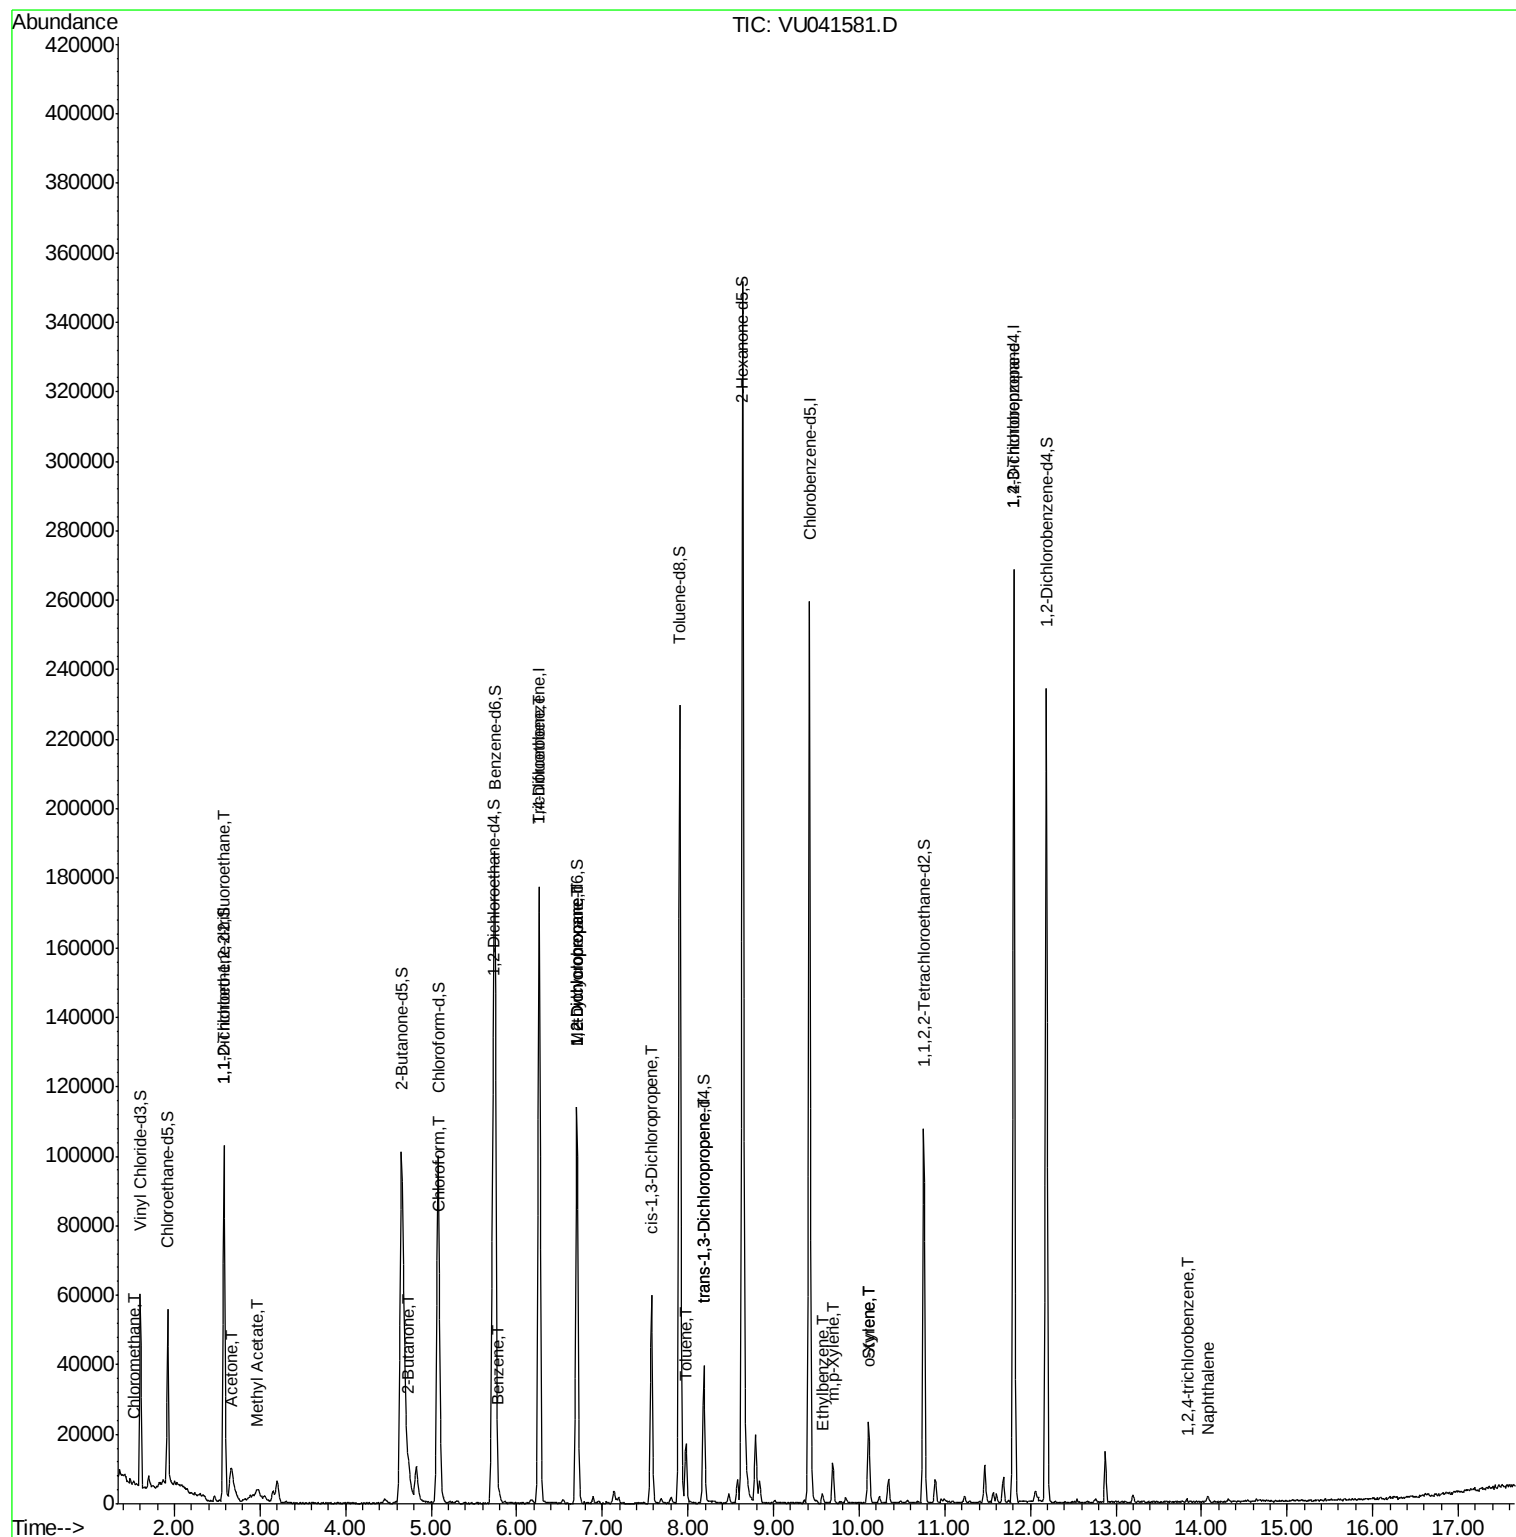


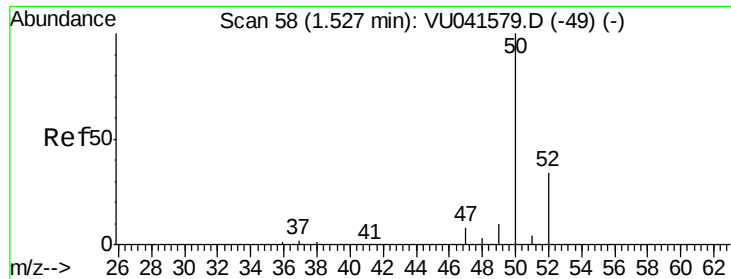

#3
Chloromethane
Concen: 0.076 ug/L
RT: 1.52 min Scan# 57
Delta R.T. -0.00 min
Lab File: VU041581.D
Acq: 12 Dec 2020 21:20




Instrument :
MSVOA_U
ClientSampleId :
C0AS2


Tot Ion: 50 Resp: 950
Ion Ratio Lower Upper
50 100
52 33.6 24.1 44.8

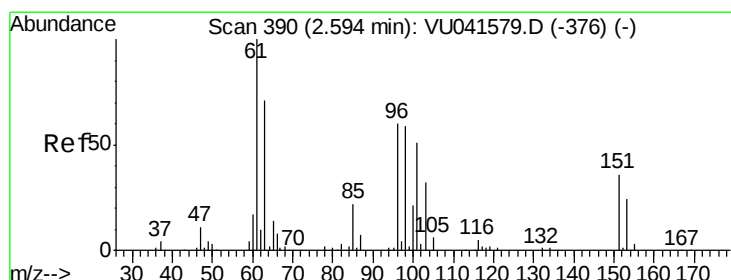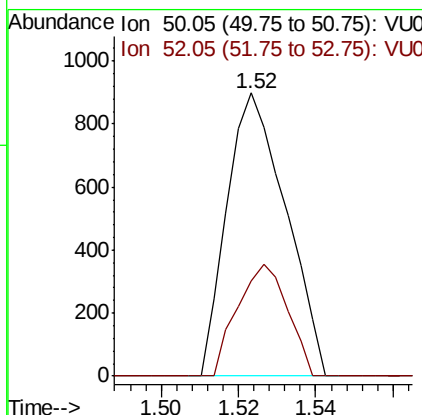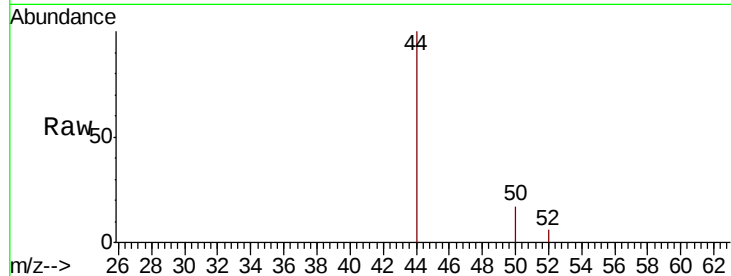

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.056 ug/L
RT: 2.58 min Scan# 385
Delta R.T. -0.02 min
Lab File: VU041581.D
Acq: 12 Dec 2020 21:20

Tgt Ion: 101 Resp: 584
Ion Ratio Lower Upper
101 100
85 0.0 33.6 50.4#
151 0.0 56.2 84.4#

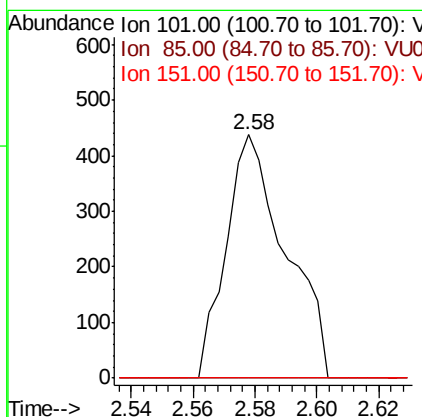

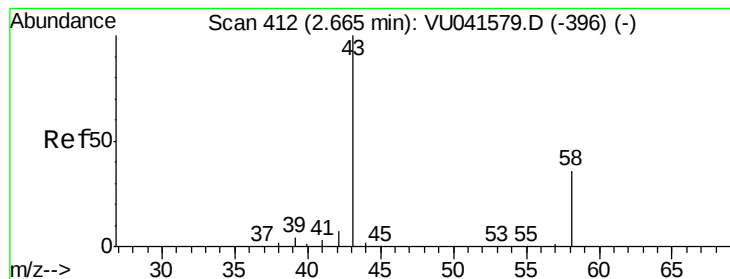

#13

Acetone

Concen: 10.730 ug/L

RT: 2.67 min Scan# 413

Delta R.T. 0.00 min

Lab File: VU041581.D

Acq: 12 Dec 2020 21:20

Instrument :

MSVOA_U

ClientSampleId :


C0AS2

Tot Ion: 43 Resp: 23340

Ion Ratio Lower Upper




43 100

58 11.9 0.0 73.2

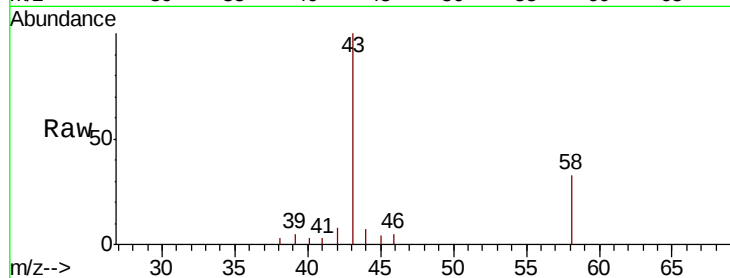

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

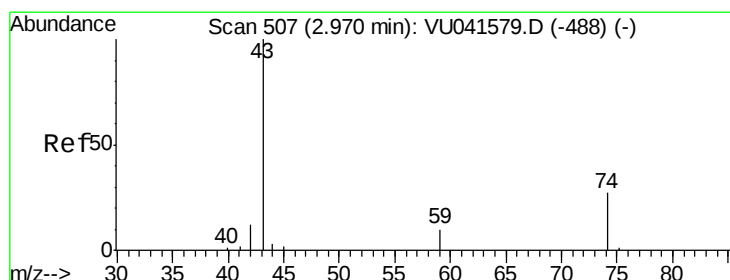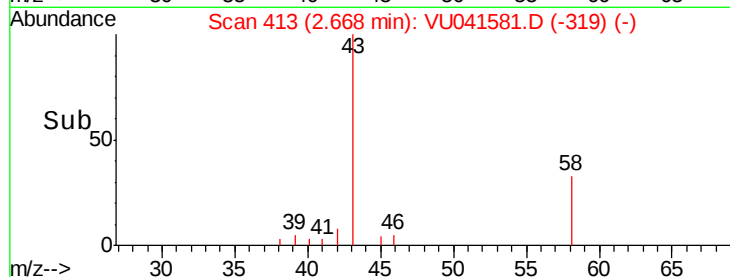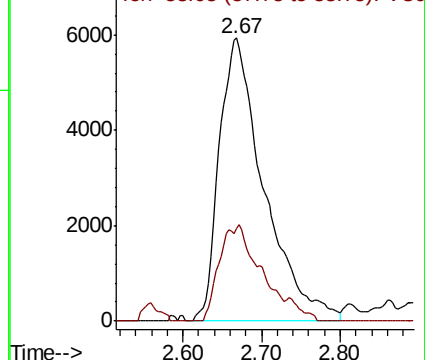

#15

Methyl Acetate

Concen: 0.443 ug/L

RT: 2.97 min Scan# 508

Delta R.T. 0.00 min

Lab File: VU041581.D


Acq: 12 Dec 2020 21:20

Tgt Ion: 43 Resp: 2503

Ion Ratio Lower Upper



43 100


74 25.5 19.2 28.8

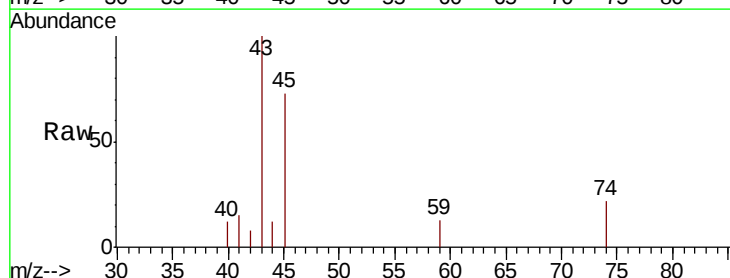

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 74.05 (73.75 to 74.75): VU0



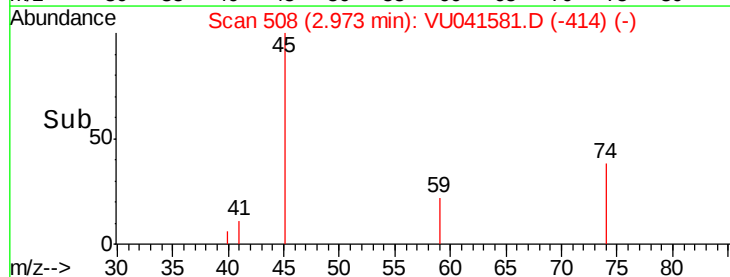
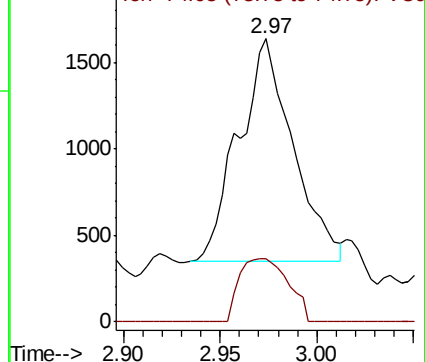


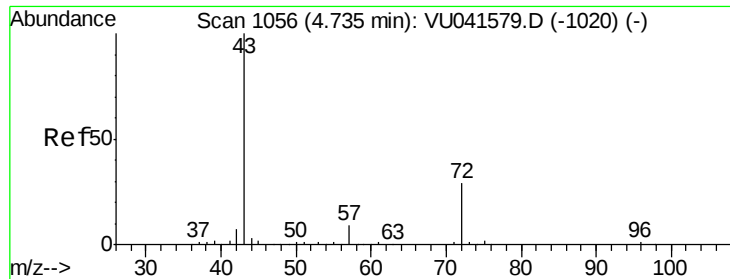

#21
2-Butanone
Concen: 2.217 ug/L
RT: 4.74 min Scan# 1057
Delta R.T. 0.00 min
Lab File: VU041581.D
Acq: 12 Dec 2020 21:20




Instrument :
MSVOA_U
ClientSampleId :
C0AS2


Tot Ion: 43 Resp: 7855
Ion Ratio Lower Upper
43 100
72 29.1 14.6 44.0

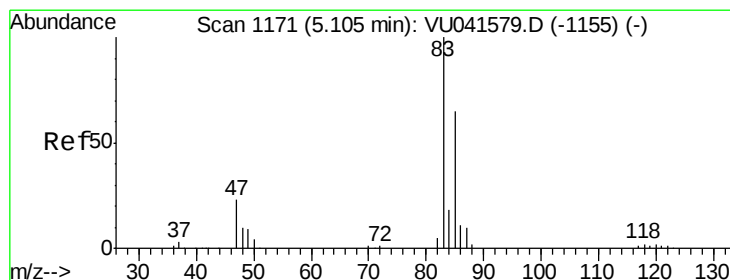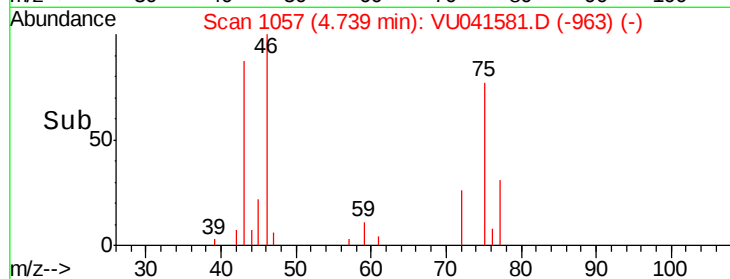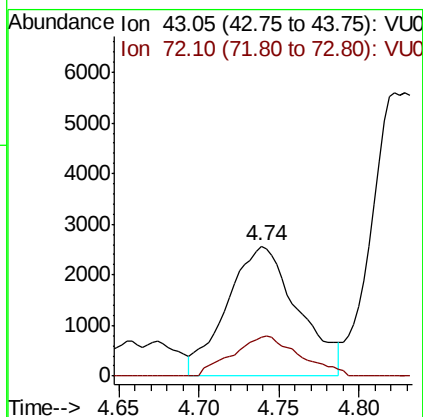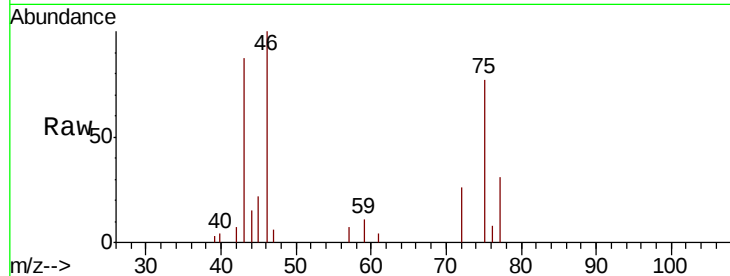

#25
Chloroform
Concen: 0.080 ug/L
RT: 5.11 min Scan# 1171
Delta R.T. -0.00 min
Lab File: VU041581.D
Acq: 12 Dec 2020 21:20

Tgt Ion: 83 Resp: 1609
Ion Ratio Lower Upper
83 100
85 61.6 44.2 82.0

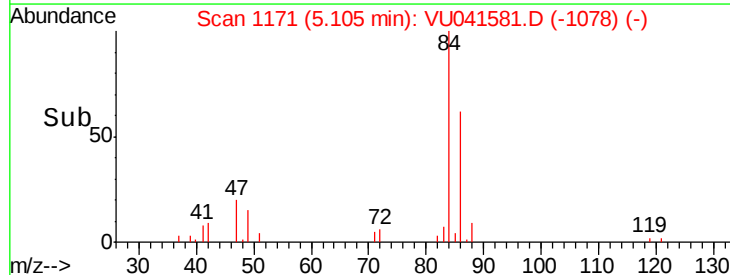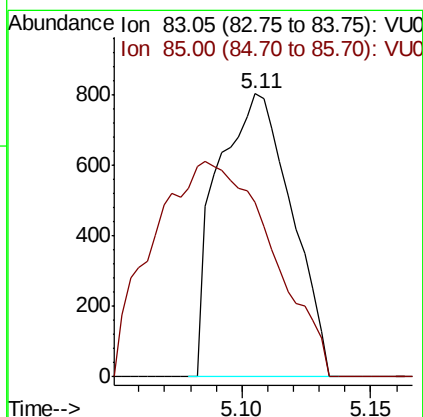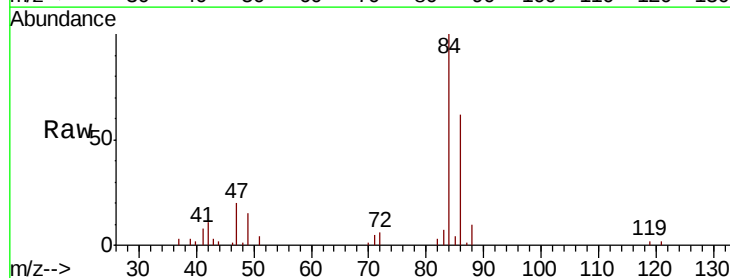

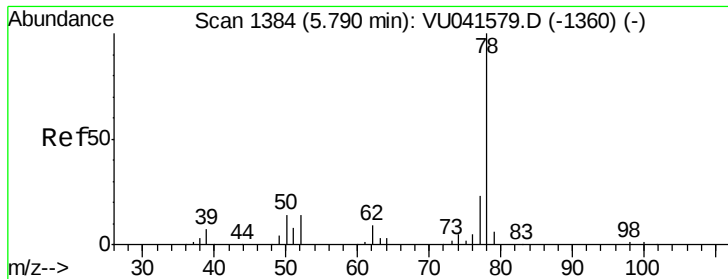

#33

Benzene

Concen: 0.059 ug/L

RT: 5.79 min Scan# 1383

Delta R.T. -0.00 min

Lab File: VU041581.D

Acq: 12 Dec 2020 21:20


Instrument :

MSVOA_U




ClientSampleId :

C0AS2

Tgt Ion: 78 Resp: 2772

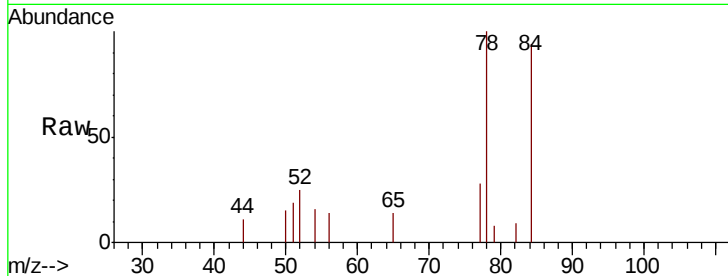

Abundance Ion 78.10 (77.80 to 78.80): VU0

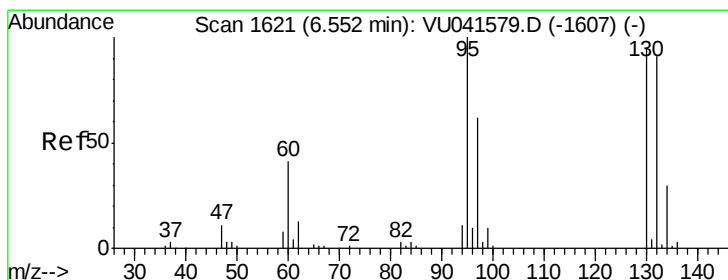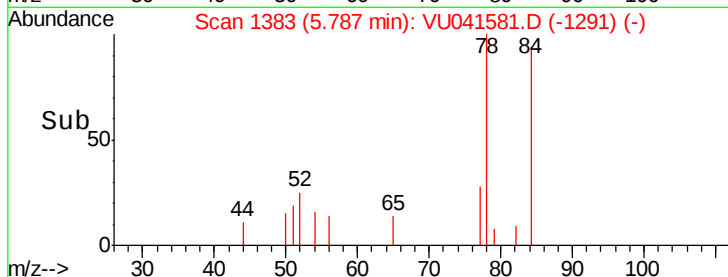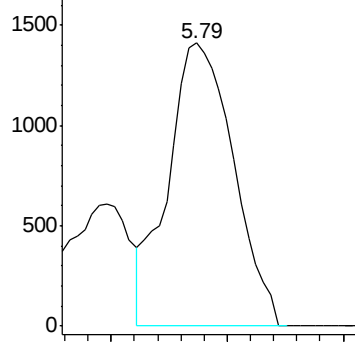

#34

Trichloroethene

Concen: 0.210 ug/L

RT: 6.27 min Scan# 1532

Delta R.T. -0.29 min

Lab File: VU041581.D

Acq: 12 Dec 2020 21:20

Tgt Ion: 95 Resp: 2486


Ion Ratio Lower Upper

95 100

97 0.0 43.9 81.5#

132 0.0 63.1 117.3#

130 0.0 67.4 125.2#


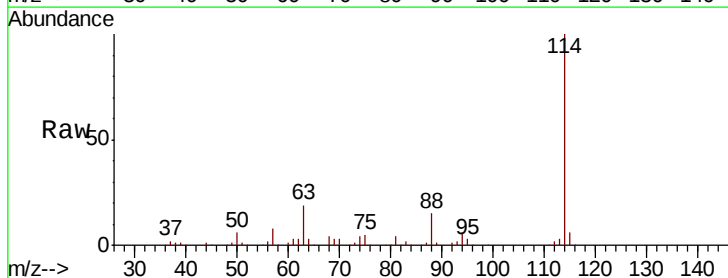



Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V



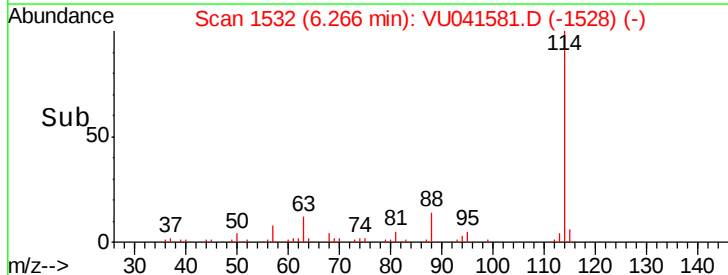
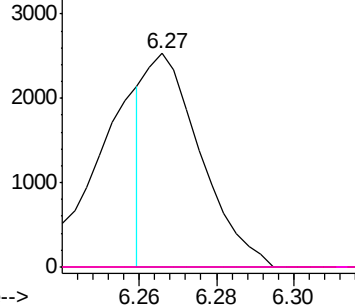


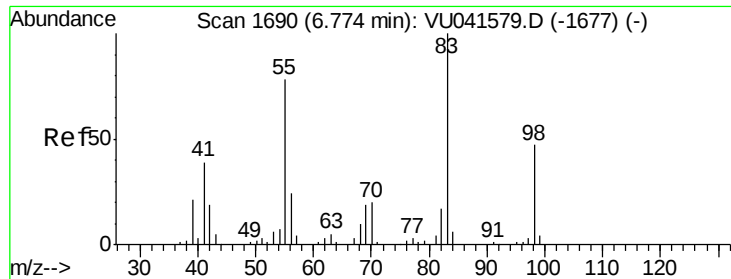

#35
Methvlcvclohexane
Concen: 0.672 ug/L
RT: 6.70 min Scan# 1667
Delta R.T. -0.07 min
Lab File: VU041581.D
Acq: 12 Dec 2020 21:20




Instrument :
MSVOA_U
ClientSampleId :
C0AS2


Tot Ion: 83 Resp: 12881
Ion Ratio Lower Upper
83 100
55 0.3 61.2 91.8#
98 0.3 36.6 54.8#

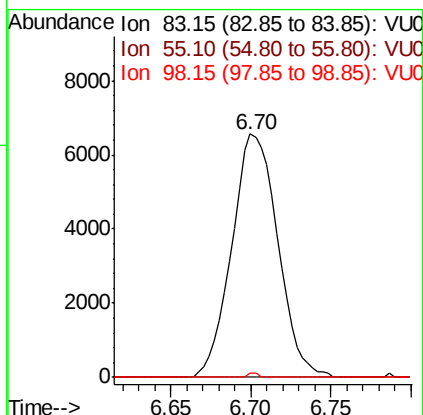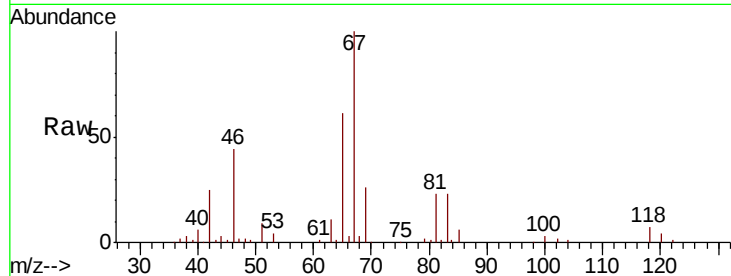

#37
1,2-Dichloropropane
Concen: 0.490 ug/L
RT: 6.70 min Scan# 1668
Delta R.T. -0.10 min
Lab File: VU041581.D
Acq: 12 Dec 2020 21:20

Tgt Ion: 63 Resp: 5914
Ion Ratio Lower Upper
63 100
112 0.0 3.1 4.7#


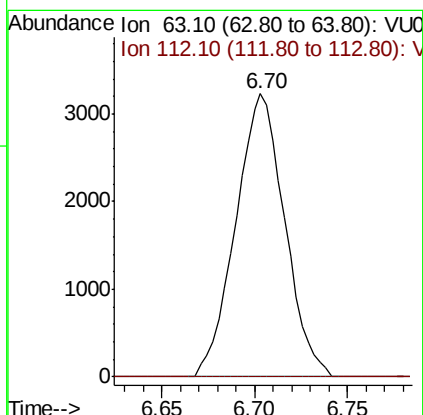




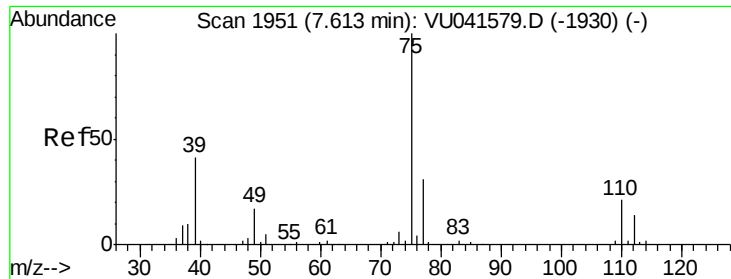

#39
 cis-1,3-Dichloropropene
 Concen: 0.078 ug/L
 RT: 7.58 min Scan# 1940
 Delta R.T. -0.04 min
 Lab File: VU041581.D
 Acq: 12 Dec 2020 21:20




Instrument :
 MSVOA_U
 ClientSampleId :
 C0AS2


Tot Ion: 75 Resp: 1389
 Ion Ratio Lower Upper
 75 100
 77 44.7 22.3 41.3#

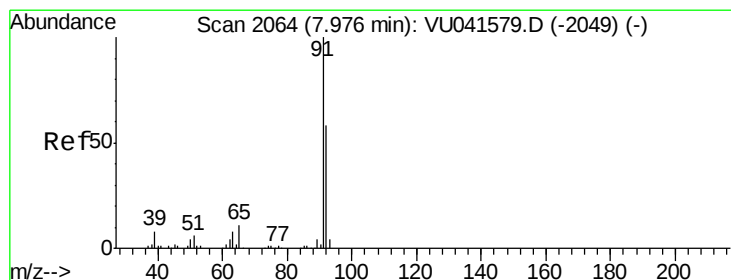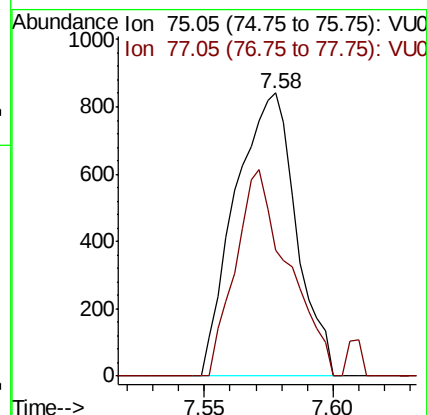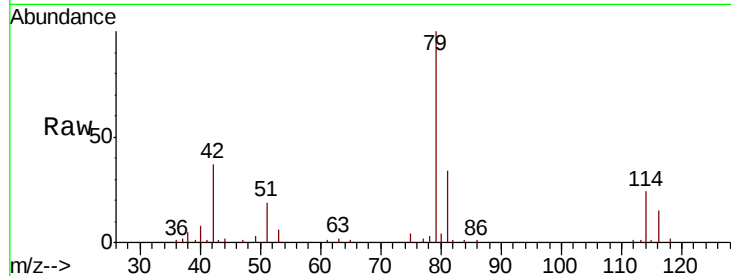

#42
 Toluene
 Concen: 0.259 ug/L
 RT: 7.98 min Scan# 2064
 Delta R.T. -0.00 min
 Lab File: VU041581.D
 Acq: 12 Dec 2020 21:20

Tgt Ion: 91 Resp: 12631
 Ion Ratio Lower Upper
 91 100
 92 55.0 40.0 74.2

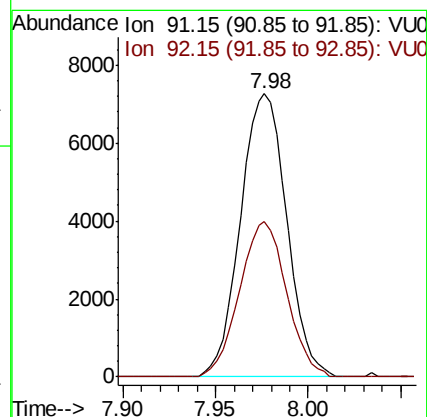

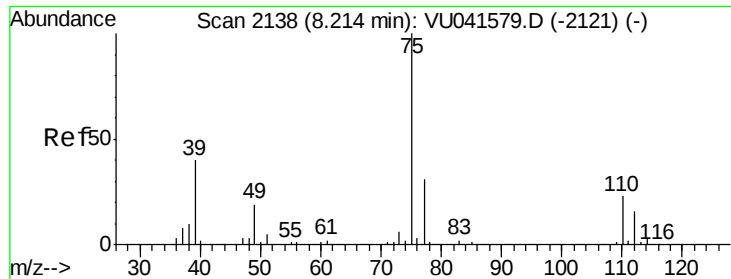

#44

trans-1,3-Dichloropropene

Concen: 0.065 ug/L

RT: 8.18 min Scan# 2128

Delta R.T. -0.03 min

Lab File: VU041581.D

Acq: 12 Dec 2020 21:20

Instrument :

MSVOA_U

ClientSampled :


C0AS2

Tot Ion: 75 Resp: 1039

Ion Ratio Lower Upper




75 100

77 40.5 23.8 44.2

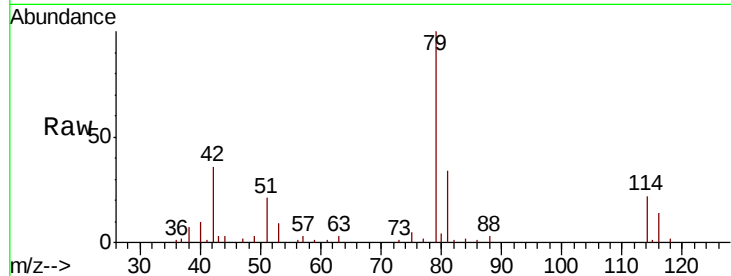

Abundance Ion 75.05 (74.75 to 75.75): VU0

Ion 77.05 (76.75 to 77.75): VU0

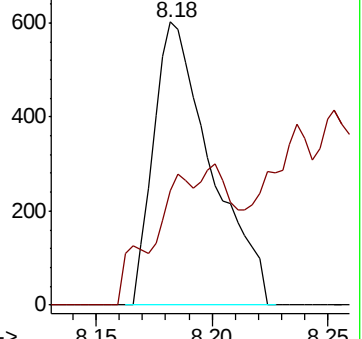

#52

Ethylbenzene

Concen: 0.054 ug/L

RT: 9.57 min Scan# 2560

Delta R.T. -0.00 min

Lab File: VU041581.D


Acq: 12 Dec 2020 21:20

Tgt Ion: 91 Resp: 2800

Ion Ratio Lower Upper



91 100


106 30.1 21.1 39.3



Abundance Ion 91.15 (90.85 to 91.85): VU0

Ion 106.15 (105.85 to 106.85): V

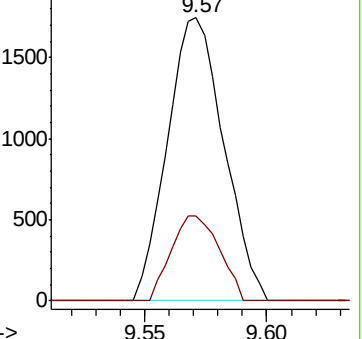

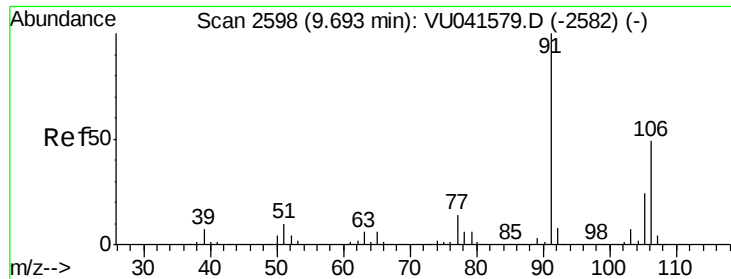

#53

m,p-Xylene

Concen: 0.176 ug/L

RT: 9.69 min Scan# 2597

Delta R.T. -0.00 min

Lab File: VU041581.D

Acq: 12 Dec 2020 21:20

Instrument :

MSVOA_U

ClientSampleId :


C0AS2

Tot Ion:106 Resp: 3410

Ion Ratio Lower Upper




106 100

91 201.1 140.4 260.8

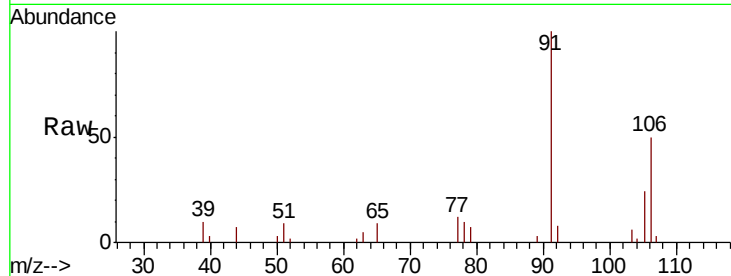

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

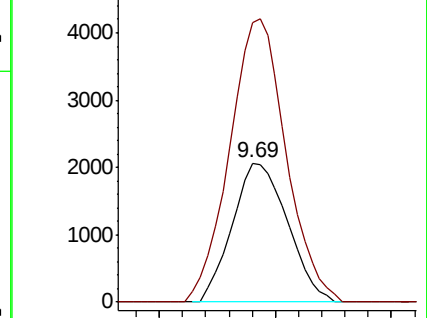

#54

o-Xylene

Concen: 0.072 ug/L

RT: 10.10 min Scan# 2724

Delta R.T. -0.00 min

Lab File: VU041581.D


Acq: 12 Dec 2020 21:20

Tgt Ion:106 Resp: 1373

Ion Ratio Lower Upper



106 100


91 236.4 151.3 281.1



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

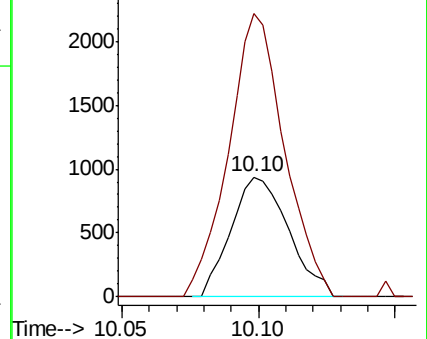

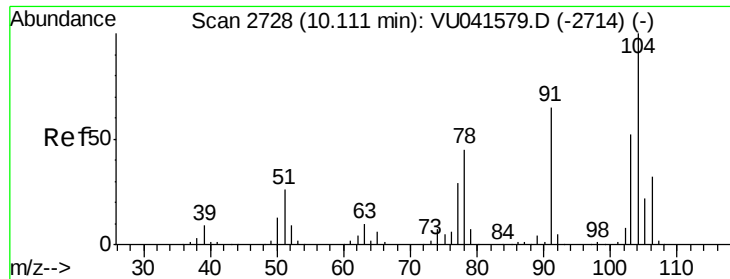

#55

Stvrene

Concen: 0.330 ug/L

RT: 10.11 min Scan# 2729

Delta R.T. 0.00 min

Lab File: VU041581.D

Acq: 12 Dec 2020 21:20

Instrument :

MSVOA_U

ClientSampled :


C0AS2

Tot Ion:104 Resp: 10816

Ion Ratio Lower Upper




104 100

78 42.5 31.1 57.9

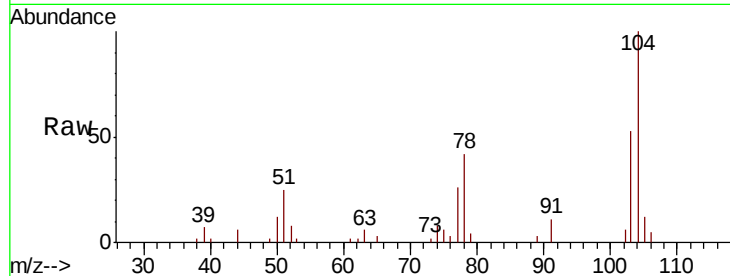

Abundance Ion 104.10 (103.80 to 104.80): VU041581.D (-2635) (-)

Ion 78.10 (77.80 to 78.80): VU041581.D (-2635) (-)

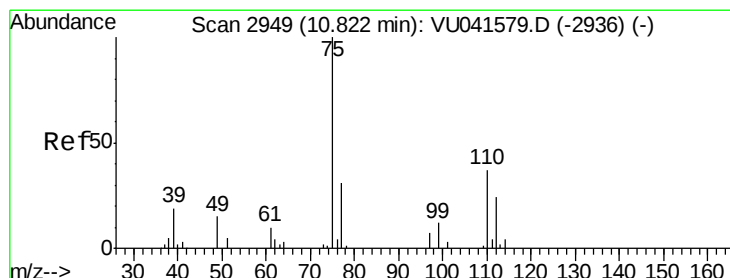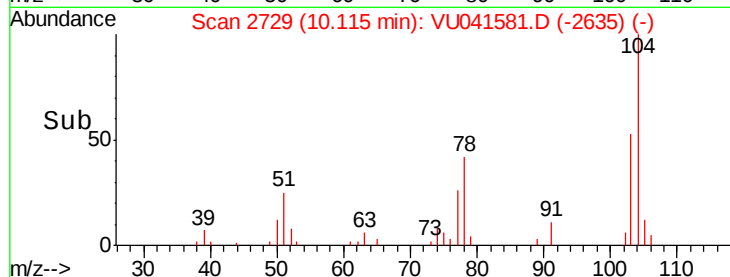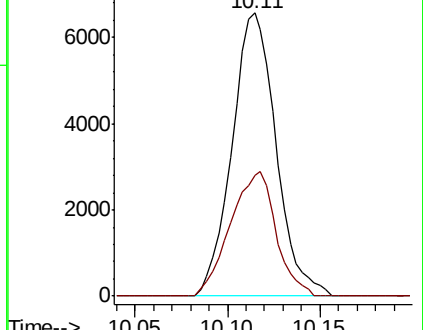

#59

1,2,3-Trichloropropane

Concen: 0.970 ug/L

RT: 11.81 min Scan# 3255

Delta R.T. 0.98 min

Lab File: VU041581.D


Acq: 12 Dec 2020 21:20

Tgt Ion: 75 Resp: 8794

Ion Ratio Lower Upper



75 100


77 31.1 26.2 39.2

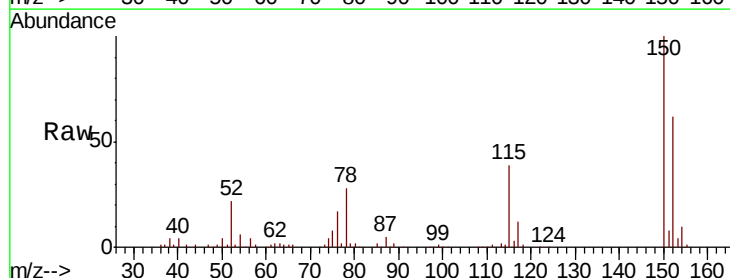

Abundance Ion 75.00 (74.70 to 75.70): VU041581.D (-2327) (-)

Ion 77.00 (76.70 to 77.70): VU041581.D (-2327) (-)

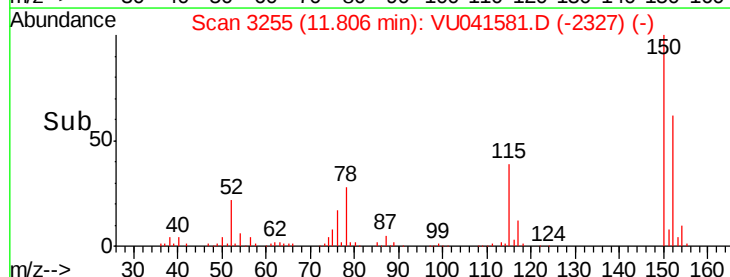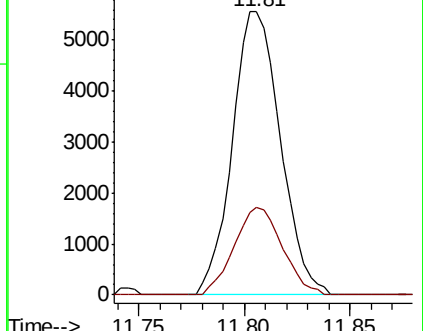


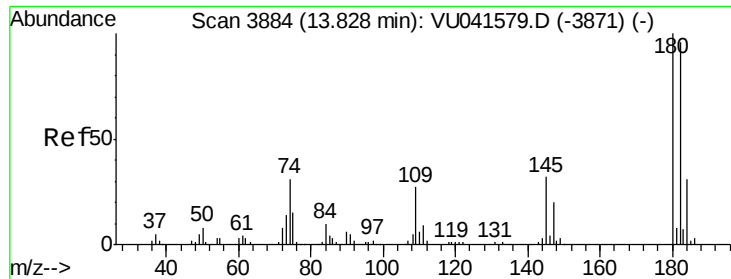




#68
 1,2,4-trichlorobenzene
 Concen: 0.030 ug/L
 RT: 13.83 min Scan# 3884
 Delta R.T. -0.00 min
 Lab File: VU041581.D
 Acq: 12 Dec 2020 21:20

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AS2

Tot Ion:180 Resp: 404
 Ion Ratio Lower Upper
 180 100
 182 88.9 75.4 113.0
 145 10.9 24.5 36.7#




Abundance Ion 179.90 (179.60 to 180.60): V
 Ion 182.00 (181.70 to 182.70): V
 Ion 144.95 (144.65 to 145.65): V

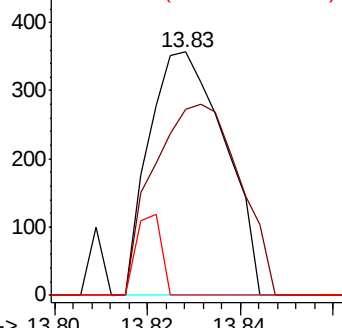

#69
 Naphthalene
 Concen: 0.070 ug/L
 RT: 14.07 min Scan# 3960
 Delta R.T. -0.00 min
 Lab File: VU041581.D
 Acq: 12 Dec 2020 21:20

Tgt Ion:128 Resp: 1930
 Ion Ratio Lower Upper
 128 100
 129 5.5 8.7 13.1#
 127 3.3 10.2 15.4#



Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 129.00 (128.70 to 129.70): V
 Ion 127.00 (126.70 to 127.70): V

