

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121220\
 Data File : VU041587.D
 Acq On : 12 Dec 2020 23:39
 Operator : SY/MD
 Sample : L5060-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B07

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 3:43:33 PM

Quant Time: Dec 13 12:01:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Dec 13 11:26:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	139065	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	132184	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	67783	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	35458	3.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.20%
7) Chloroethane-d5	1.92	69	34043	4.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.00%
11) 1,1-Dichloroethene-d2	2.58	63	57549	2.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.40%#
20) 2-Butanone-d5	4.66	46	168217	53.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.72%
24) Chloroform-d	5.08	84	83408	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.72	65	48433	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.74	84	167624	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
36) 1,2-Dichloropropane-d6	6.70	67	55474	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.91	98	144462	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	8.19	79	22487	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	8.64	63	126284	43.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.58%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	52301	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	56586	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%

Target Compounds				Ovalue
13) Acetone	2.66	43	3267m	1.645 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121220\
Data File : VU041587.D
Acq On : 12 Dec 2020 23:39
Operator : SY/MD
Sample : L5060-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0B07

Manual Integrations
APPROVED

MMDadoda
12/14/2020 3:43:33 PM

Quant Time: Dec 13 12:01:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Dec 13 11:26:38 2020
Response via : Initial Calibration

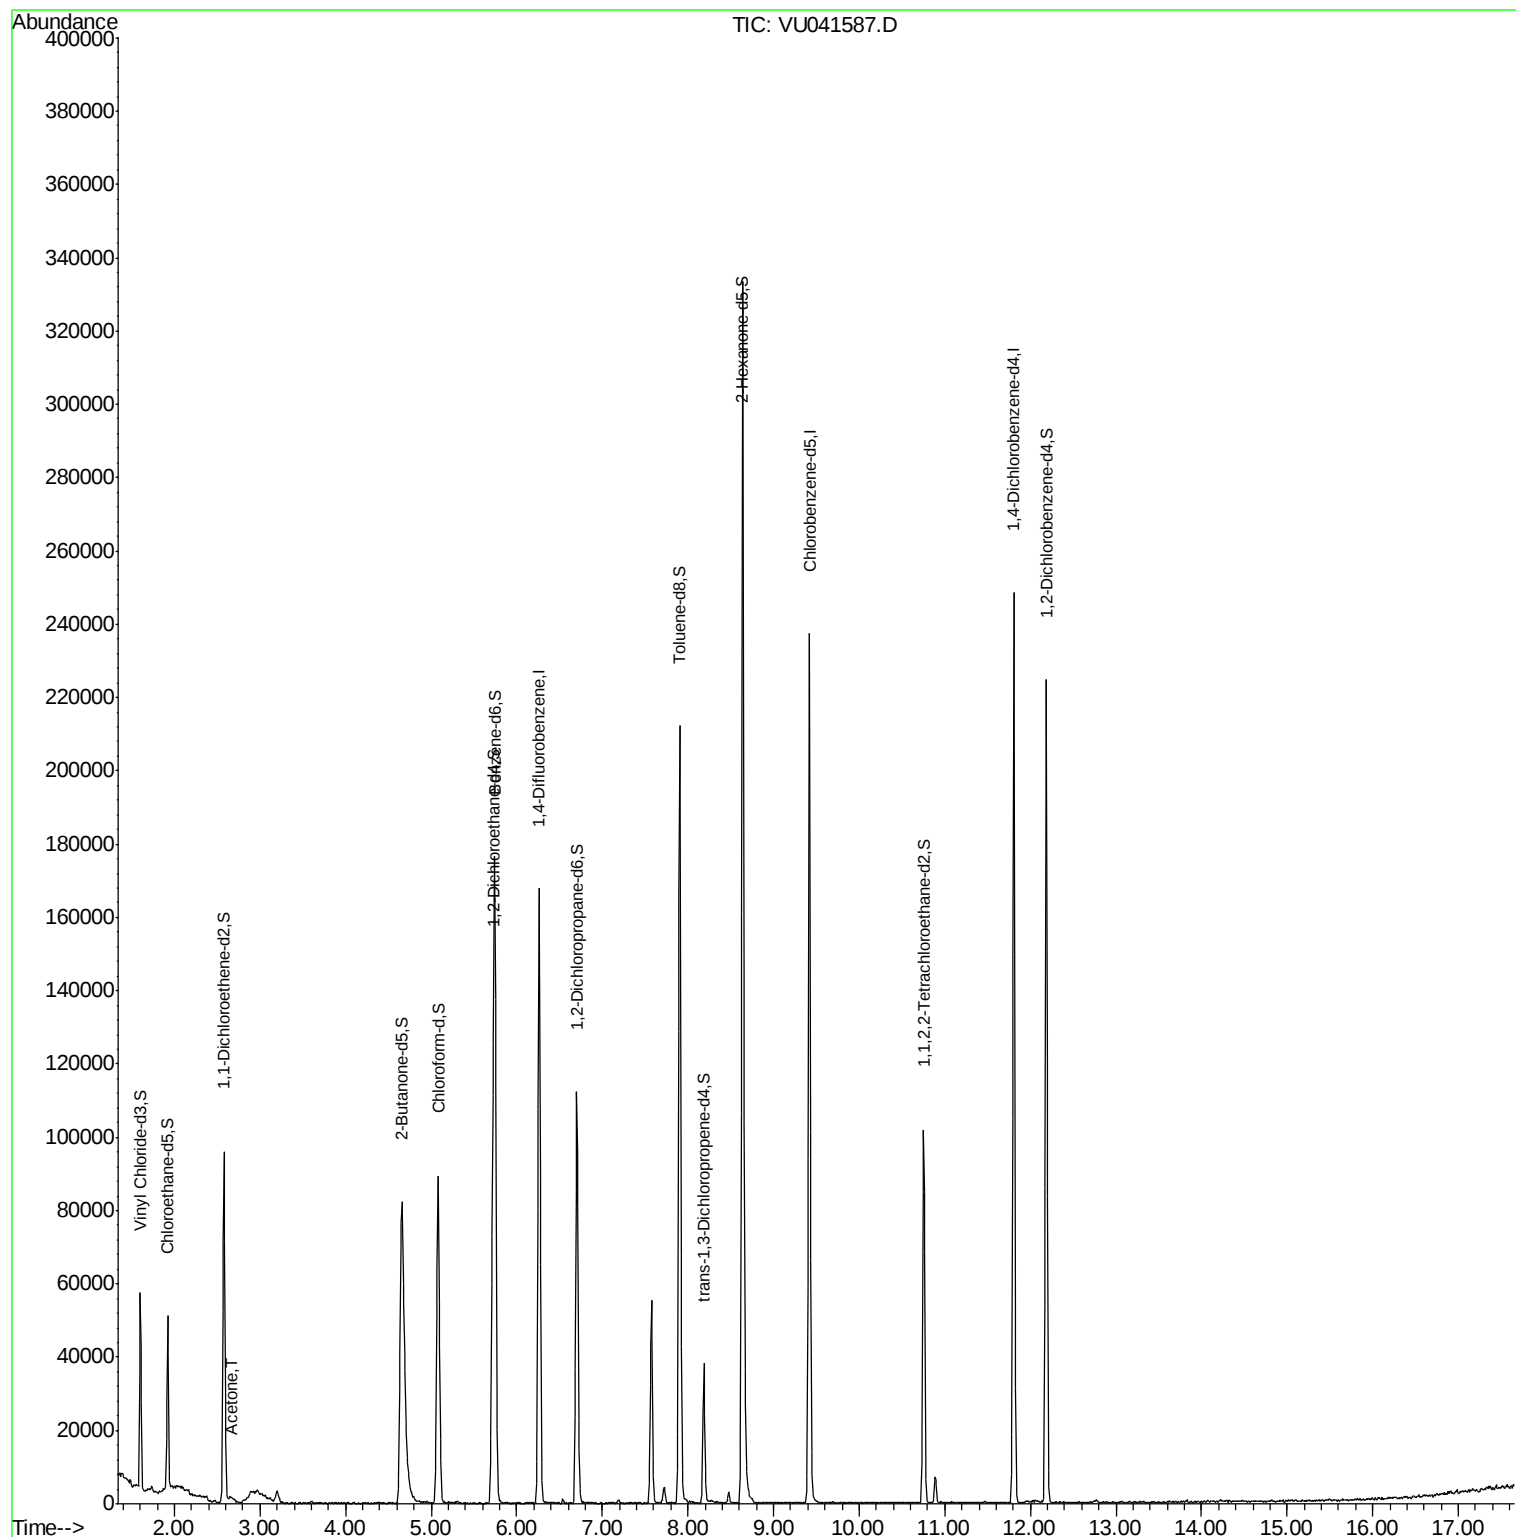

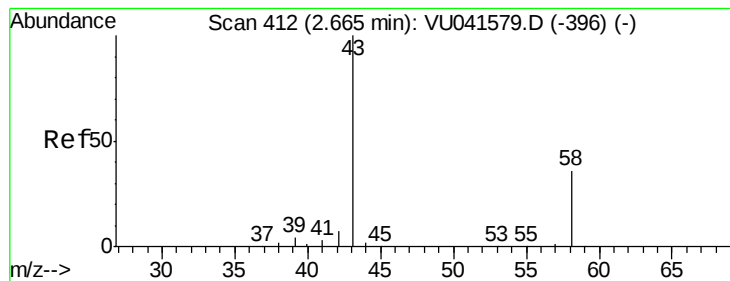

#13

Acetone

Concen: 1.645 ug/L m

RT: 2.66 min Scan# 412

Delta R.T. 0.00 min

Lab File: VU041587.D

Acq: 12 Dec 2020 23:39

Tot Ion: 43 Resp: 3267

Ion Ratio Lower Upper

43 100

58 26.0 0.0 73.2

Instrument :

MSVOA_U

ClientSampleId :

C0B07

Manual Integrations

APPROVED

MMDadoda

12/14/2020 3:43:33 PM

