


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121220\
 Data File : VU041572.D
 Acq On : 12 Dec 2020 16:36
 Operator : SY/MD
 Sample : BFB23
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB23

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sun Dec 13 11:26:38 2020

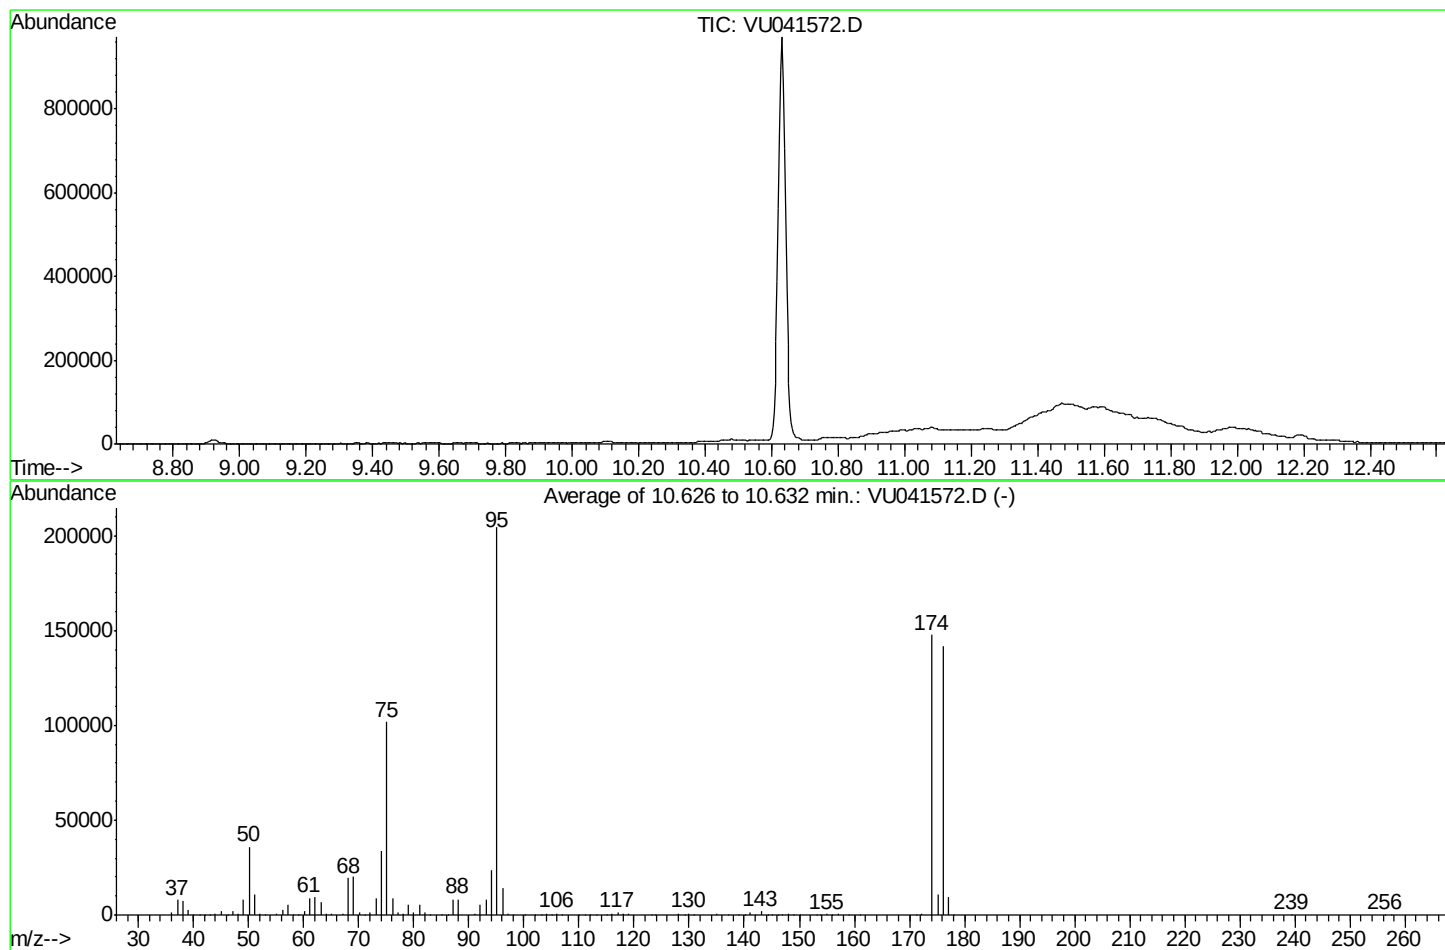

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	35824	PASS
75	95	30	80	49.8	101741	PASS
95	95	100	100	100.0	204352	PASS
96	95	5	9	6.9	14174	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.2	147584	PASS
175	174	5	9	7.5	11123	PASS
176	174	95	101	95.9	141466	PASS
177	176	5	9	6.8	9599	PASS

m/z	Abundance
36.00	1511.0
37.10	7775.0
38.10	7489.0
39.10	3236.0
40.00	159.0
41.00	944.0
42.00	312.0
43.10	1059.0
44.00	1322.0
45.00	1799.0
46.10	201.0
47.00	2297.0
48.00	997.0
49.10	7680.0
50.10	34560.0
51.10	10569.0
52.00	401.0
53.10	146.0
55.10	1023.0
56.10	2525.0
57.10	5654.0
58.10	252.0
59.10	275.0
60.10	2595.0
61.10	8516.0
62.10	9106.0
63.10	6713.0
64.00	798.0
65.10	772.0
67.10	568.0
68.10	18808.0
69.10	19888.0
70.10	1554.0
71.10	508.0
72.00	1088.0
73.10	8583.0
74.10	32720.0
75.10	96992.0
76.10	8574.0
77.00	1248.0
77.90	907.0
79.00	5405.0
80.00	1532.0
81.00	4926.0
82.00	1058.0
83.00	215.0
84.20	103.0
85.00	151.0
86.10	357.0
87.10	7700.0
88.00	8320.0
91.00	610.0
92.10	5072.0
93.10	7685.0
94.10	22696.0
95.10	194624.0
96.10	13840.0
97.10	528.0
98.10	113.0
102.10	685.0
103.20	212.0
104.00	762.0
104.90	167.0
106.00	756.0
107.00	209.0
111.00	137.0
113.00	144.0
114.90	229.0
115.90	571.0
117.00	1151.0
118.00	690.0
119.00	882.0
123.90	120.0
128.00	551.0
129.10	509.0
130.00	759.0
130.90	220.0
135.00	479.0
137.10	307.0
141.10	1572.0
142.10	162.0
143.10	1812.0
144.20	116.0
145.10	330.0
146.00	251.0
146.90	130.0
148.00	394.0
149.00	119.0
153.10	104.0
153.90	131.0
155.00	481.0
157.00	392.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

159.00	164.0
161.10	163.0
171.30	130.0
172.10	1030.0
174.10	137728.0
175.10	10653.0
176.10	130128.0
177.10	8838.0
178.10	225.0
239.50	269.0
256.40	474.0
257.50	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	1634.0
37.10	8275.0
38.10	7827.0
39.10	3165.0
40.10	175.0
41.00	883.0
42.00	314.0
43.10	1045.0
44.00	1213.0
45.10	1791.0
46.10	182.0
47.10	2338.0
48.00	970.0
49.10	8321.0
50.10	36976.0
51.10	11296.0
52.00	387.0
53.00	170.0
55.10	1197.0
56.10	2982.0
57.10	5811.0
58.10	196.0
59.10	248.0
60.10	2676.0
61.10	9273.0
62.10	9856.0
63.10	7122.0
64.00	813.0
65.10	760.0
67.00	602.0
68.10	19864.0
69.10	21504.0
70.10	1599.0
71.10	491.0
72.00	1155.0
73.10	9301.0
74.10	35176.0
75.10	105160.0
76.10	9277.0
77.00	1293.0
77.90	1071.0
79.00	5468.0
80.00	1518.0
81.00	5432.0
82.00	1236.0
82.90	229.0
84.20	132.0
85.00	206.0
86.10	311.0
87.00	8499.0
88.00	8806.0
91.00	613.0
92.10	5606.0
93.10	8481.0
94.10	24072.0
95.10	211200.0
96.10	14743.0
97.10	560.0
98.10	130.0
100.10	106.0
102.20	614.0
103.20	204.0
104.00	812.0
104.90	203.0
106.00	824.0
107.00	202.0
110.00	107.0
111.00	146.0
112.00	104.0
113.10	118.0
114.90	198.0
115.90	770.0
117.00	1220.0
118.00	733.0
119.00	913.0
123.10	101.0
123.90	149.0
128.00	673.0
129.10	473.0
130.00	847.0
130.90	229.0
135.00	529.0
137.10	327.0
139.00	108.0
141.10	1778.0
142.00	245.0
143.10	1916.0
145.10	321.0
146.10	299.0
146.90	189.0
148.00	451.0
149.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

153.10	120.0
153.90	107.0
155.10	546.0
156.00	112.0
157.00	434.0
159.00	216.0
161.00	181.0
172.10	1026.0
174.10	152832.0
175.10	11534.0
176.10	146112.0
177.10	9872.0
178.00	253.0
239.50	314.0
256.40	443.0
257.50	324.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	1585.0
37.00	7974.0
38.00	7324.0
39.10	2972.0
40.00	205.0
41.00	747.0
42.00	331.0
43.10	1074.0
44.00	1143.0
45.00	1680.0
46.10	166.0
47.10	2193.0
48.00	974.0
49.10	8088.0
50.10	35936.0
51.10	10965.0
52.00	429.0
53.00	155.0
55.10	1264.0
56.10	3242.0
57.10	5586.0
58.10	174.0
59.10	205.0
60.10	2689.0
61.10	9320.0
62.10	9322.0
63.10	6735.0
64.10	839.0
65.00	733.0
67.00	612.0
68.10	19544.0
69.10	20928.0
70.10	1508.0
71.20	512.0
72.00	1164.0
73.10	9228.0
74.10	34064.0
75.10	103072.0
76.10	9029.0
77.10	1258.0
78.00	1044.0
79.00	5266.0
80.00	1478.0
81.00	5418.0
82.00	1269.0
83.00	285.0
84.10	146.0
85.00	247.0
86.10	254.0
87.00	8915.0
88.00	8182.0
91.00	641.0
92.10	5640.0
93.10	8304.0
94.10	23672.0
95.10	207232.0
96.10	13941.0
97.10	563.0
98.10	173.0
102.20	616.0
103.00	197.0
104.00	767.0
105.00	216.0
106.00	848.0
106.90	199.0
110.00	117.0
111.10	158.0
112.00	116.0
113.10	104.0
115.00	167.0
115.90	841.0
117.00	1241.0
118.00	670.0
119.00	871.0
123.10	107.0
123.90	147.0
128.00	701.0
129.10	448.0
130.00	890.0
130.90	183.0
135.00	507.0
137.10	300.0
139.00	126.0
140.20	119.0
141.00	1742.0
142.00	294.0
143.10	1960.0
145.10	282.0
146.10	296.0
146.90	172.0
148.00	457.0
149.00	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

150.10	104.0
153.00	117.0
155.10	560.0
156.00	118.0
157.00	410.0
159.00	222.0
161.00	168.0
172.10	914.0
174.10	152192.0
175.10	11184.0
176.10	148160.0
177.10	10088.0
178.00	238.0
239.40	303.0
256.40	401.0
257.40	312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
39.00	180.0
40.10	101.0
41.10	702.0
42.10	274.0
43.00	965.0
44.00	461.0
55.10	470.0
57.00	417.0
59.00	227.0
60.00	641.0
61.00	233.0
69.10	316.0
70.00	106.0
71.10	332.0
73.10	284.0
83.00	223.0
84.10	154.0
85.10	152.0
98.10	103.0
99.10	104.0
102.10	563.0
111.20	127.0
129.20	174.0
185.20	117.0
239.50	134.0
256.40	356.0
257.60	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23