

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
 Data File : VU052355.D
 Acq On : 12 Dec 2022 16:10
 Operator : JC/MD
 Sample : N5930-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 EXZA0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 12/13/2022
 Supervised By :Mahesh Dadoda 12/13/2022

Supervised By :Mahesh
 Dadoda
 12/13/2022

Quant Time: Dec 13 01:04:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 13 01:01:45 2022
 Response via : Initial Calibration

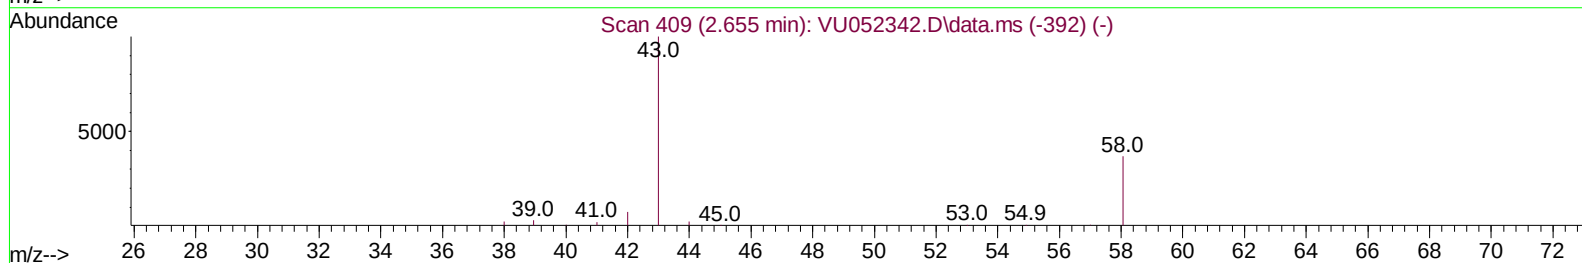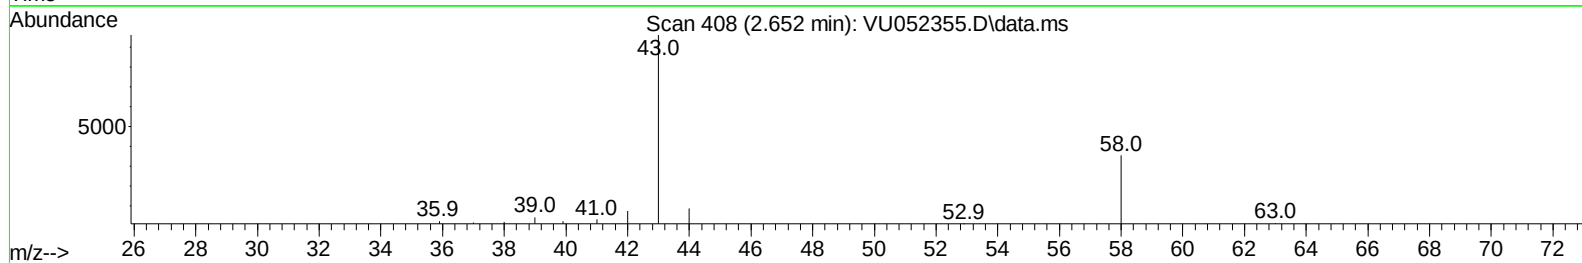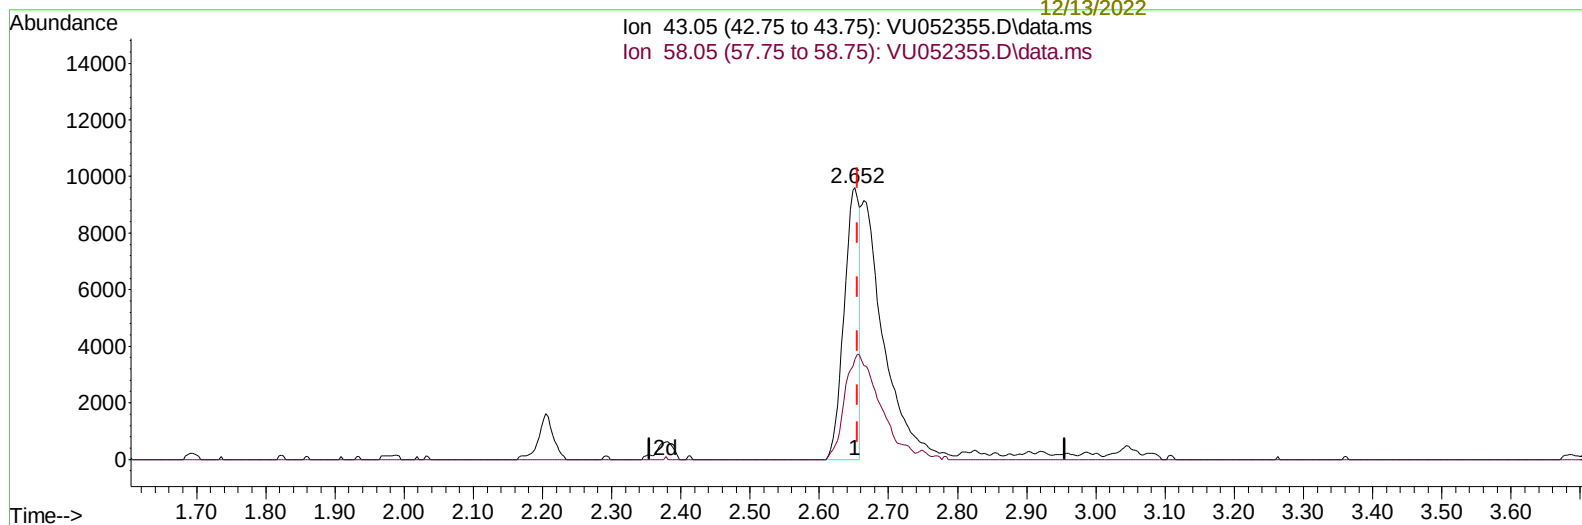

TIC: VU052355.D\data.ms

(13) Acetone (T)

2.652min (-0.003) 4.91 ug/L

response 14749

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	38.00	88.68#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
 Data File : VU052355.D
 Acq On : 12 Dec 2022 16:10
 Operator : JC/MD
 Sample : N5930-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 EXZA0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 12/13/2022
 Supervised By :Mahesh Dadoda 12/13/2022

Supervised By :Mahesh
 Dadoda
 12/13/2022

Quant Time: Dec 13 01:04:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 13 01:01:45 2022
 Response via : Initial Calibration

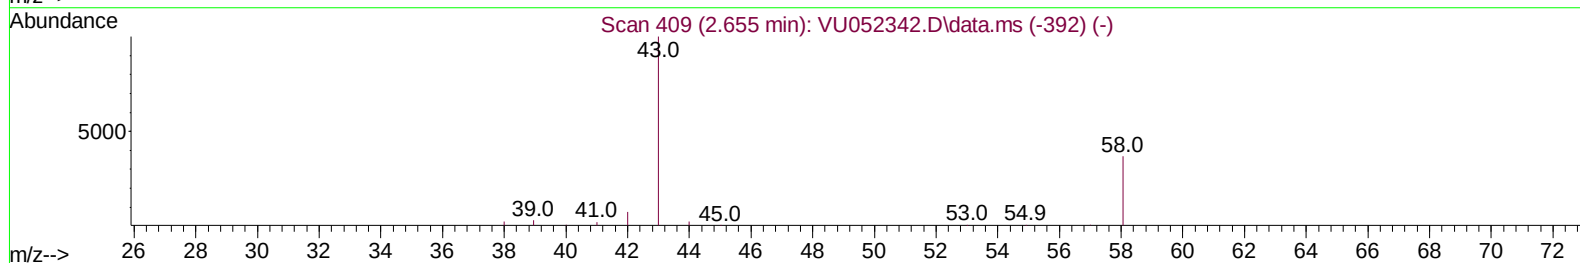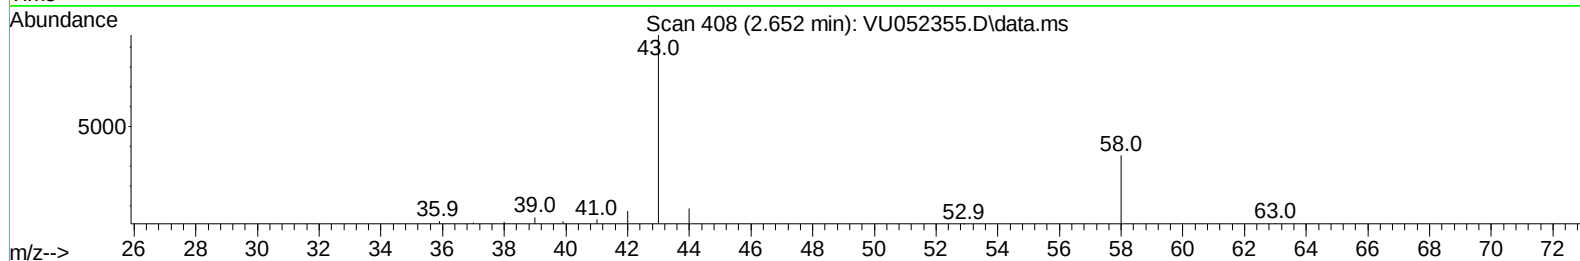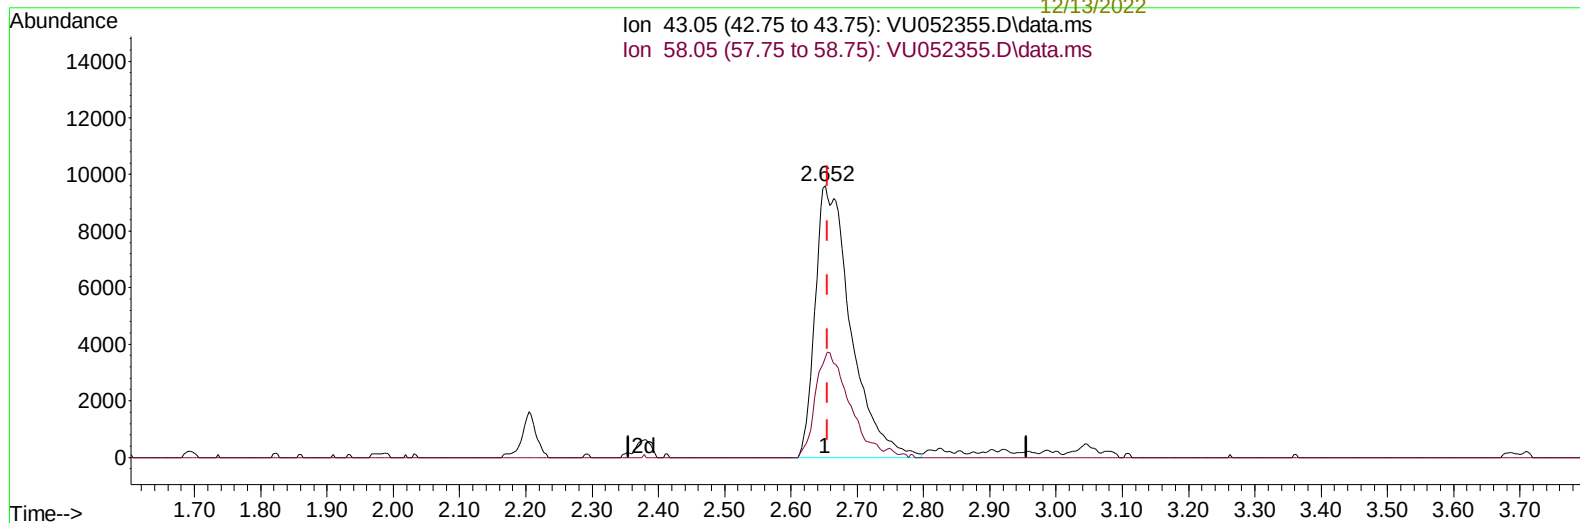

TIC: VU052355.D\data.ms

(13) Acetone (T)

2.652min (-0.003) 11.96 ug/L m

response 35944

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	38.00	36.39
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
 Data File : VU052355.D
 Acq On : 12 Dec 2022 16:10
 Operator : JC/MD
 Sample : N5930-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZA0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 12/13/2022
 Supervised By :Mahesh Dadoda 12/13/2022

Supervised By :Mahesh
 Dadoda
 12/13/2022

Quant Time: Dec 13 01:04:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 13 01:01:45 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		250936	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117		258070	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152		106379	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.600	65		88025	3.606	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	72.200%	
7) Chloroethane-d5	1.915	69		78314	4.131	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	82.600%	
11) 1,1-Dichloroethene-d2	2.568	65		34770	3.974	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	79.400%	
20) 2-Butanone-d5	4.636	46		250115	56.531	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	113.060%	
24) Chloroform-d	5.063	84		181003	5.047	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.700	65		88226	4.870	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	97.400%	
32) Benzene-d6	5.726	84		340037	4.438	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.800%	
36) 1,2-Dichloropropane-d6	6.687	67		112900	4.762	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	95.200%	
41) Toluene-d8	7.896	98		271872	3.922	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	78.400%	
43) trans-1,3-Dichloroprop...	8.176	79		35919	4.157	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	83.200%	
46) 2-Hexanone-d5	8.632	63		172823	47.197	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	94.400%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84		100304	4.879	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	12.188	152		103027	5.059	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	101.200%	
Target Compounds							
							Qvalue
13) Acetone	2.652	43		35944m	11.964	ug/L	
16) Methylene chloride	3.047	84		121968	4.953	ug/L	99
25) Chloroform	5.086	83		364814	10.237	ug/L	95
34) Trichloroethene	6.542	95		10964	0.523	ug/L	97
38) Bromodichloromethane	7.105	83		7667	0.289	ug/L	91
49) Dibromochloromethane	8.803	129		1335	0.073	ug/L	93
53) m,p-Xylene	9.693	106		3134	0.096	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052355.D
Acq On : 12 Dec 2022 16:10
Operator : JC/MD
Sample : N5930-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 12/13/2022
Supervised By :Mahesh Dadoda 12/13/2022

Supervised By :Mahesh
Dadoda
12/13/2022

Quant Time: Dec 13 01:04:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 13 01:01:45 2022
Response via : Initial Calibration

