

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
 Data File : VU052347.D
 Acq On : 12 Dec 2022 13:03
 Operator : JC/MD
 Sample : N5960-02DL2 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L25DL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rBV	134947	155208	14.55%	1.665%
2	1.916	170	179	196	rBV	109289	148309	13.90%	1.591%
3	2.568	370	382	399	rBV	204298	334627	31.37%	3.589%
4	3.047	518	531	556	rVB	43235	84994	7.97%	0.912%
5	3.189	562	575	586	rBV2	9549	21616	2.03%	0.232%
6	4.655	1009	1031	1075	rBV3	161767	647113	60.67%	6.941%
7	5.060	1140	1157	1179	rBV	182913	407060	38.16%	4.366%
8	5.723	1342	1363	1404	rBV2	374805	980677	91.94%	10.518%
9	6.247	1511	1526	1562	rBV	302182	582240	54.59%	6.245%
10	6.539	1602	1617	1642	rBV	541576	1028846	96.46%	11.035%
11	6.687	1650	1663	1685	rBV	233979	460322	43.16%	4.937%
12	7.562	1923	1935	1957	rBV	105075	191507	17.95%	2.054%
13	7.896	2025	2039	2060	rBV	424071	747618	70.09%	8.019%
14	8.179	2116	2127	2142	rBV	63715	112422	10.54%	1.206%
15	8.636	2256	2269	2305	rBV2	514538	1066634	100.00%	11.440%
16	9.414	2492	2511	2539	rBV	445600	742133	69.58%	7.960%
17	10.751	2913	2927	2946	rBV	195445	327961	30.75%	3.518%
18	11.809	3244	3256	3274	rBV	389492	630351	59.10%	6.761%
19	12.189	3361	3374	3397	rBV	402765	653789	61.29%	7.012%




Sum of corrected areas: 9323427

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052347.D
Acq On : 12 Dec 2022 13:03
Operator : JC/MD
Sample : N5960-02DL2 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L25DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

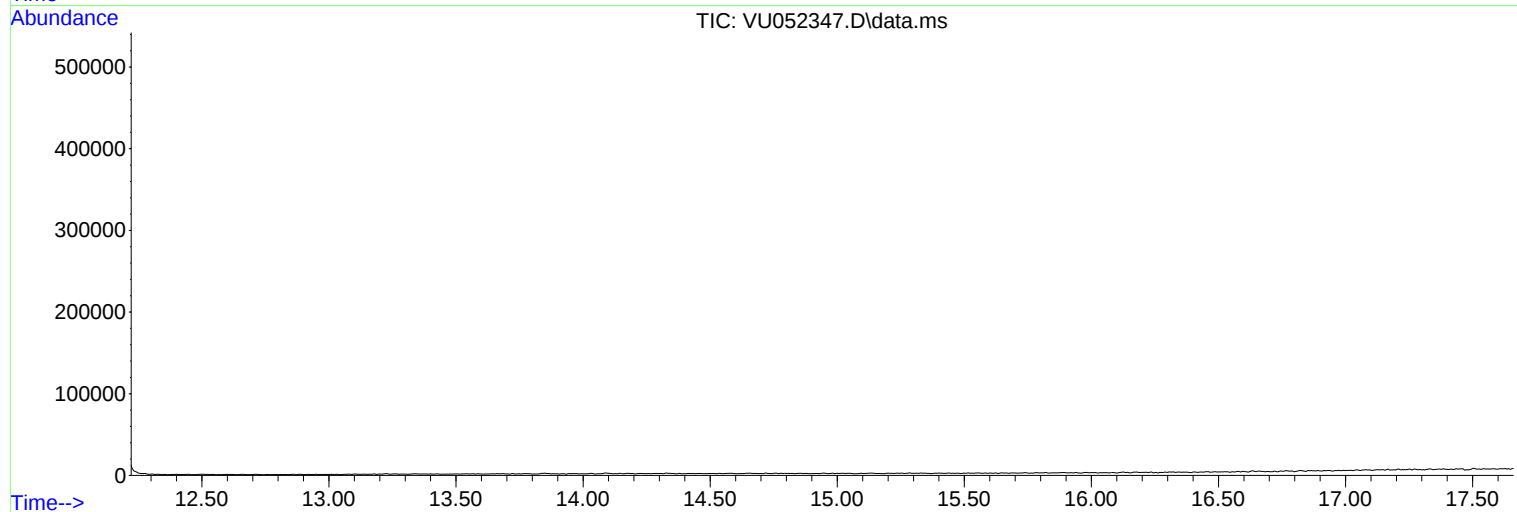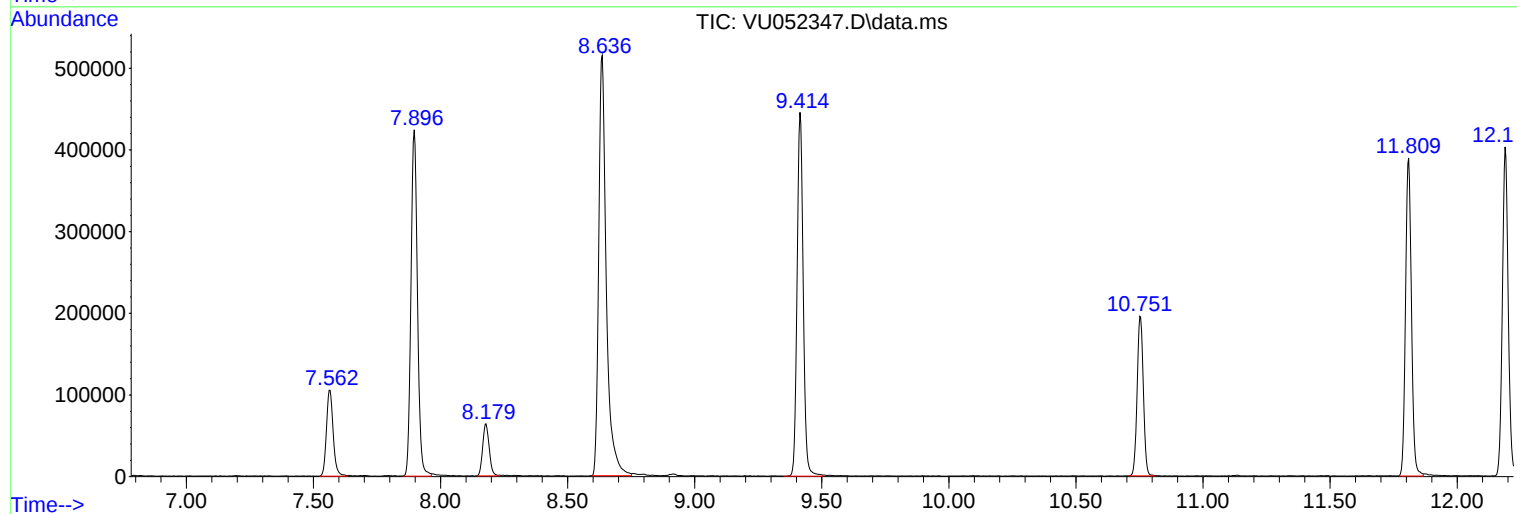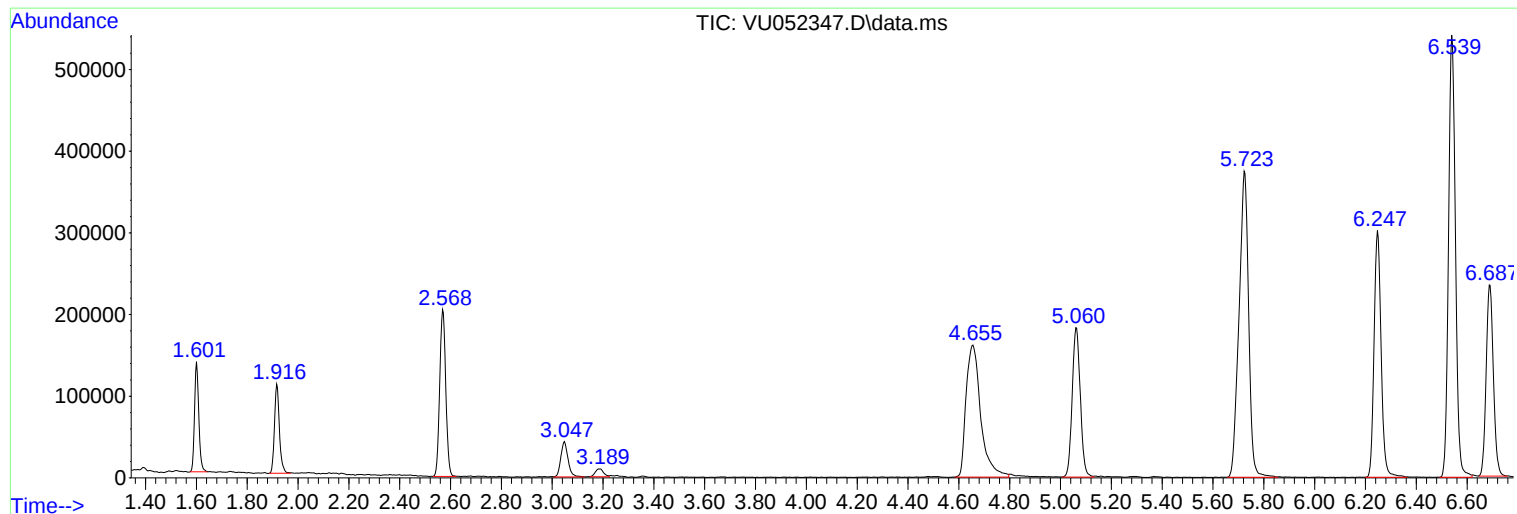

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052347.D
Acq On : 12 Dec 2022 13:03
Operator : JC/MD
Sample : N5960-02DL2 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L25DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052347.D
Acq On : 12 Dec 2022 13:03
Operator : JC/MD
Sample : N5960-02DL2 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L25DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc