

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
 Data File : VU052350.D
 Acq On : 12 Dec 2022 14:13
 Operator : JC/MD
 Sample : N5922-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB	146872	169804	14.91%	2.019%
2	1.916	169	179	201	rBV	116927	160267	14.07%	1.906%
3	2.568	370	382	397	rBV	225704	369886	32.48%	4.399%
4	3.047	519	531	545	rVB2	9320	17708	1.56%	0.211%
5	4.639	1009	1026	1061	rBV	138677	477480	41.93%	5.679%
6	5.060	1141	1157	1187	rBV	195541	429566	37.72%	5.109%
7	5.722	1338	1363	1398	rBV2	400070	1040150	91.34%	12.371%
8	6.247	1510	1526	1549	rBV	295264	571006	50.14%	6.791%
9	6.687	1649	1663	1690	rBV	243743	490195	43.05%	5.830%
10	7.562	1920	1935	1957	rBV	106398	195866	17.20%	2.329%
11	7.896	2024	2039	2065	rBV	450840	794753	69.79%	9.452%
12	8.176	2113	2126	2148	rBV2	69157	121475	10.67%	1.445%
13	8.632	2254	2268	2302	rBV2	554312	1138732	100.00%	13.543%
14	9.414	2498	2511	2539	rBV	430637	730204	64.12%	8.684%
15	10.751	2912	2927	2944	rBV	210058	342020	30.04%	4.068%
16	11.809	3243	3256	3280	rBV	374000	600306	52.72%	7.139%
17	12.060	3325	3334	3345	rBV3	9323	16989	1.49%	0.202%
18	12.188	3360	3374	3407	rBV	429617	705050	61.92%	8.385%
19	16.883	4826	4834	4845	rVB2	25643	36832	3.23%	0.438%




Sum of corrected areas: 8408289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052350.D
Acq On : 12 Dec 2022 14:13
Operator : JC/MD
Sample : N5922-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

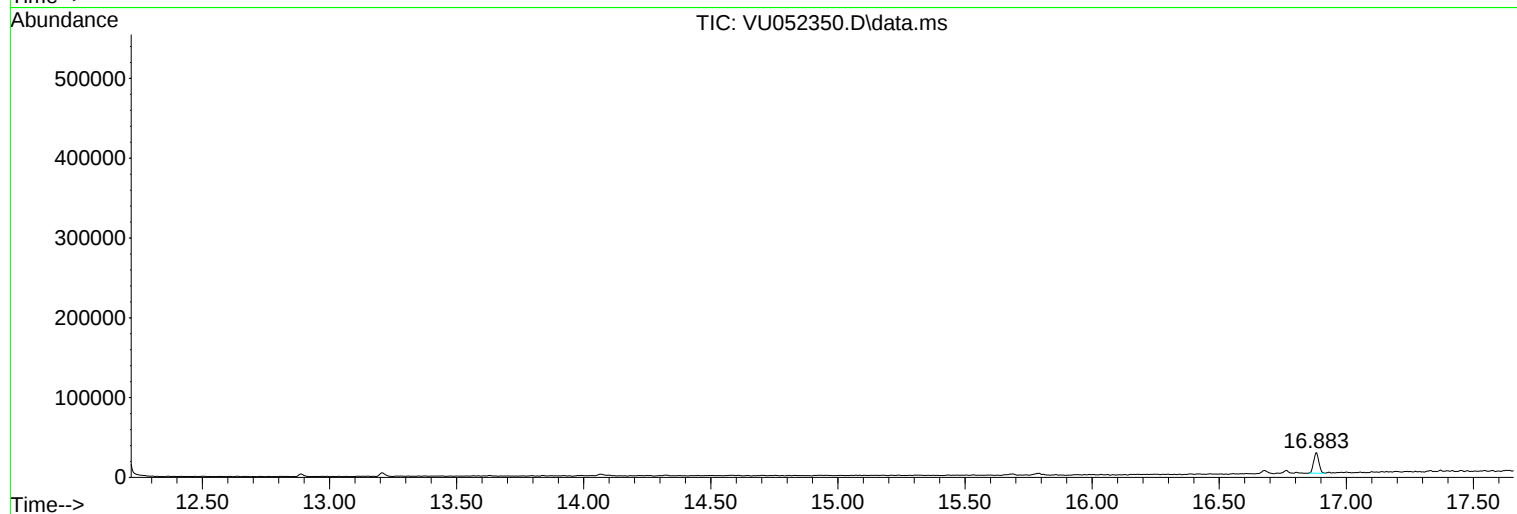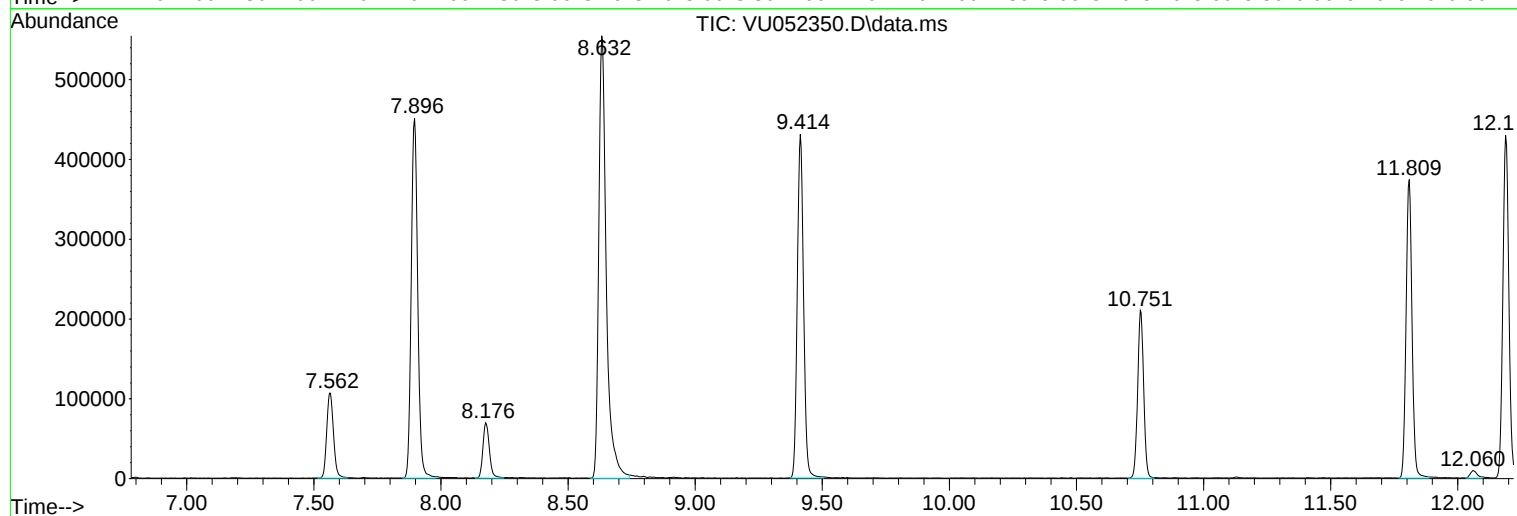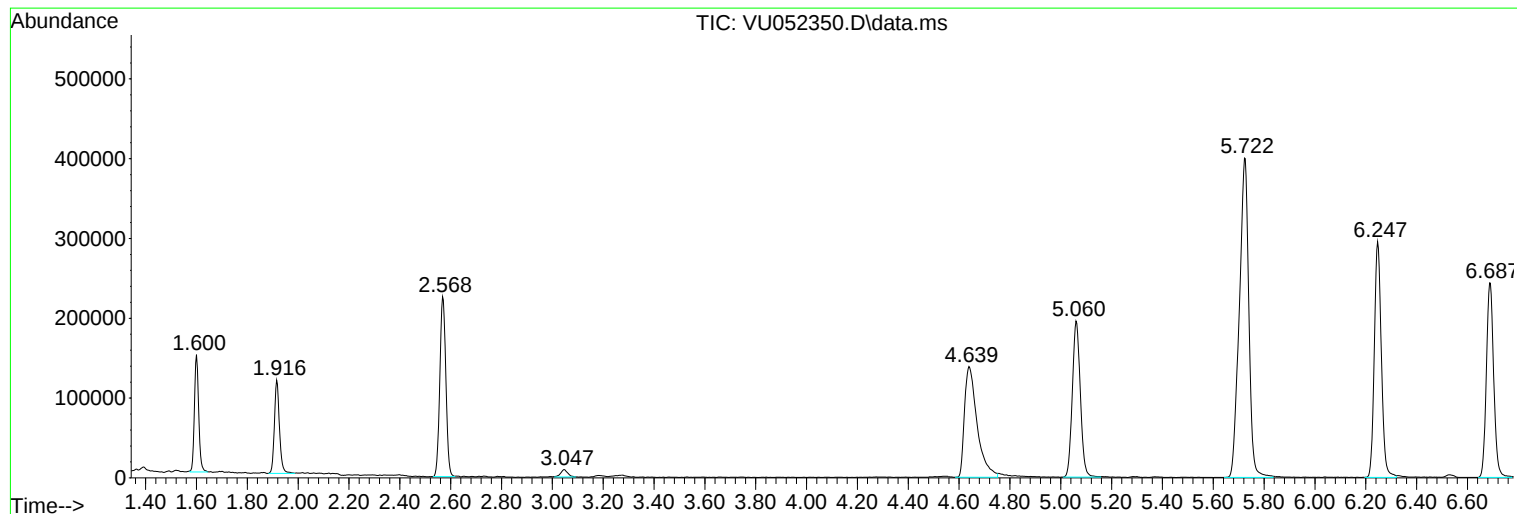

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052350.D
Acq On : 12 Dec 2022 14:13
Operator : JC/MD
Sample : N5922-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052350.D
Acq On : 12 Dec 2022 14:13
Operator : JC/MD
Sample : N5922-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc