


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121222\
Data File : VU052341.D
Acq On : 12 Dec 2022 09:33
Operator : JC/MD
Sample : BFB177
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB177

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 13 01:01:45 2022

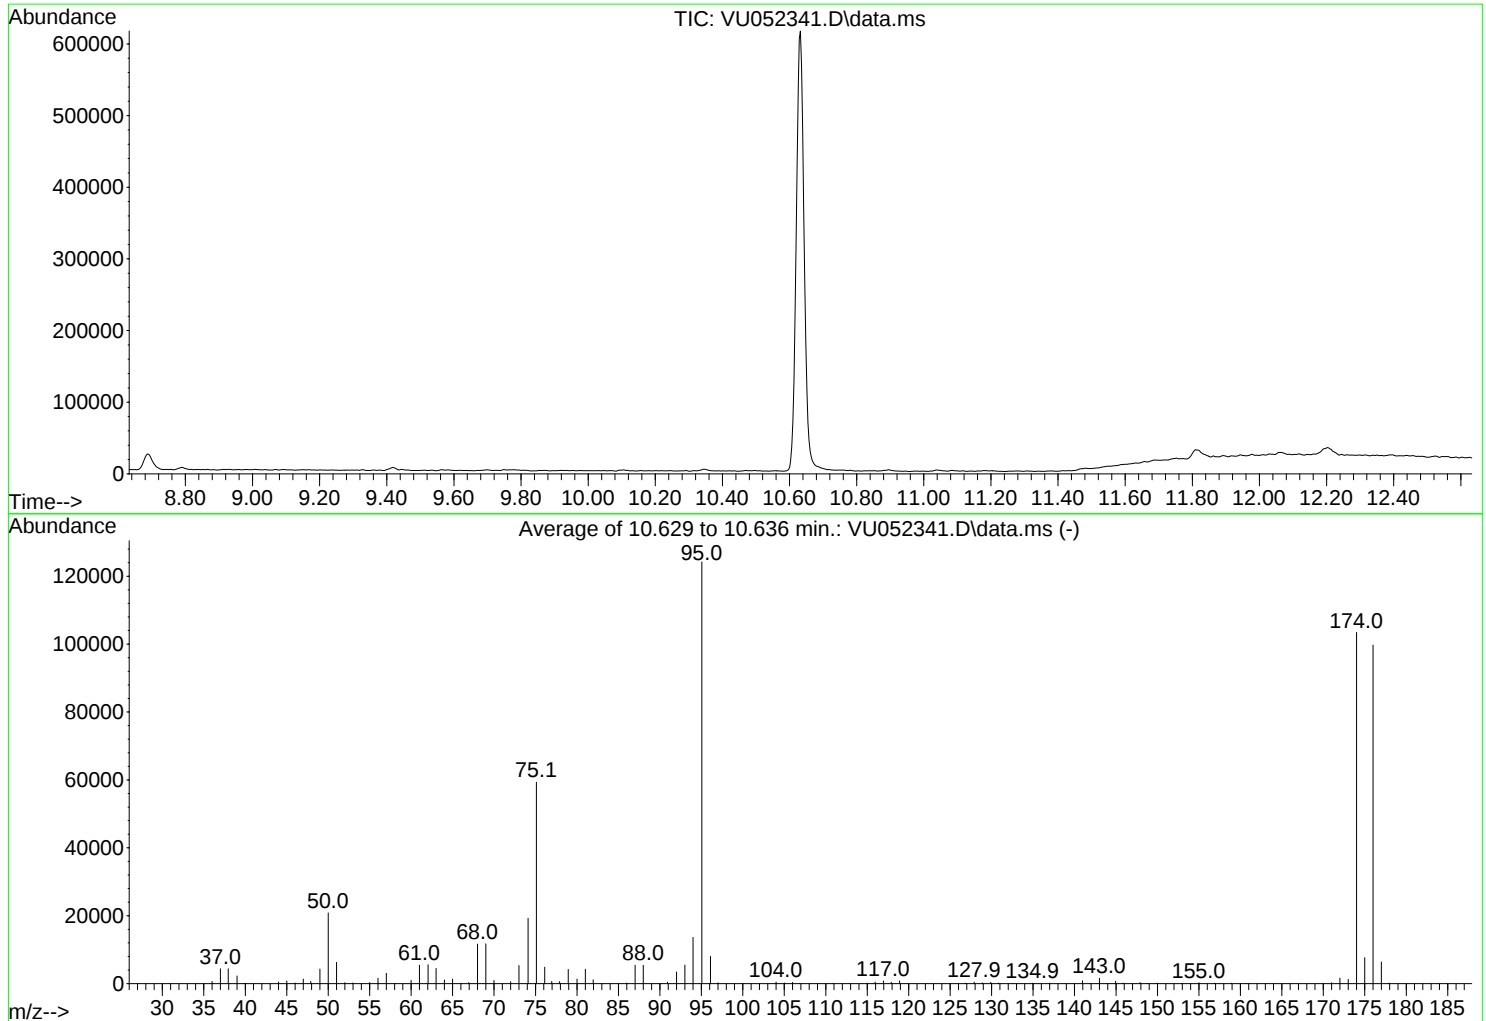

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	20851	PASS
75	95	30	80	47.8	59347	PASS
95	95	100	100	100.0	124235	PASS
96	95	5	9	6.5	8024	PASS
173	174	0.00	2	1.2	1292	PASS
174	95	50	120	83.3	103440	PASS
175	174	5	9	7.4	7649	PASS
176	174	95	101	96.4	99731	PASS
177	176	5	9	6.4	6377	PASS

m/z	Abundance
36.00	2282.0
37.00	184.0
37.90	774.0
39.90	244.0
44.00	369.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
36.00	2907.0
37.00	4831.0
38.00	5344.0
39.00	2200.0
39.90	363.0
44.00	801.0
45.00	880.0
46.00	217.0
47.00	1516.0
47.90	676.0
49.00	4563.0
50.00	21848.0
51.00	6476.0
52.00	273.0
53.00	229.0
55.00	308.0
56.00	1654.0
57.00	3352.0
60.00	1043.0
61.00	5568.0
62.00	5759.0
63.00	4543.0
64.00	1007.0
65.00	1472.0
66.10	114.0
67.00	309.0
68.00	11718.0
69.00	11813.0
70.00	938.0
72.00	604.0
73.00	5288.0
74.10	19480.0
75.10	60744.0
76.10	4750.0
76.90	659.0
77.90	608.0
79.00	4307.0
80.00	1324.0
81.00	4388.0
82.00	1322.0
83.00	106.0
86.00	236.0
87.00	5466.0
88.00	5882.0
90.90	475.0
92.00	3416.0
93.00	5745.0
94.00	13919.0
95.10	127760.0
96.10	8275.0
97.00	249.0
104.00	552.0
105.10	179.0
106.00	456.0
110.90	138.0
115.10	112.0
116.00	490.0
117.00	827.0
117.90	478.0
118.90	923.0
126.80	174.0
127.90	497.0
128.90	287.0
129.90	411.0
130.90	165.0
134.90	154.0
137.00	168.0
140.90	883.0
141.90	123.0
143.00	1776.0
143.90	110.0
145.00	714.0
145.80	157.0
147.90	310.0
148.80	110.0
149.90	140.0
152.90	103.0
155.00	321.0
156.90	123.0
158.90	106.0
161.00	110.0
171.00	286.0
172.00	1745.0
173.00	1371.0
174.00	102392.0
175.00	7913.0
176.00	98104.0
177.00	6426.0
177.90	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
36.00	2937.0
37.00	4767.0
38.00	5251.0
39.00	2352.0
39.90	337.0
44.00	856.0
45.00	862.0
46.00	192.0
47.00	1371.0
47.90	690.0
49.00	4392.0
50.00	21624.0
51.00	6479.0
52.00	312.0
53.00	211.0
55.00	348.0
56.00	1654.0
57.00	3158.0
60.00	1027.0
61.00	5639.0
62.00	5688.0
63.00	4609.0
64.00	1141.0
65.00	1318.0
66.00	111.0
67.00	344.0
68.00	12087.0
69.00	12165.0
70.00	969.0
72.00	571.0
73.00	5540.0
74.10	19800.0
75.10	61152.0
76.10	5051.0
76.90	676.0
77.90	625.0
79.00	4291.0
80.00	1421.0
81.00	4390.0
82.00	1181.0
83.00	114.0
86.00	172.0
87.00	5555.0
88.00	5673.0
90.90	409.0
92.00	3509.0
93.00	5560.0
94.00	14097.0
95.10	128032.0
96.10	8252.0
97.00	226.0
104.00	492.0
105.00	214.0
106.00	395.0
106.80	103.0
110.80	118.0
115.00	120.0
116.00	469.0
117.00	814.0
117.90	452.0
118.90	784.0
126.80	151.0
127.90	478.0
128.90	267.0
129.90	454.0
130.80	186.0
135.00	160.0
137.00	175.0
141.00	848.0
141.90	100.0
143.00	1659.0
144.90	729.0
145.80	192.0
147.90	343.0
148.80	125.0
149.90	148.0
152.90	107.0
155.00	296.0
156.90	124.0
158.90	137.0
160.70	116.0
171.00	311.0
172.00	1682.0
173.00	1334.0
174.00	106848.0
175.00	7773.0
176.00	103312.0
177.00	6594.0
177.90	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
36.00	2949.0
37.00	4117.0
38.00	4827.0
39.00	2221.0
39.80	283.0
44.00	832.0
45.00	713.0
46.00	160.0
47.00	1204.0
47.90	561.0
49.00	3897.0
50.00	19080.0
51.00	5891.0
52.00	322.0
52.90	161.0
55.00	362.0
56.00	1481.0
57.00	2731.0
58.10	110.0
60.00	949.0
61.00	5086.0
62.10	5194.0
63.00	4355.0
64.00	1114.0
65.00	1176.0
66.10	119.0
66.90	331.0
68.00	11157.0
69.00	11247.0
70.00	881.0
72.00	549.0
73.00	5177.0
74.10	18408.0
75.10	56144.0
76.10	4758.0
77.00	660.0
77.90	562.0
78.90	3945.0
80.00	1382.0
81.00	3968.0
81.90	914.0
86.00	113.0
87.00	5185.0
88.00	4704.0
90.90	330.0
92.00	3368.0
93.00	5078.0
94.00	12918.0
95.00	116912.0
96.10	7546.0
97.00	245.0
104.00	396.0
105.00	236.0
106.00	357.0
114.90	136.0
115.90	434.0
116.90	807.0
117.90	408.0
118.90	657.0
126.90	114.0
127.90	410.0
128.90	213.0
129.90	405.0
130.80	184.0
135.00	130.0
137.00	156.0
141.00	770.0
143.00	1391.0
144.90	692.0
145.90	204.0
147.90	288.0
148.90	106.0
150.00	144.0
155.00	209.0
156.90	157.0
158.90	134.0
160.70	112.0
171.00	302.0
172.00	1504.0
173.00	1170.0
174.00	101080.0
175.00	7260.0
176.00	97776.0
177.00	6110.0
178.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177