

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
 Data File : VU056789.D
 Acq On : 12 Dec 2023 16:32
 Operator : MD/SY
 Sample : 05664-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0Y41

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	110	rVB	130103	153149	14.66%	1.850%
2	1.727	130	136	145	rVB	10855	13163	1.26%	0.159%
3	1.907	184	192	207	rVB	96284	135553	12.98%	1.637%
4	2.563	383	396	412	rBV	217414	358003	34.27%	4.324%
5	3.181	572	588	609	rBV2	16556	39884	3.82%	0.482%
6	4.618	1017	1035	1076	rBV	141776	401727	38.46%	4.852%
7	5.055	1151	1171	1207	rVB	207766	468328	44.83%	5.657%
8	5.721	1357	1378	1407	rBV2	399712	1044625	100.00%	12.618%
9	6.245	1528	1541	1569	rBV	285054	563436	53.94%	6.806%
10	6.685	1665	1678	1710	rBV	246542	490456	46.95%	5.924%
11	7.560	1939	1950	1973	rBV	116976	215345	20.61%	2.601%
12	7.894	2040	2054	2071	rBV	455932	825107	78.99%	9.966%
13	7.965	2071	2076	2092	rVB2	17084	32218	3.08%	0.389%
14	8.177	2128	2142	2157	rBV	71660	127149	12.17%	1.536%
15	8.631	2271	2283	2321	rBV2	499852	984593	94.25%	11.893%
16	9.415	2514	2527	2558	rBV	394631	708215	67.80%	8.555%
17	10.749	2930	2942	2961	rBV	170887	283999	27.19%	3.430%
18	11.743	3243	3251	3259	rBV6	7895	12216	1.17%	0.148%
19	11.807	3259	3271	3292	rBV	375037	660023	63.18%	7.972%
20	12.064	3342	3351	3366	rBV4	10439	24733	2.37%	0.299%
21	12.187	3375	3389	3415	rBV	416153	736916	70.54%	8.901%




Sum of corrected areas: 8278838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056789.D
Acq On : 12 Dec 2023 16:32
Operator : MD/SY
Sample : 05664-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0Y41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

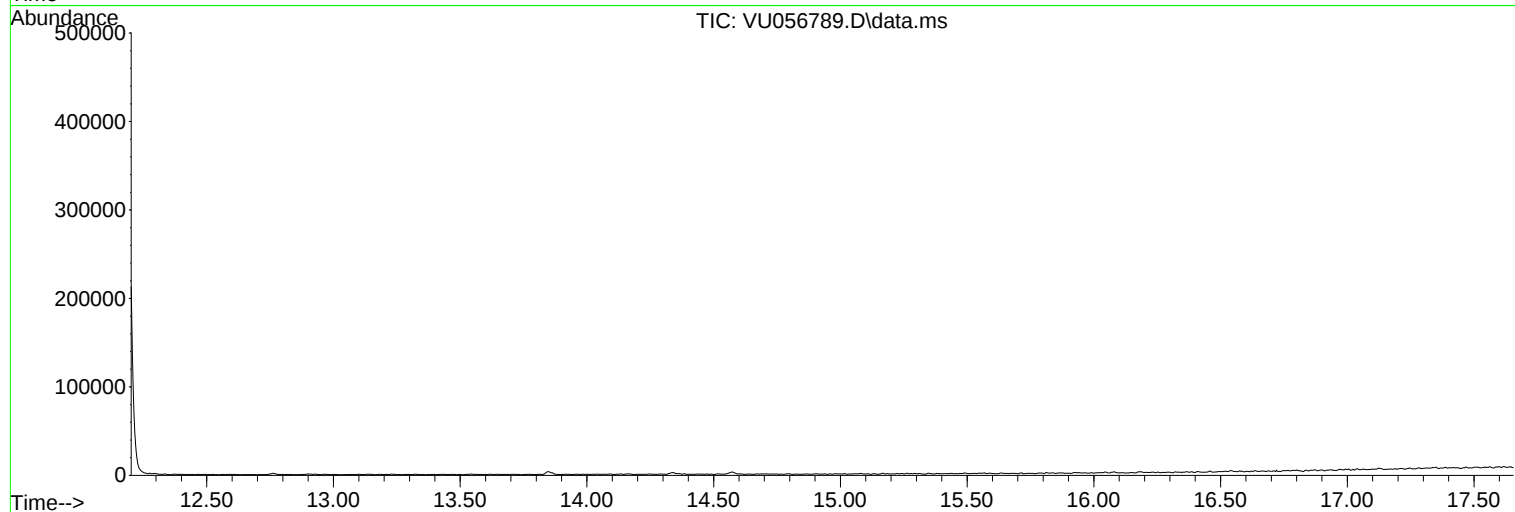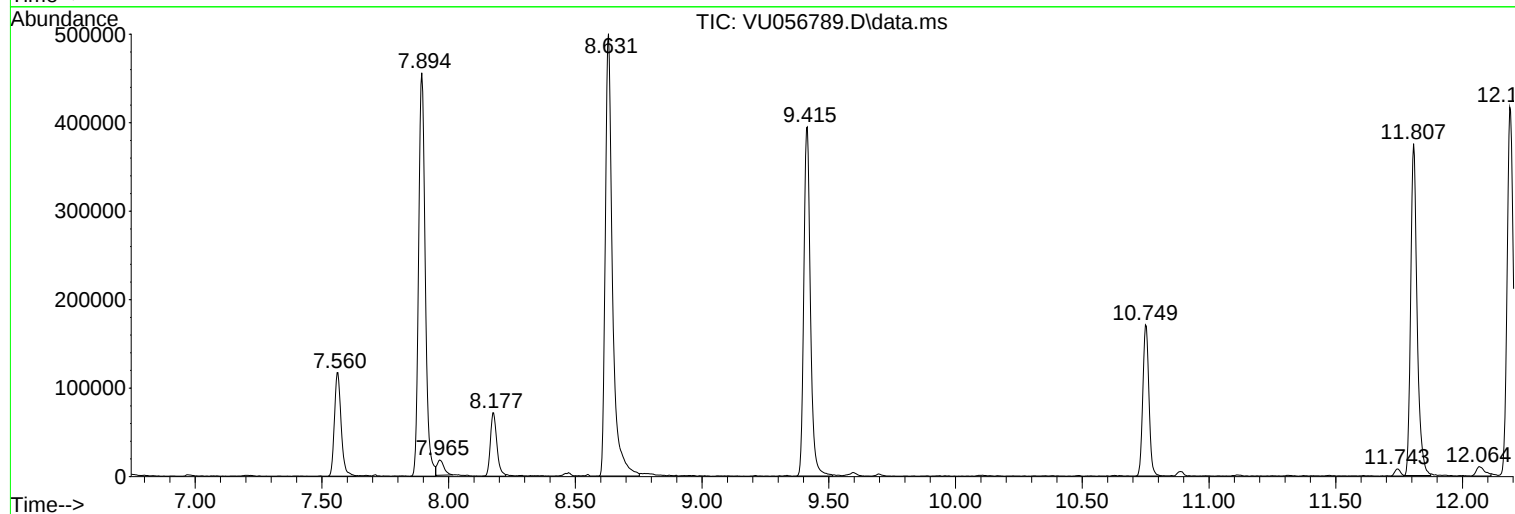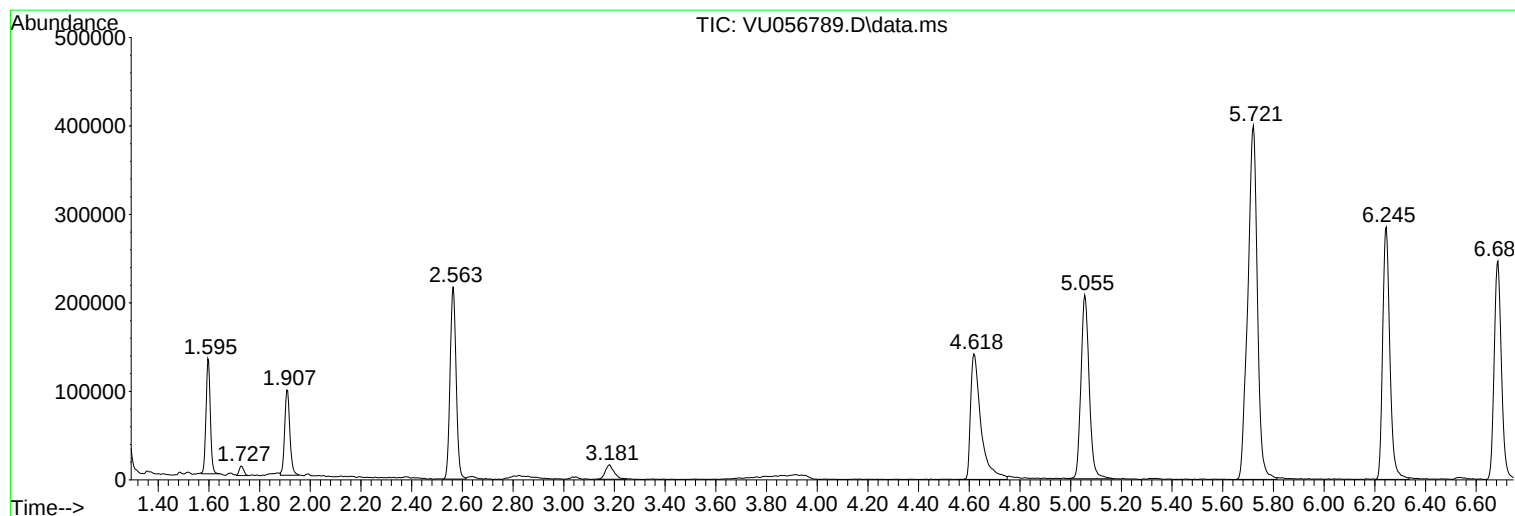

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056789.D
Acq On : 12 Dec 2023 16:32
Operator : MD/SY
Sample : 05664-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0Y41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056789.D
Acq On : 12 Dec 2023 16:32
Operator : MD/SY
Sample : 05664-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0Y41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc