

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
 Data File : VU056815.D
 Acq On : 13 Dec 2023 04:13
 Operator : MD/SY
 Sample : 05627-09DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCLC3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	119998	141419	12.60%	1.589%
2	1.908	183	192	211	rVB	99411	137777	12.28%	1.548%
3	2.564	384	396	411	rBV	198437	323194	28.80%	3.631%
4	3.043	531	545	557	rBV4	6543	13828	1.23%	0.155%
5	3.178	573	587	603	rBV2	16613	40727	3.63%	0.457%
6	4.615	1016	1034	1074	rBV	136527	375319	33.44%	4.216%
7	5.055	1154	1171	1203	rBV	197316	447153	39.85%	5.023%
8	5.721	1353	1378	1409	rBV2	378996	990184	88.23%	11.123%
9	6.245	1526	1541	1568	rBV	282903	550417	49.05%	6.183%
10	6.538	1617	1632	1657	rBV	581582	1122222	100.00%	12.606%
11	6.682	1664	1677	1707	rVB	236997	473900	42.23%	5.323%
12	7.560	1939	1950	1970	rBV	110876	203005	18.09%	2.280%
13	7.895	2041	2054	2079	rBV	431607	786090	70.05%	8.830%
14	8.174	2130	2141	2162	rBV2	68462	120331	10.72%	1.352%
15	8.628	2271	2282	2317	rBV2	486359	964684	85.96%	10.837%
16	9.412	2514	2526	2559	rBV	389226	695176	61.95%	7.809%
17	10.750	2931	2942	2965	rBV2	162087	270250	24.08%	3.036%
18	11.808	3259	3271	3293	rBV	365095	606706	54.06%	6.815%
19	12.187	3376	3389	3408	rBV	370152	639733	57.01%	7.186%




Sum of corrected areas: 8902115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056815.D
Acq On : 13 Dec 2023 04:13
Operator : MD/SY
Sample : 05627-09DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCLC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

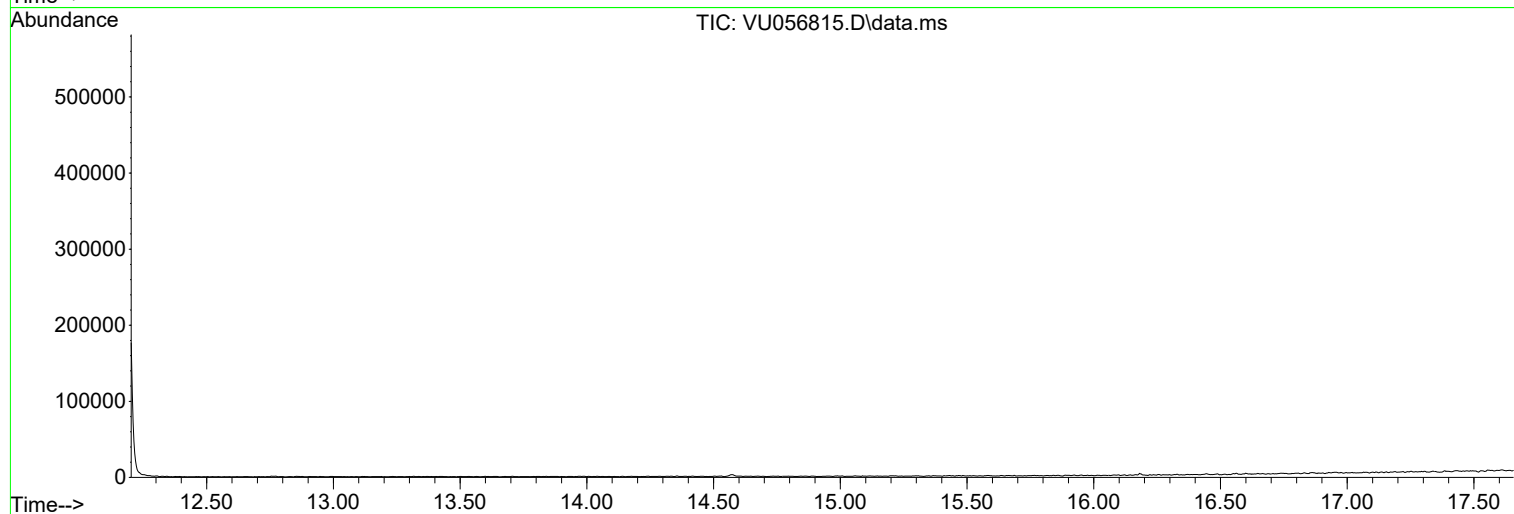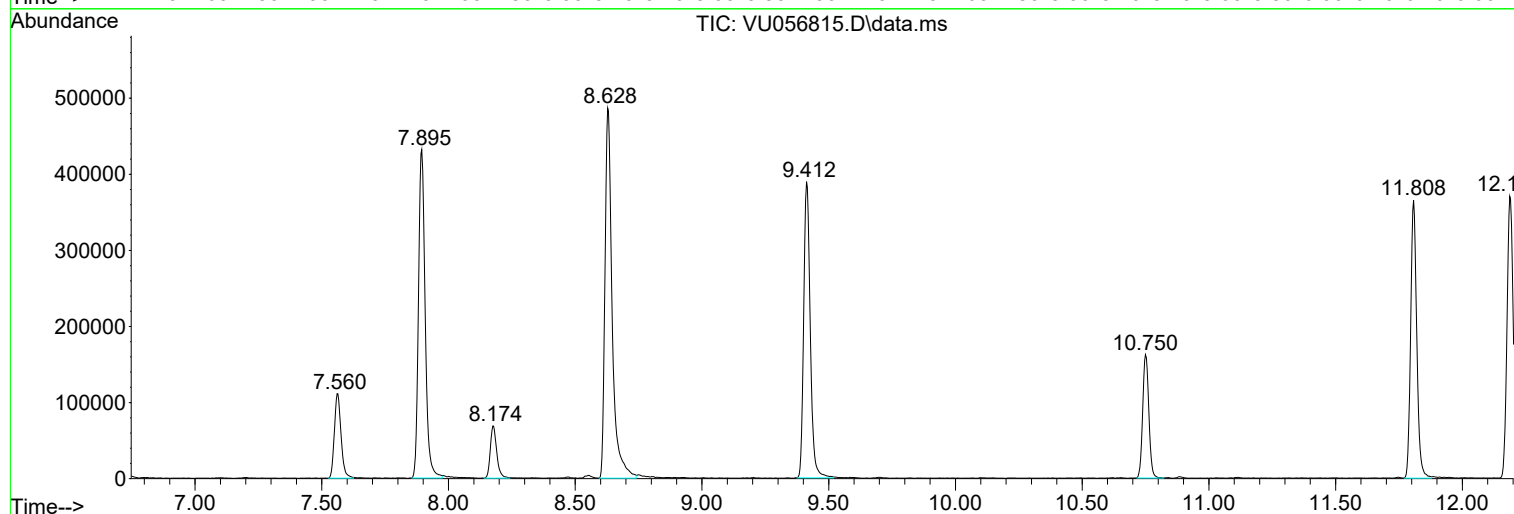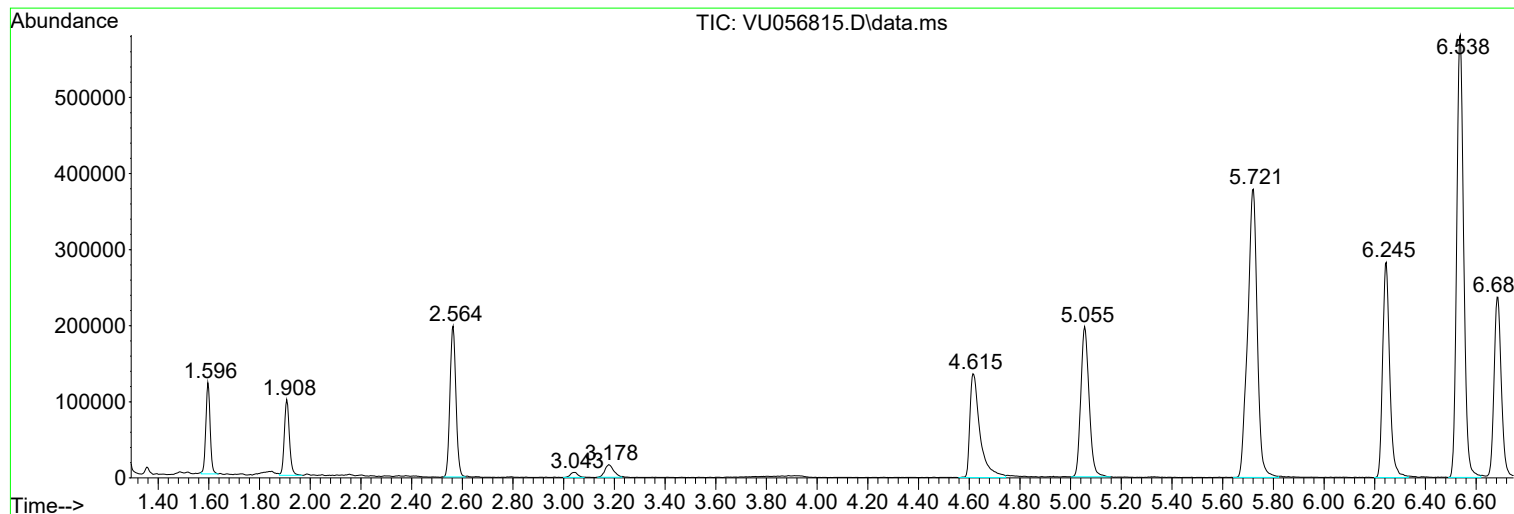

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056815.D
Acq On : 13 Dec 2023 04:13
Operator : MD/SY
Sample : 05627-09DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCLC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056815.D
Acq On : 13 Dec 2023 04:13
Operator : MD/SY
Sample : 05627-09DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCLC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc