

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
 Data File : VU056817.D
 Acq On : 13 Dec 2023 05:01
 Operator : MD/SY
 Sample : 05684-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E06H6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	109	rVB	119995	137896	14.17%	1.785%
2	1.907	183	192	205	rBV	101489	133578	13.73%	1.729%
3	2.563	384	396	409	rBV	201213	329256	33.84%	4.261%
4	4.615	1023	1034	1063	rBV	125791	334625	34.39%	4.331%
5	5.055	1152	1171	1205	rVB	194336	466582	47.95%	6.038%
6	5.515	1301	1314	1328	rVB4	4205	9926	1.02%	0.128%
7	5.721	1358	1378	1405	rBV3	366954	973078	100.00%	12.593%
8	6.245	1528	1541	1562	rBV	282606	555348	57.07%	7.187%
9	6.537	1623	1632	1647	rBV6	11693	24111	2.48%	0.312%
10	6.685	1662	1678	1699	rBV	230513	459054	47.18%	5.941%
11	7.560	1936	1950	1970	rBV	107525	197639	20.31%	2.558%
12	7.894	2038	2054	2074	rBV	418569	761692	78.28%	9.858%
13	8.177	2131	2142	2166	rVB	63027	115306	11.85%	1.492%
14	8.547	2247	2257	2269	rBV2	20367	34844	3.58%	0.451%
15	8.627	2271	2282	2314	rBV2	456392	900935	92.59%	11.660%
16	9.412	2512	2526	2568	rBV	398457	775480	79.69%	10.036%
17	10.749	2929	2942	2963	rBV	163811	270101	27.76%	3.496%
18	11.807	3259	3271	3298	rBV	361579	610758	62.77%	7.904%
19	12.187	3377	3389	3406	rBV	376831	636820	65.44%	8.241%




Sum of corrected areas: 7727029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056817.D
Acq On : 13 Dec 2023 05:01
Operator : MD/SY
Sample : 05684-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E06H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

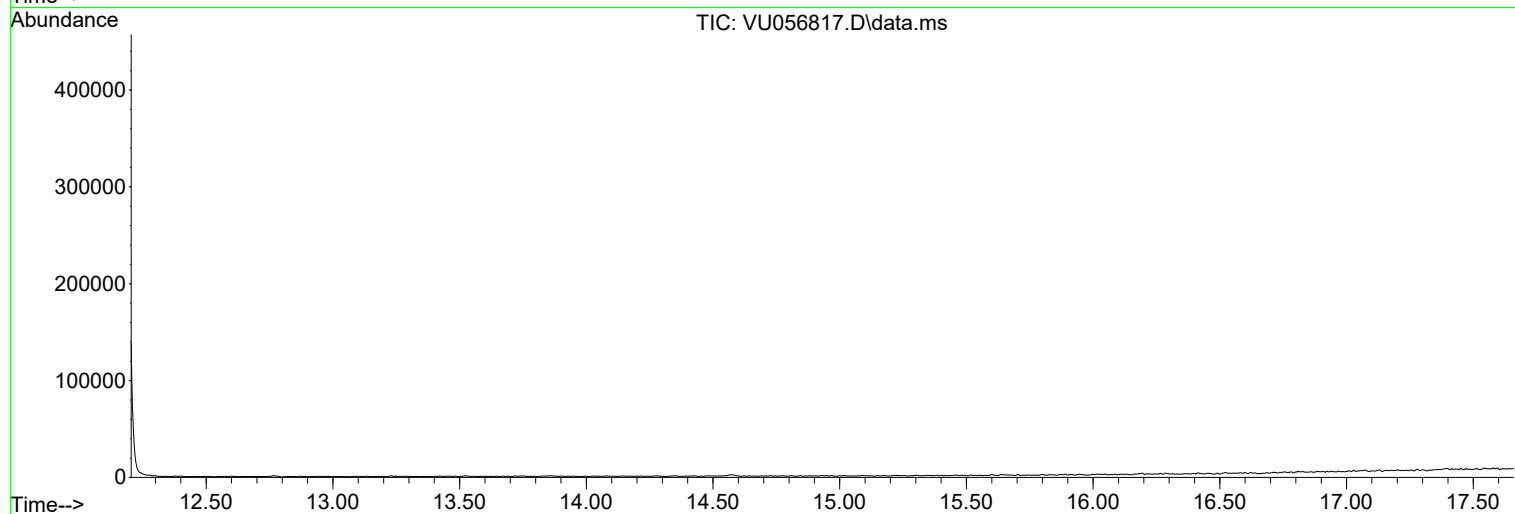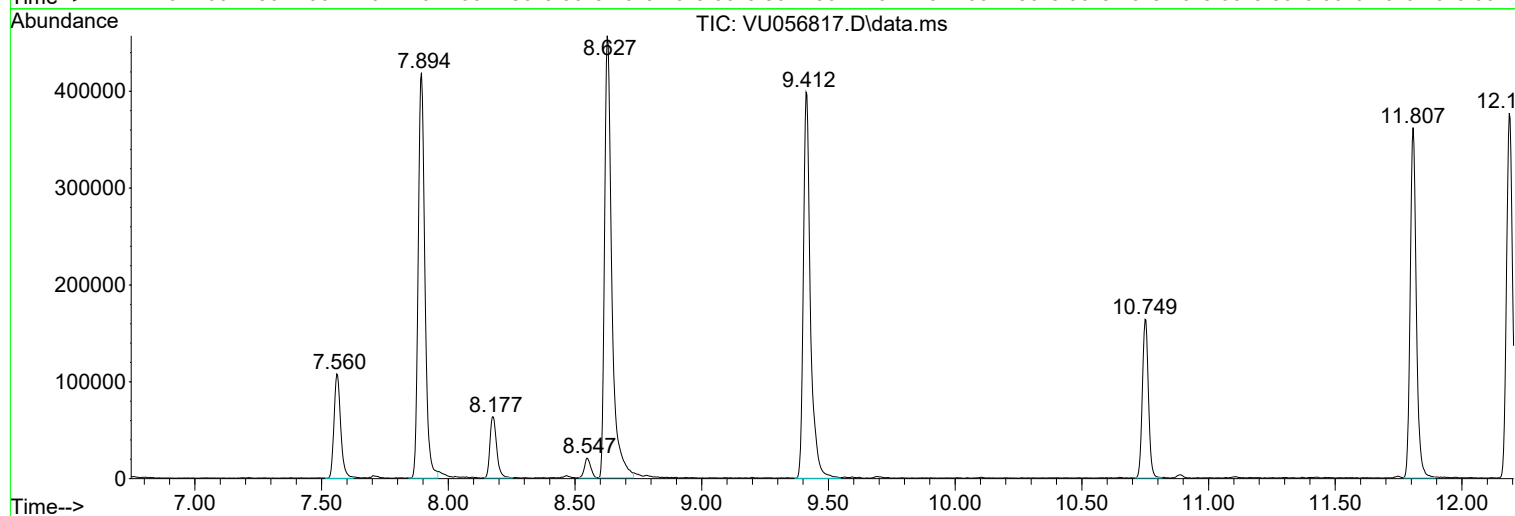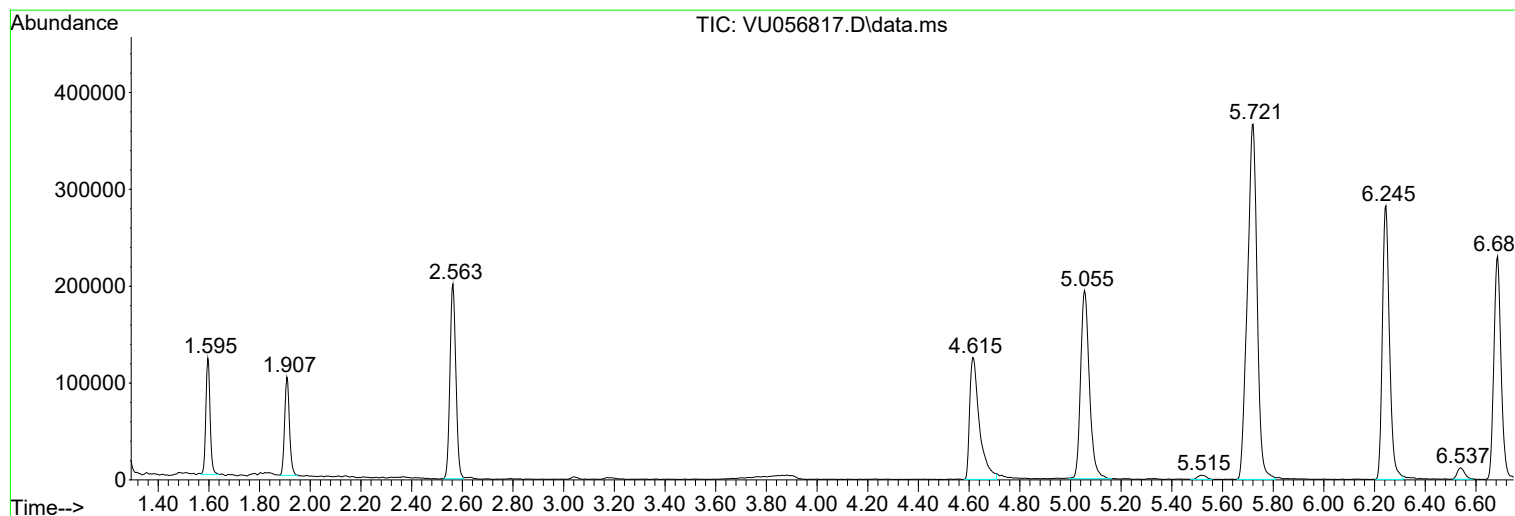

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056817.D
Acq On : 13 Dec 2023 05:01
Operator : MD/SY
Sample : 05684-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E06H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056817.D
Acq On : 13 Dec 2023 05:01
Operator : MD/SY
Sample : 05684-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E06H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc