

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
 Data File : VU056819.D
 Acq On : 13 Dec 2023 05:50
 Operator : MD/SY
 Sample : 05684-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E06H9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	106	rVB	124763	141888	9.06%	1.391%
2	1.907	184	192	207	rVB	100663	136193	8.69%	1.335%
3	2.563	382	396	406	rBV	205338	336977	21.51%	3.303%
4	2.624	406	415	436	rVB	94333	185565	11.84%	1.819%
5	2.788	451	466	468	rBV2	12193	21015	1.34%	0.206%
6	4.618	1024	1035	1061	rBV	127461	343926	21.95%	3.372%
7	5.055	1151	1171	1202	rBV	215992	503801	32.16%	4.939%
8	5.721	1357	1378	1412	rBV3	383977	999779	63.81%	9.801%
9	6.245	1528	1541	1566	rBV	303793	591218	37.74%	5.796%
10	6.685	1662	1678	1696	rBV	237569	467608	29.85%	4.584%
11	7.563	1936	1951	1973	rBV	109901	203188	12.97%	1.992%
12	7.894	2041	2054	2072	rBV	439429	785521	50.14%	7.701%
13	8.177	2131	2142	2163	rBV2	67666	119650	7.64%	1.173%
14	8.550	2248	2258	2271	rVB2	31596	53465	3.41%	0.524%
15	8.630	2271	2283	2317	rBV2	479237	937438	59.83%	9.190%
16	9.412	2514	2526	2558	rBV	424899	787828	50.28%	7.723%
17	10.749	2929	2942	2962	rBV	169563	277220	17.69%	2.718%
18	11.740	3237	3250	3260	rBV2	132509	216790	13.84%	2.125%
19	11.830	3260	3278	3313	rVB2	576672	1525014	97.34%	14.950%
20	12.203	3376	3394	3417	rBV2	638937	1566740	100.00%	15.359%




Sum of corrected areas: 10200824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056819.D
Acq On : 13 Dec 2023 05:50
Operator : MD/SY
Sample : 05684-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E06H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

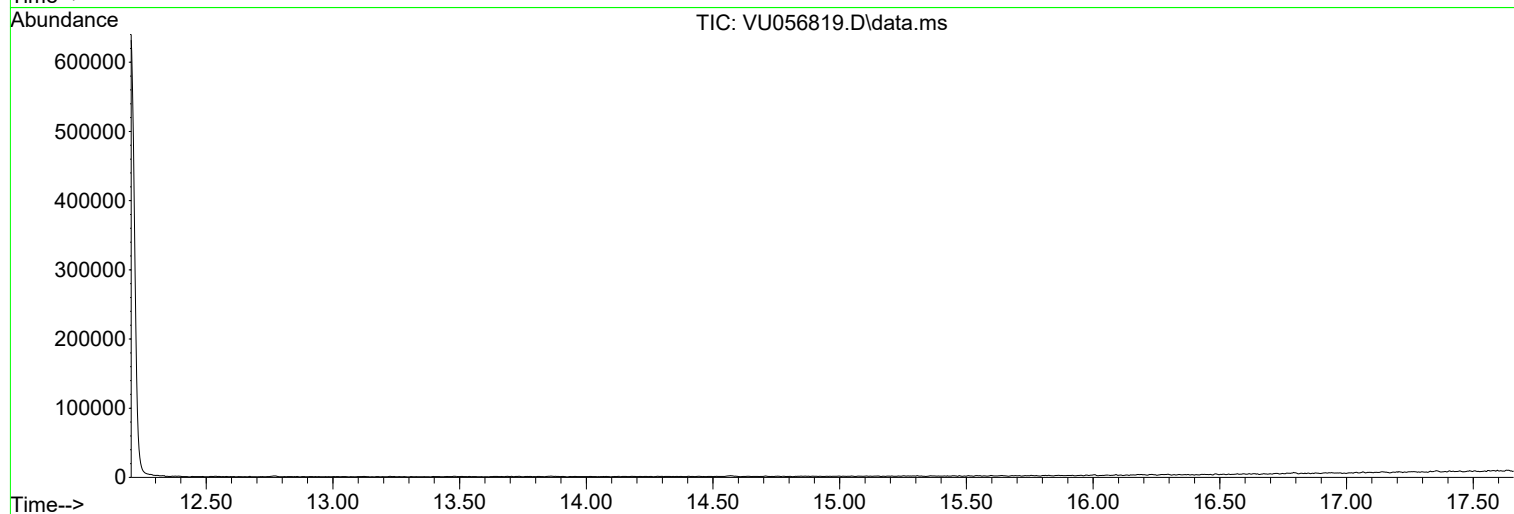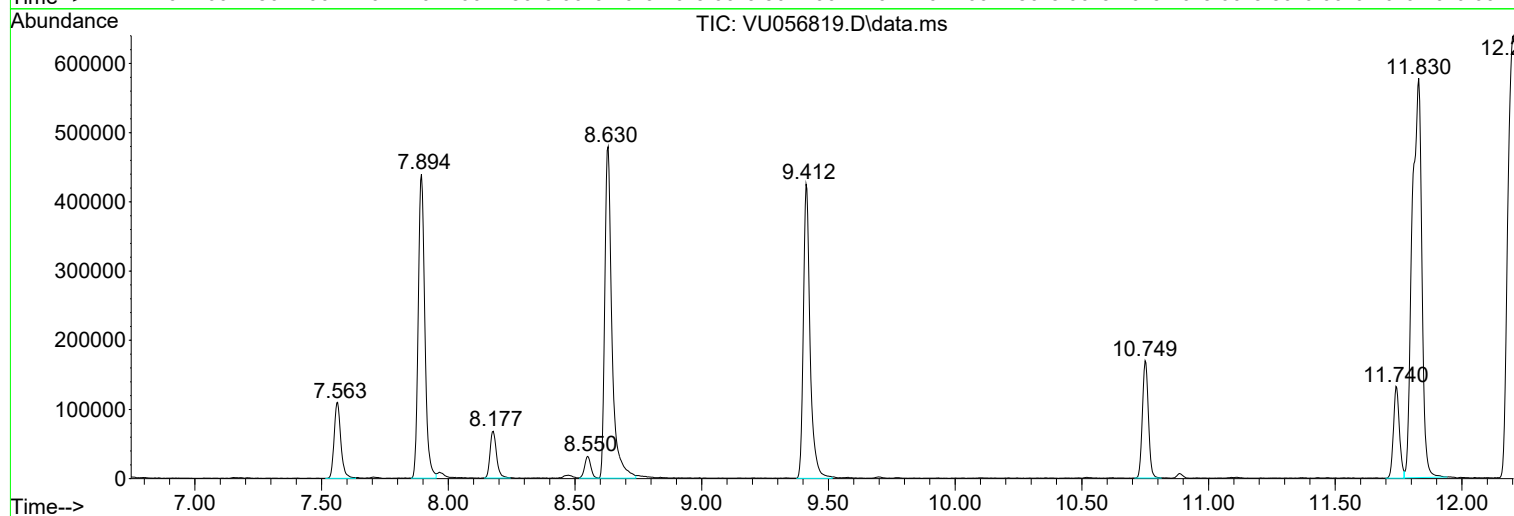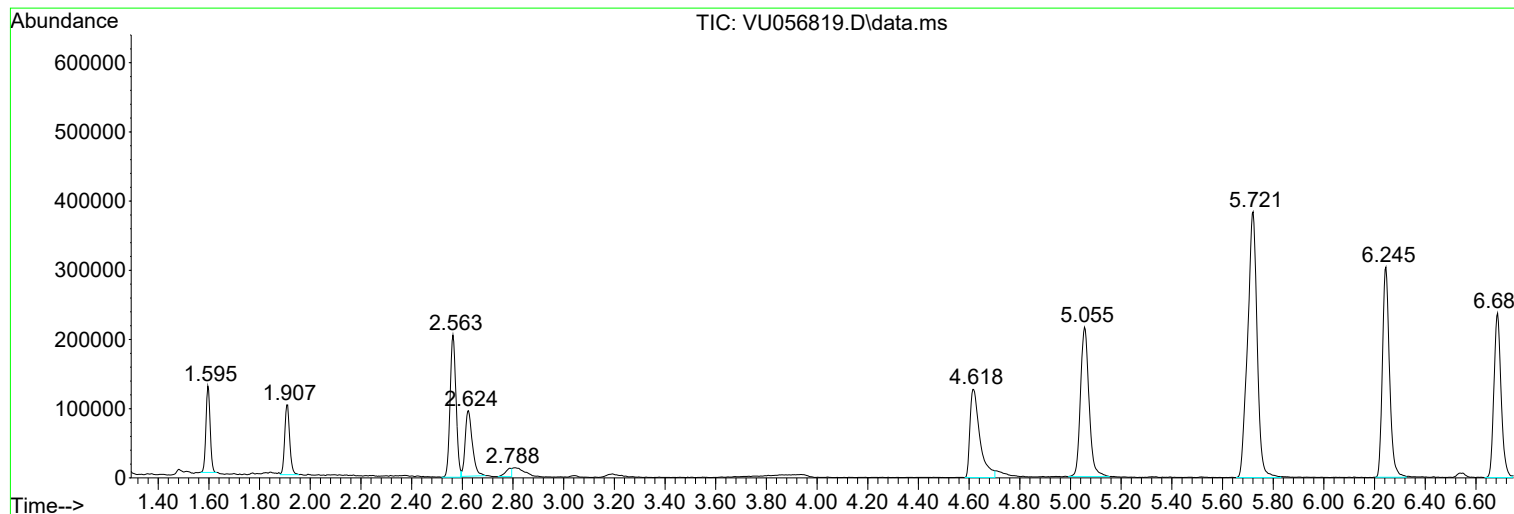

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056819.D
Acq On : 13 Dec 2023 05:50
Operator : MD/SY
Sample : 05684-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E06H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056819.D
Acq On : 13 Dec 2023 05:50
Operator : MD/SY
Sample : 05684-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E06H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc