
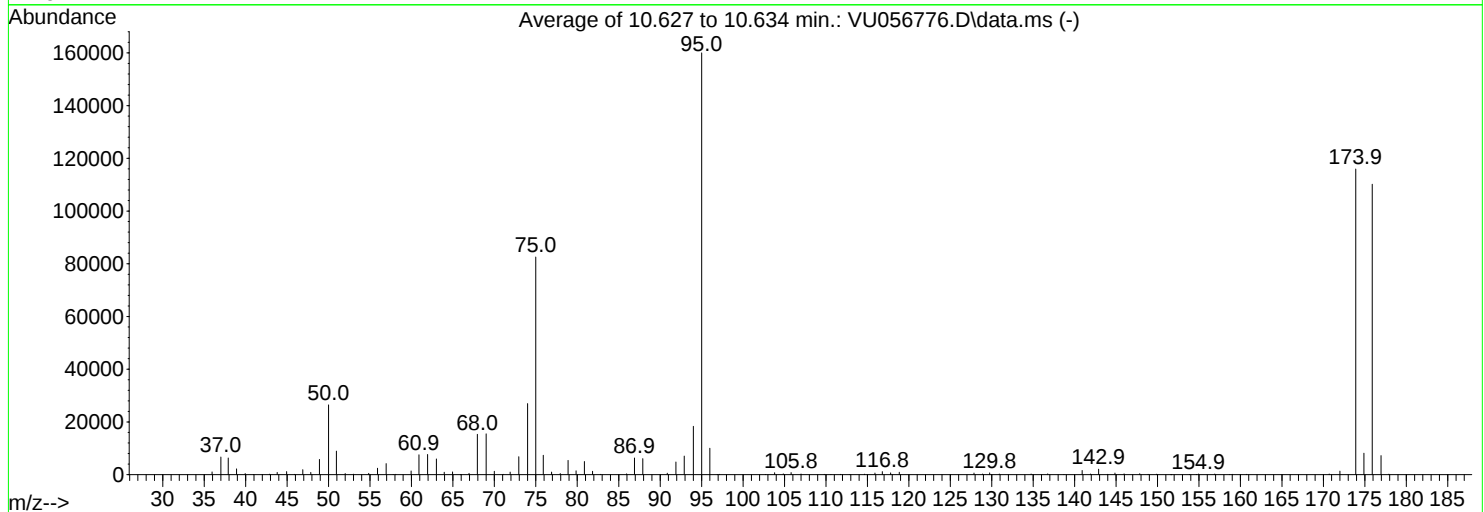


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121223\
Data File : VU056776.D
Acq On : 12 Dec 2023 10:07
Operator : MD/SY
Sample : BFB091
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB091

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 13 01:32:29 2023

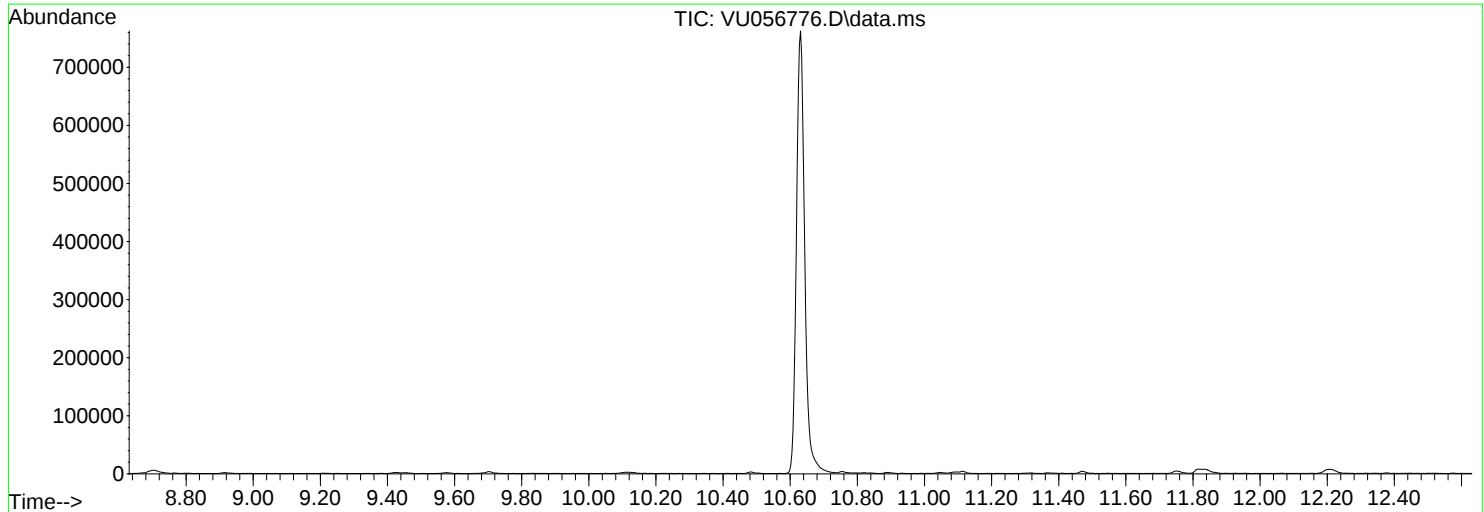

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	26467	PASS
75	95	30	80	51.6	82552	PASS
95	95	100	100	100.0	160021	PASS
96	95	5	9	6.3	10036	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	115915	PASS
175	174	5	9	7.0	8149	PASS
176	174	95	101	95.1	110187	PASS
177	176	5	9	6.6	7247	PASS

m/z	Abundance
39.70	253.0
42.90	150.0
43.80	279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
35.90	1165.0
37.00	6614.0
37.90	6410.0
38.90	2109.0
39.90	473.0
42.90	293.0
43.80	1169.0
44.90	1114.0
46.00	133.0
46.90	2070.0
47.80	978.0
48.90	5741.0
50.00	26728.0
51.00	9198.0
52.00	493.0
52.90	154.0
54.80	482.0
55.90	2298.0
57.00	3997.0
57.80	226.0
60.00	1439.0
60.90	8070.0
62.00	7533.0
63.00	6139.0
63.90	991.0
65.00	1057.0
65.90	104.0
66.90	494.0
68.00	15280.0
69.00	15487.0
70.00	1270.0
71.10	144.0
71.90	1033.0
73.00	6908.0
74.00	27848.0
75.00	83072.0
75.90	6994.0
76.90	866.0
77.90	599.0
78.90	5558.0
79.90	1322.0
80.90	5232.0
81.90	1375.0
82.80	105.0
86.00	324.0
86.90	6557.0
87.90	5910.0
90.90	602.0
91.90	4911.0
92.90	7024.0
94.00	18440.0
95.00	159808.0
96.00	10284.0
96.90	257.0
103.80	761.0
105.00	315.0
105.90	894.0
107.00	179.0
109.80	154.0
110.60	171.0
112.90	167.0
114.60	150.0
115.90	644.0
116.80	1209.0
117.80	627.0
118.90	927.0
127.80	511.0
128.80	287.0
129.80	663.0
130.80	178.0
134.80	287.0
136.80	308.0
138.70	128.0
140.90	1646.0
141.90	164.0
142.90	2174.0
144.00	185.0
144.90	614.0
145.90	331.0
147.90	354.0
148.90	142.0
149.90	153.0
153.90	129.0
154.70	241.0
154.90	233.0
156.90	258.0
159.00	249.0
160.70	117.0
170.60	288.0
172.00	1232.0
173.90	113800.0
174.90	8162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

175.90108344.0

177.007408.0

177.90170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
35.90	1102.0
37.00	6888.0
37.90	6614.0
38.90	2267.0
40.00	453.0
40.90	103.0
42.00	126.0
42.90	318.0
43.90	1125.0
44.90	1236.0
45.90	133.0
46.90	2018.0
47.90	877.0
48.90	5915.0
50.00	27208.0
50.90	9213.0
52.00	414.0
53.00	182.0
54.90	490.0
55.90	2508.0
57.00	4291.0
58.10	181.0
59.90	1448.0
60.90	7766.0
61.90	7915.0
63.00	6108.0
63.90	951.0
65.00	1066.0
67.00	518.0
68.00	15706.0
69.00	15969.0
70.00	1284.0
71.00	154.0
71.90	1008.0
72.90	6995.0
74.00	27808.0
75.00	84688.0
75.90	7563.0
76.90	1002.0
78.00	657.0
78.90	5551.0
79.90	1478.0
80.80	5064.0
81.90	1277.0
82.80	117.0
85.90	283.0
86.90	6490.0
87.90	6278.0
90.90	546.0
91.90	4855.0
92.90	7293.0
94.00	18880.0
95.00	164544.0
96.00	10375.0
97.20	254.0
102.70	127.0
103.80	744.0
104.80	313.0
105.80	779.0
107.00	237.0
109.80	159.0
110.60	104.0
111.70	133.0
114.60	182.0
115.90	610.0
116.80	1128.0
117.80	731.0
118.90	929.0
127.90	657.0
128.90	247.0
129.80	665.0
130.90	219.0
134.70	264.0
136.80	298.0
138.70	104.0
140.90	1663.0
141.90	289.0
142.90	2144.0
144.00	153.0
144.90	632.0
145.90	308.0
147.90	373.0
148.80	144.0
149.90	166.0
151.60	108.0
153.80	107.0
154.90	293.0
156.90	284.0
159.00	206.0
160.80	139.0
170.70	255.0
172.00	1432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

173.90	119832.0
174.90	8382.0
175.90	113656.0
177.00	7409.0
177.90	204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
36.00	927.0
37.00	6569.0
37.90	5913.0
38.90	2292.0
40.00	457.0
41.00	111.0
42.00	115.0
42.90	322.0
43.90	1084.0
45.00	1189.0
45.80	141.0
46.90	1642.0
47.90	746.0
48.90	5594.0
50.00	25464.0
50.90	8439.0
52.00	344.0
53.10	206.0
54.90	436.0
55.90	2418.0
56.90	4210.0
58.10	139.0
59.90	1384.0
60.90	6798.0
61.90	7526.0
63.00	5615.0
64.00	803.0
64.90	949.0
67.00	475.0
67.90	14834.0
69.00	15045.0
70.00	1220.0
71.00	146.0
71.90	973.0
72.90	6492.0
74.00	25264.0
75.00	79896.0
75.90	7504.0
76.90	1133.0
78.90	5155.0
79.80	1567.0
80.80	4611.0
81.80	1144.0
82.80	149.0
85.90	265.0
86.90	5874.0
87.90	5970.0
90.70	516.0
91.90	4606.0
92.90	6881.0
94.00	17672.0
95.00	155712.0
96.00	9449.0
97.10	210.0
102.70	121.0
103.80	743.0
104.80	350.0
105.70	662.0
107.00	251.0
109.80	120.0
111.80	168.0
114.70	177.0
115.90	580.0
116.80	1050.0
117.80	709.0
118.80	852.0
127.90	705.0
129.00	231.0
129.70	663.0
131.00	279.0
134.70	227.0
136.70	296.0
140.90	1499.0
141.90	311.0
142.90	1829.0
144.80	555.0
146.00	241.0
147.80	342.0
148.80	134.0
149.90	188.0
155.00	296.0
156.90	281.0
158.70	161.0
160.80	111.0
170.80	228.0
172.00	1421.0
173.90	114112.0
174.90	7903.0
175.90	108560.0
176.90	6924.0
177.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091