

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121318\
 Data File : VU028642.D
 Acq On : 12 Dec 2018 11:08
 Operator : MD/SY
 Sample : J6357-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB.2018.12.11

Quant Time: Dec 13 03:01:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 07 00:39:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	113278	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	203668	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	183865	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	72880	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	87157	50.42	ug/l	0.00
Spiked Amount						
			Recovery	=	100.84%	
35) Dibromofluoromethane	4.88	113	66599	51.96	ug/l	0.00
Spiked Amount						
			Recovery	=	103.92%	
50) Toluene-d8	7.56	98	255017	50.30	ug/l	0.00
Spiked Amount						
			Recovery	=	100.60%	
62) 4-Bromofluorobenzene	10.31	95	86845	45.83	ug/l	0.00
Spiked Amount						
			Recovery	=	91.66%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121318\
Data File : VU028642.D
Acq On : 12 Dec 2018 11:08
Operator : MD/SY
Sample : J6357-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB.2018.12.11

Quant Time: Dec 13 03:01:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 07 00:39:42 2018
Response via : Initial Calibration

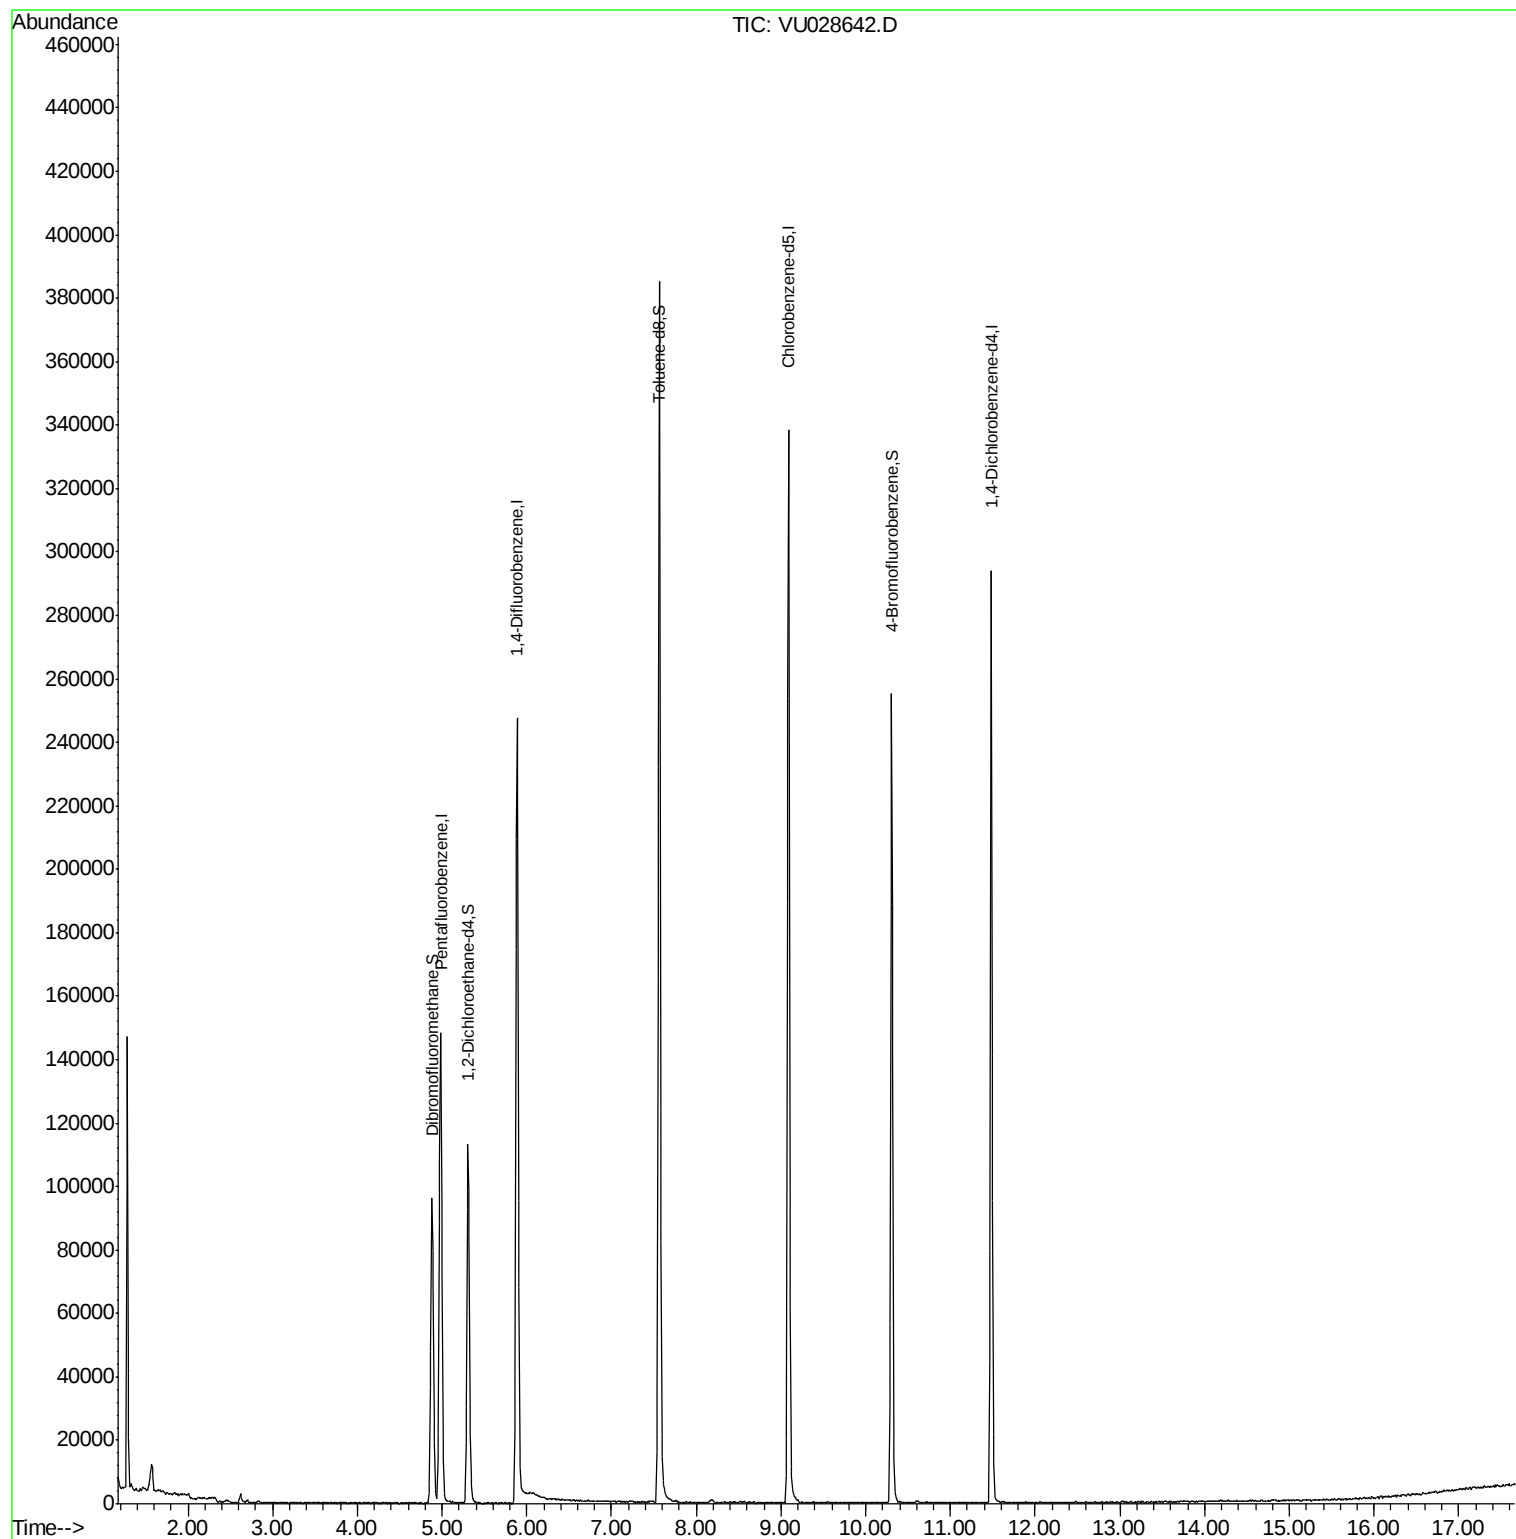



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1185

Delta R.T. 0.00 min

Lab File: VU028642.D

Acq: 12 Dec 2018 11:08

Instrument :

MSVOA_U

ClientSampleId :


TB.2018.12.11

Tot Ion:168 Resp: 113278

Ion Ratio Lower Upper

168 100

99 58.7 46.6 69.8

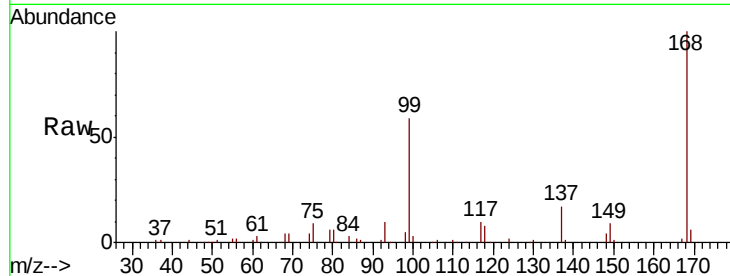

Abundance Ion 167.90 (167.60 to 168.60): VU028495.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028495.D (-1168) (-)

4.98

50000

40000

30000



20000

10000

0

4.90 5.00 5.10

Time-->

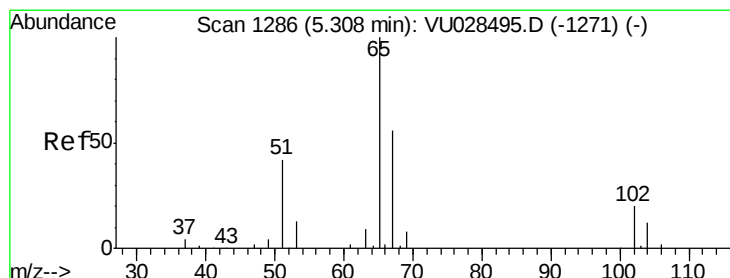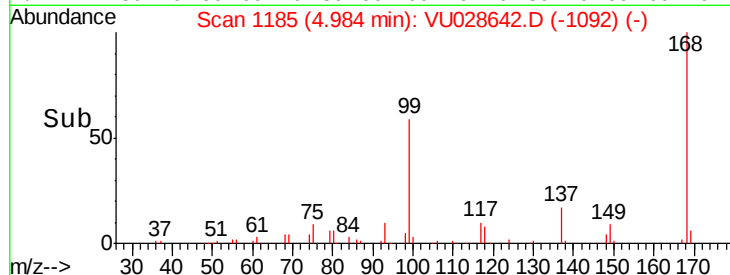

#33

1,2-Dichloroethane-d4

Concen: 50.418 ug/l

RT: 5.31 min Scan# 1286

Delta R.T. 0.00 min

Lab File: VU028642.D


Acq: 12 Dec 2018 11:08

Tgt Ion: 65 Resp: 87157

Ion Ratio Lower Upper

65 100

67 54.5 0.0 110.6

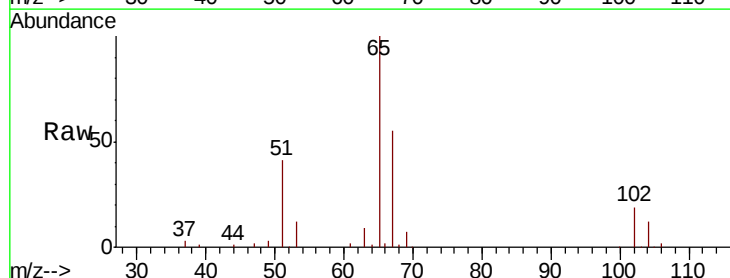

Abundance Ion 64.90 (64.60 to 65.60): VU028495.D (-1271) (-)

Ion 66.90 (66.60 to 67.60): VU028495.D (-1271) (-)

5.31

40000

30000


20000


10000

0

5.20 5.25 5.30 5.35 5.40

Time-->

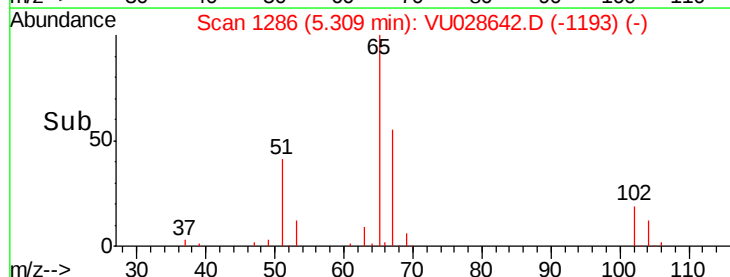


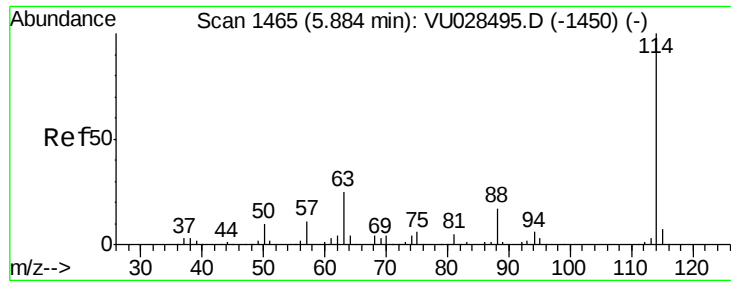




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. 0.00 min
 Lab File: VU028642.D
 Acq: 12 Dec 2018 11:08

Instrument :
 MSVOA_U
 ClientSampleId :
 TB.2018.12.11

Tot Ion:	114	Resp:	203668
Ion	Ratio	Lower	Upper
114	100		
63	24.2	0.0	49.2
88	16.9	0.0	33.4

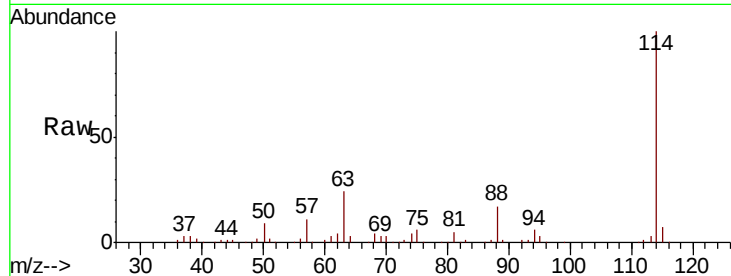


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

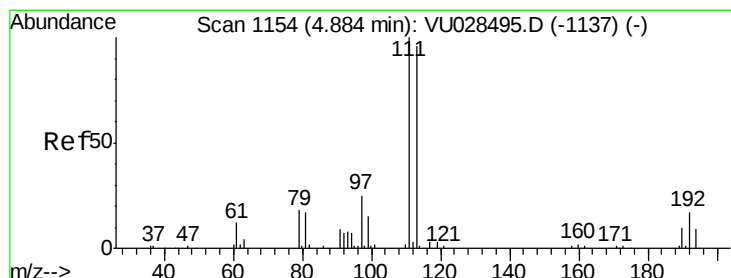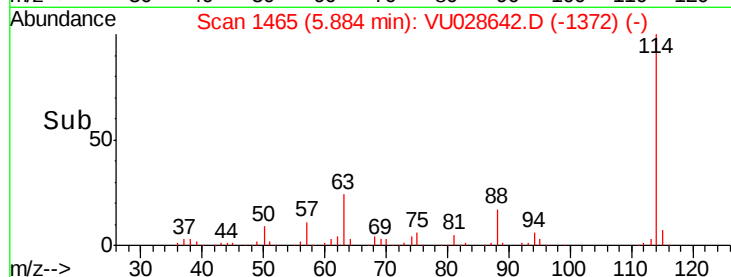
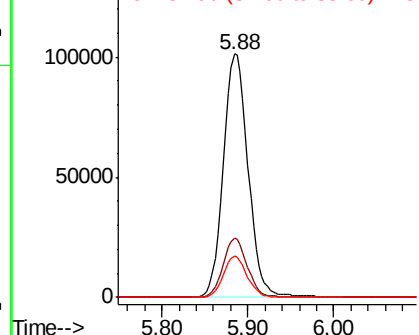



#35
 Dibromofluoromethane
 Concen: 51.962 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. -0.00 min
 Lab File: VU028642.D
 Acq: 12 Dec 2018 11:08

Tgt Ion:	113	Resp:	66599
Ion	Ratio	Lower	Upper
113	100		
111	104.1	83.4	125.0
192	19.9	14.8	22.2

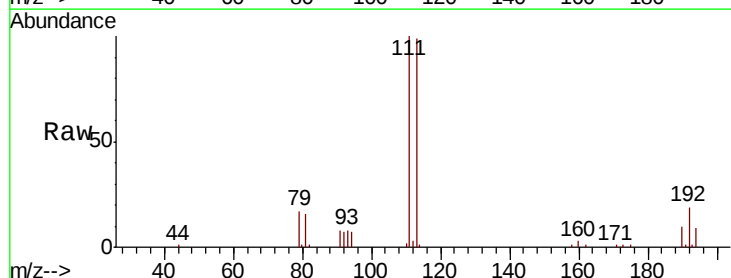

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



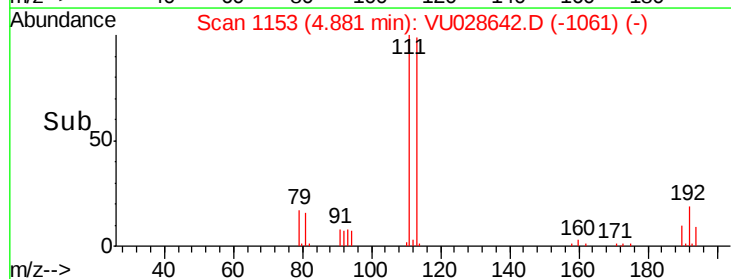
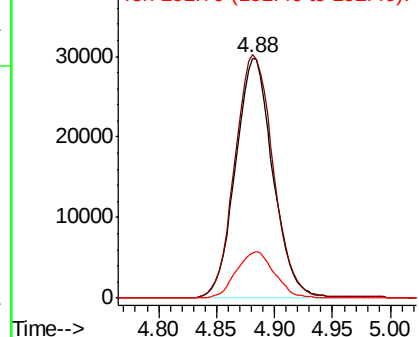


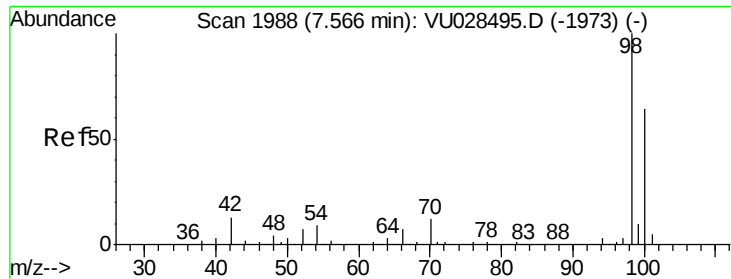

#50
Toluene-d8
Concen: 50.298 ug/l
RT: 7.56 min Scan# 1987
Delta R.T. -0.00 min
Lab File: VU028642.D
Acq: 12 Dec 2018 11:08




Instrument :
MSVOA_U
ClientSampleId :
TB.2018.12.11


Tot Ion: 98 Resp: 255017
Ion Ratio Lower Upper
98 100
100 64.2 51.0 76.6

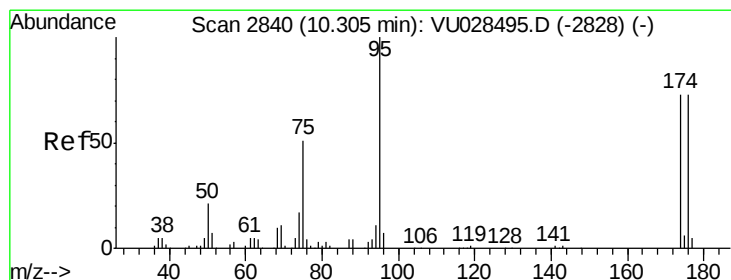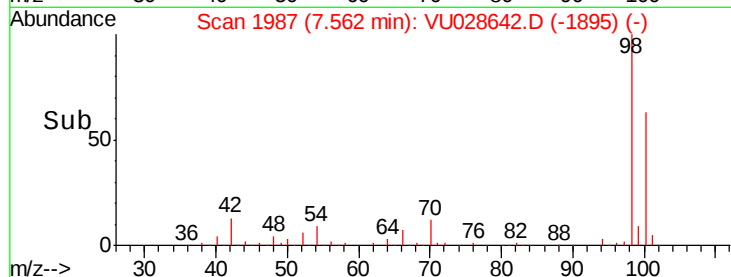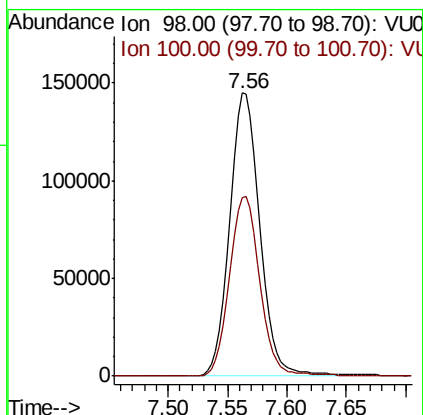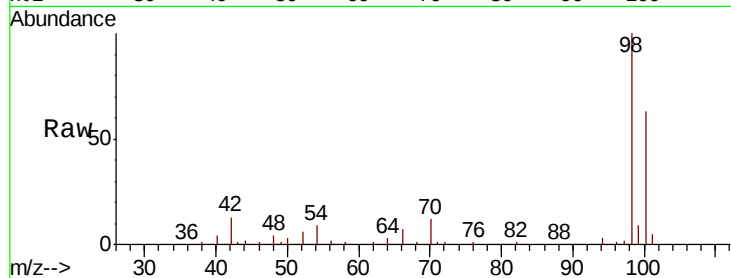

#62
4-Bromofluorobenzene
Concen: 45.827 ug/l
RT: 10.31 min Scan# 2840
Delta R.T. 0.00 min
Lab File: VU028642.D
Acq: 12 Dec 2018 11:08

Tgt Ion: 95 Resp: 86845
Ion Ratio Lower Upper
95 100
174 76.5 0.0 150.4
176 74.4 0.0 145.2

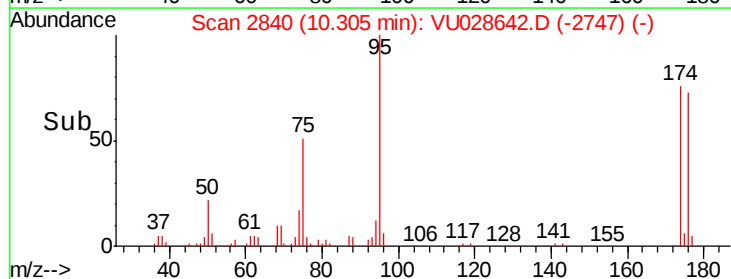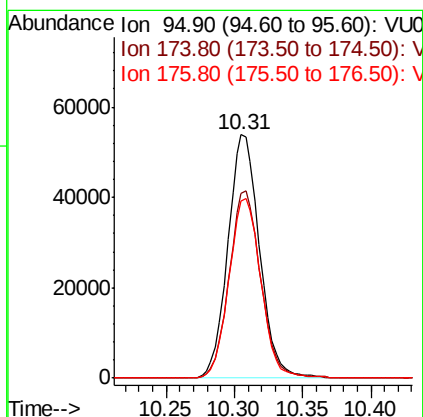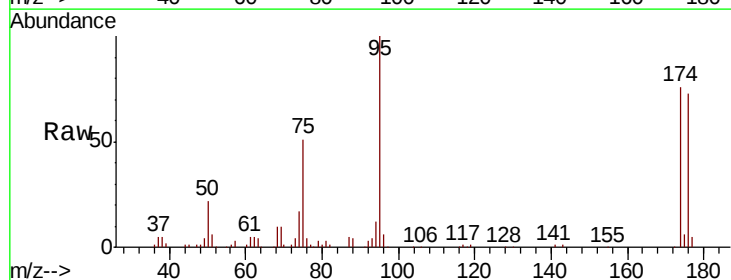


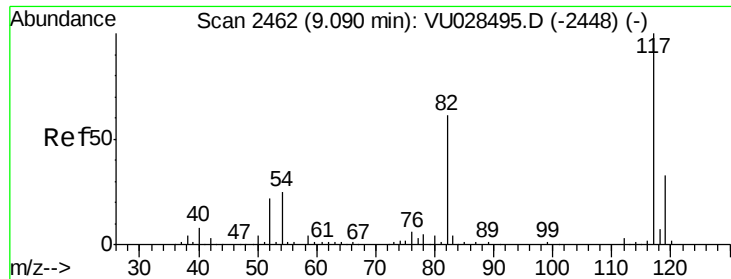




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. 0.00 min
Lab File: VU028642.D
Acq: 12 Dec 2018 11:08

Instrument :
MSVOA_U
ClientSampleId :
TB.2018.12.11

Tot Ion	Ratio	Lower	Upper
117	100		
82	59.1	48.9	73.3
119	32.0	26.2	39.4

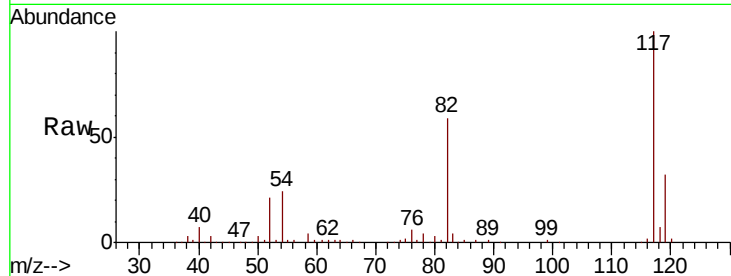


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

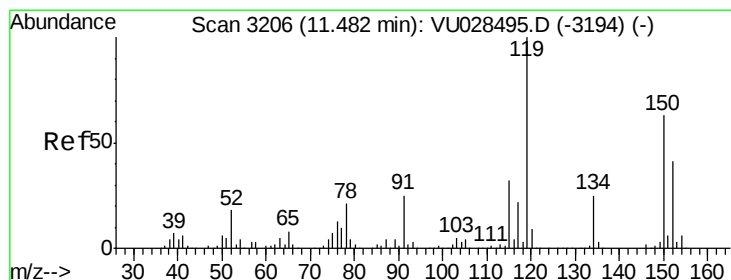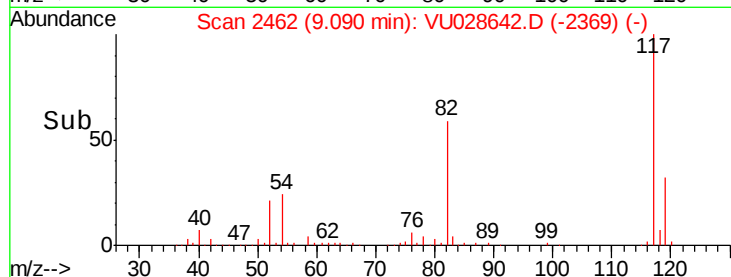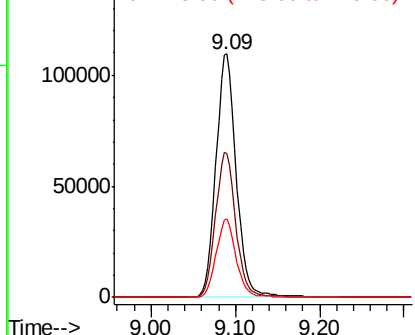

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3206
Delta R.T. 0.00 min
Lab File: VU028642.D
Acq: 12 Dec 2018 11:08

Tgt Ion	Ratio	Lower	Upper
152	100		
115	59.9	42.7	128.1
150	157.0	0.0	346.0

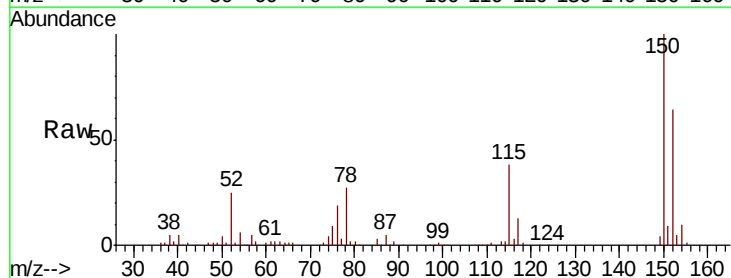

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

