


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121318\
Data File : VU028636.D
Acq On : 12 Dec 2018 08:29
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Title : SW846 8260
Last Update : Fri Dec 07 00:39:42 2018

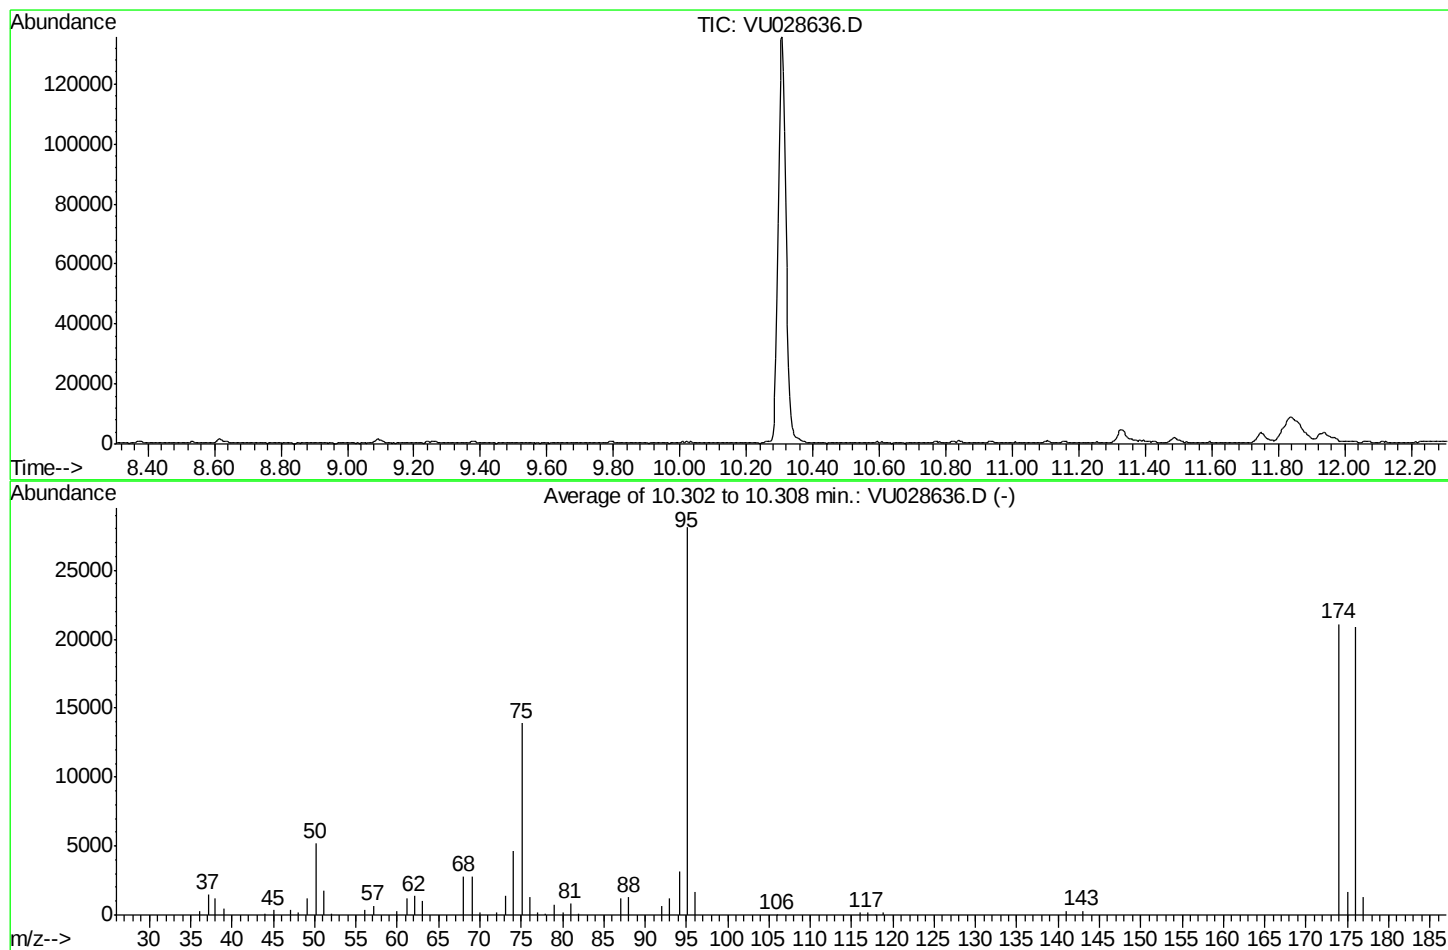

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5177	PASS
75	95	30	60	49.4	13887	PASS
95	95	100	100	100.0	28114	PASS
96	95	5	9	5.8	1635	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.0	21088	PASS
175	174	5	9	8.0	1693	PASS
176	174	95	101	99.0	20877	PASS
177	176	5	9	6.0	1263	PASS