

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U121319\
 Data File : VU036216.D
 Acq On : 13 Dec 2019 23:18
 Operator : JC/MD
 Sample : K6240-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQS3

Quant Time: Dec 14 04:12:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 14 01:19:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	227286	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	248020	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	94445	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	95414	4.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.40%
7) Chloroethane-d5	1.93	69	90588	5.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.00%
11) 1,1-Dichloroethene-d2	2.59	63	97171	3.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.40%
20) 2-Butanone-d5	4.70	46	200574	53.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.98%
24) Chloroform-d	5.11	84	160180	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.75	65	87747	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.77	84	291820	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.73	67	96757	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.93	98	234074	3.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.80%
43) trans-1,3-Dichloropropene-	8.21	79	35164	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.68	63	153983	49.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.64%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	90337	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.60%
64) 1,2-Dichlorobenzene-d4	12.22	152	97287	5.38	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.60%


Target Compounds					Ovalue
13) Acetone	2.68	43	6135	1.877 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121319\
Data File : VU036216.D
Acq On : 13 Dec 2019 23:18
Operator : JC/MD
Sample : K6240-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQS3

Quant Time: Dec 14 04:12:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 14 01:19:01 2019
Response via : Initial Calibration

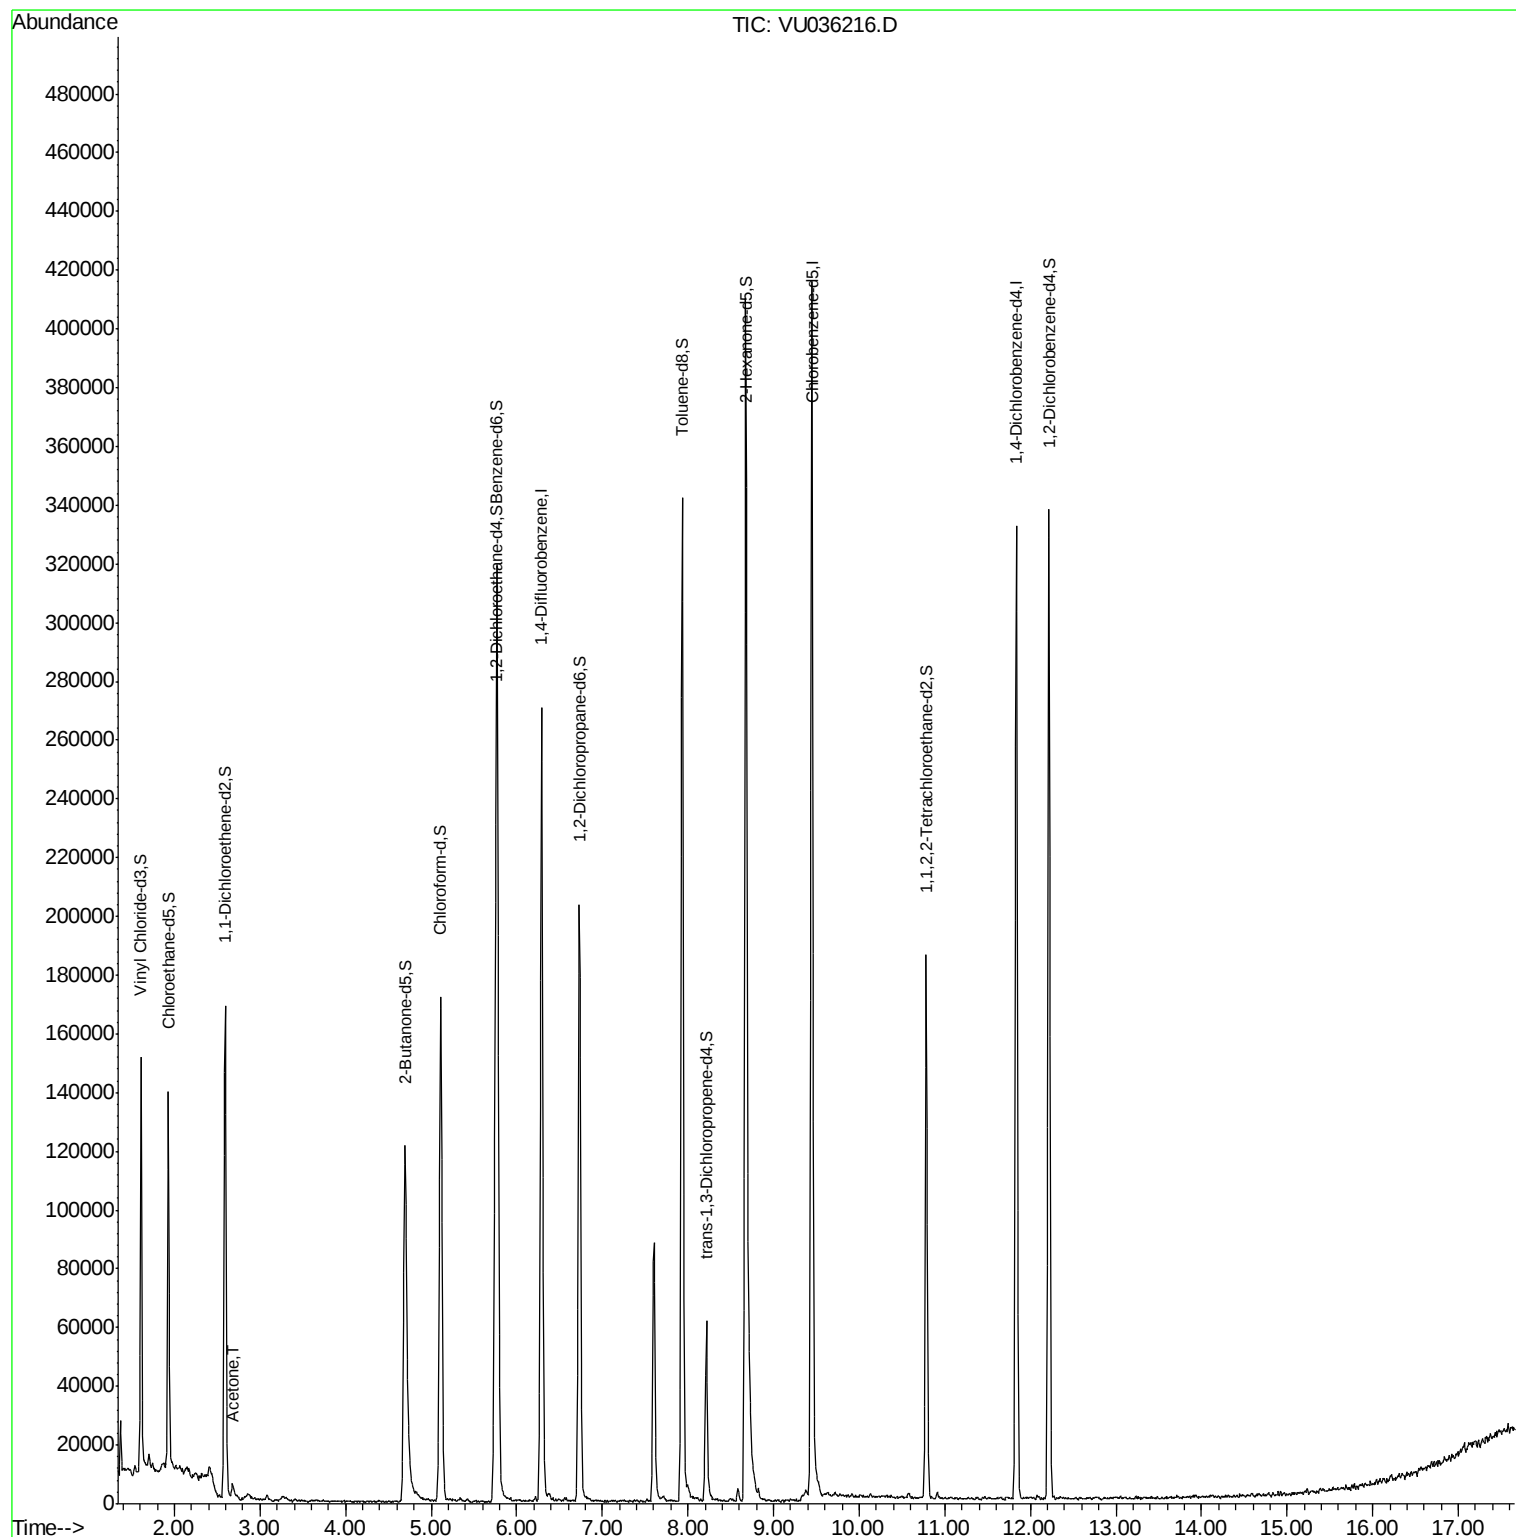

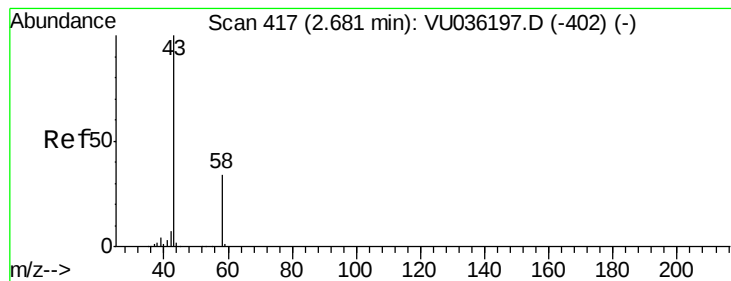

#13
Acetone
Concen: 1.877 ug/L
RT: 2.68 min Scan# 418
Delta R.T. 0.00 min
Lab File: VU036216.D
Acq: 13 Dec 2019 23:18

Instrument :
MSVOA_U
ClientSampleId :
BFQS3

Tot Ion: 43 Resp: 6135
Ion Ratio Lower Upper
43 100
58 37.4 0.0 67.6

