


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121319\
 Data File : VU036189.D
 Acq On : 13 Dec 2019 10:26
 Operator : JC/MD
 Sample : BFB18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Dec 14 01:19:01 2019

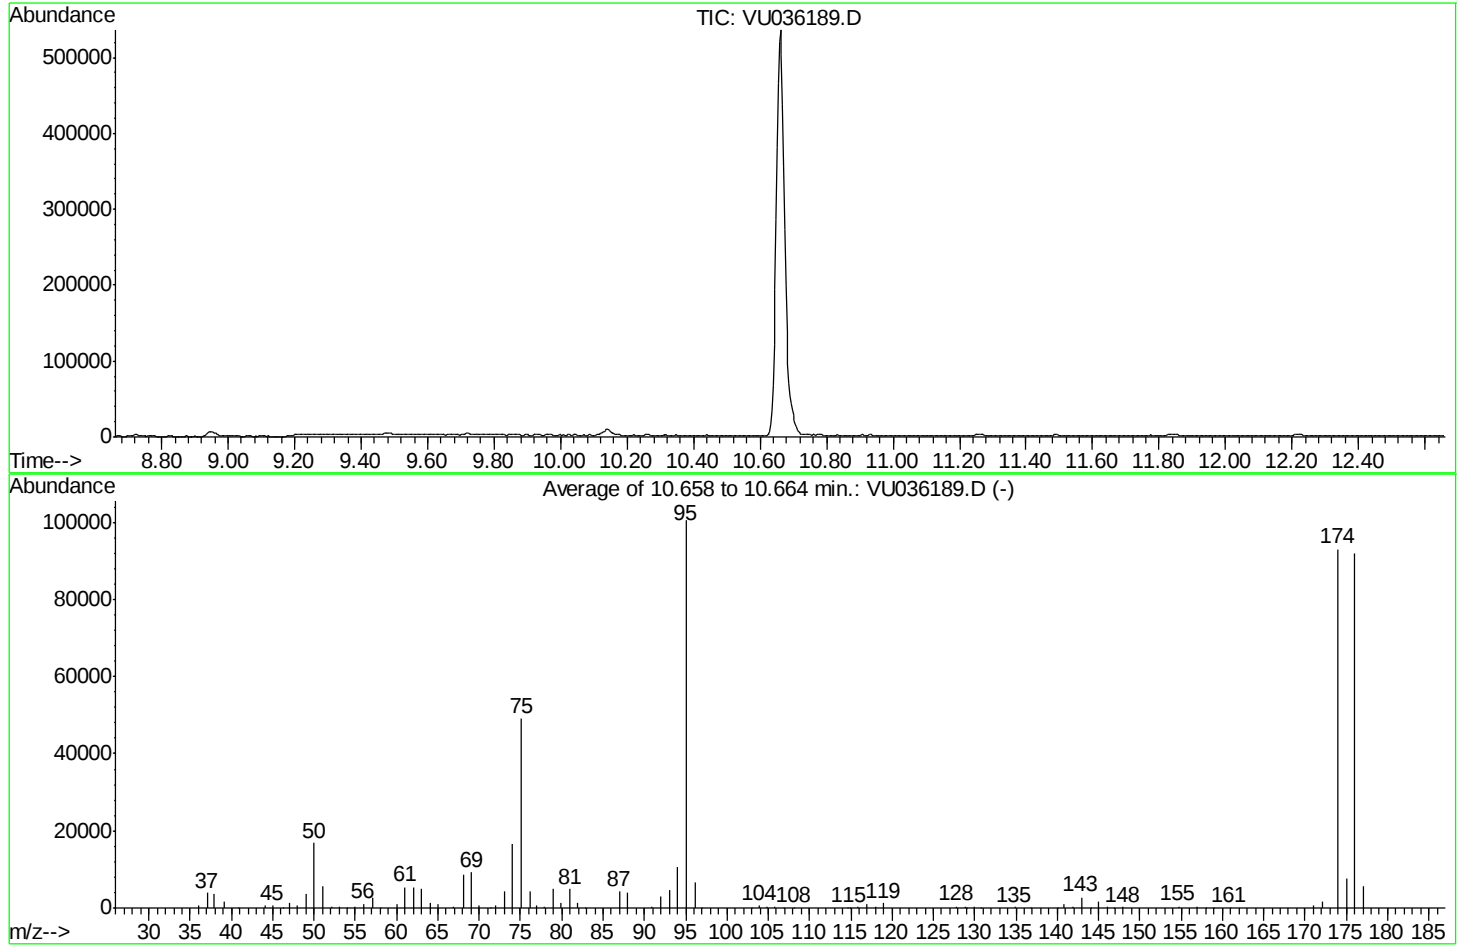

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	16880	PASS
75	95	30	80	48.8	49053	PASS
95	95	100	100	100.0	100506	PASS
96	95	5	9	6.5	6511	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.5	92984	PASS
175	174	5	9	8.1	7496	PASS
176	174	95	101	99.0	92085	PASS
177	176	5	9	6.1	5609	PASS

m/z	Abundance
36.00	1823.0
37.00	4069.0
38.00	3911.0
39.00	1672.0
40.00	222.0
40.90	123.0
44.10	1165.0
45.00	620.0
46.20	116.0
47.00	1241.0
48.00	568.0
49.00	3771.0
50.00	17864.0
51.00	5976.0
52.10	365.0
53.00	282.0
54.10	164.0
55.00	353.0
56.00	1124.0
57.00	2328.0
58.00	123.0
60.00	1078.0
61.00	5210.0
62.00	5255.0
63.00	4916.0
64.10	1234.0
65.10	1027.0
66.90	205.0
68.10	8955.0
69.10	9647.0
70.00	671.0
71.40	116.0
72.00	705.0
73.10	3891.0
74.10	16346.0
75.10	49944.0
76.10	4466.0
77.00	584.0
79.00	5010.0
79.90	1444.0
81.00	5162.0
82.00	1249.0
82.80	161.0
87.00	4464.0
88.00	4322.0
90.90	463.0
92.10	3015.0
93.00	4748.0
94.00	11091.0
95.10	100872.0
96.10	6562.0
97.00	188.0
103.00	100.0
104.00	583.0
104.90	163.0
105.80	469.0
108.20	104.0
115.80	415.0
116.90	944.0
118.00	355.0
119.00	1253.0
127.90	312.0
128.80	241.0
129.00	240.0
129.90	364.0
130.80	111.0
134.80	207.0
136.90	143.0
140.90	1075.0
141.90	221.0
142.90	2640.0
144.00	230.0
144.90	1533.0
146.00	279.0
147.90	185.0
154.70	452.0
157.00	333.0
158.00	149.0
160.90	114.0
171.00	675.0
172.00	1499.0
174.00	91264.0
175.00	7488.0
176.00	90000.0
177.00	5783.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1761.0
37.10	3846.0
38.00	4106.0
39.00	1748.0
40.00	240.0
40.90	119.0
44.10	1203.0
45.00	654.0
47.00	1232.0
48.00	716.0
49.00	3617.0
50.00	17264.0
51.00	5681.0
52.10	309.0
53.00	459.0
54.00	150.0
55.00	392.0
56.00	1174.0
57.10	2619.0
58.00	136.0
60.00	1134.0
61.00	5736.0
62.00	5429.0
63.00	4873.0
64.10	1305.0
65.10	1033.0
66.90	225.0
68.10	8843.0
69.10	9561.0
70.00	615.0
72.00	674.0
73.10	4395.0
74.00	17064.0
75.10	50344.0
76.10	4453.0
77.00	615.0
77.80	389.0
79.00	5027.0
80.00	1503.0
81.00	5069.0
82.00	1329.0
82.80	117.0
87.00	4414.0
88.00	4251.0
91.00	441.0
92.10	2959.0
93.00	4816.0
94.00	10627.0
95.10	103416.0
96.10	6767.0
96.90	149.0
103.00	110.0
104.00	570.0
104.90	189.0
105.80	482.0
106.90	110.0
108.20	135.0
114.90	101.0
115.90	450.0
116.90	979.0
118.00	439.0
119.00	1317.0
127.80	351.0
128.80	207.0
129.90	339.0
130.80	155.0
134.80	229.0
136.80	153.0
140.10	103.0
140.90	1209.0
142.00	217.0
142.90	2842.0
144.00	163.0
144.90	1576.0
146.10	353.0
148.00	206.0
154.70	420.0
157.00	321.0
158.00	133.0
158.90	113.0
160.90	115.0
171.00	663.0
172.10	1669.0
174.00	95968.0
175.00	7633.0
176.00	95520.0
177.00	5812.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1476.0
37.10	3630.0
38.00	3956.0
39.10	1589.0
40.00	271.0
44.10	1260.0
45.00	691.0
47.00	1122.0
48.00	776.0
49.10	3335.0
50.00	15514.0
51.10	4929.0
52.20	191.0
53.00	452.0
54.00	152.0
55.00	317.0
56.00	1182.0
57.10	2715.0
58.00	111.0
60.00	977.0
61.00	5398.0
62.00	5229.0
63.00	4799.0
64.10	1239.0
65.00	938.0
66.90	206.0
68.10	8062.0
69.10	8602.0
70.00	644.0
72.10	519.0
73.10	4510.0
74.00	16528.0
75.10	46872.0
76.10	4030.0
77.00	618.0
77.90	347.0
79.00	4643.0
79.90	1410.0
81.00	4566.0
81.90	1202.0
87.00	4069.0
88.00	3736.0
91.00	325.0
92.00	2627.0
93.00	4568.0
94.10	10023.0
95.00	97232.0
96.10	6205.0
96.90	107.0
103.90	524.0
104.90	206.0
105.80	465.0
108.10	147.0
114.60	107.0
114.90	102.0
115.90	423.0
116.90	1057.0
118.00	467.0
119.00	1156.0
127.90	364.0
128.80	138.0
130.00	289.0
130.80	202.0
134.90	233.0
136.80	135.0
140.10	140.0
140.80	1157.0
142.00	165.0
143.00	2618.0
144.00	113.0
145.00	1538.0
146.10	322.0
146.90	125.0
148.00	199.0
154.70	299.0
157.00	267.0
158.90	107.0
171.00	584.0
172.10	1701.0
174.00	91720.0
175.00	7368.0
176.00	90736.0
177.00	5233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

Scan 2884 (10.613 min): VU036189.D
BFB18

m/z	Abundance
35.20	134.0
35.90	953.0
37.90	308.0
40.10	301.0
44.00	608.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18