




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046324.D
Acq On : 13 Dec 2021 18:35
Operator : SY/MD
Sample : M4971-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/14/2021
Supervised By :Mahesh Dadoda 12/14/2021

Quant Time: Dec 14 03:53:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 14 03:19:41 2021
Response via : Initial Calibration

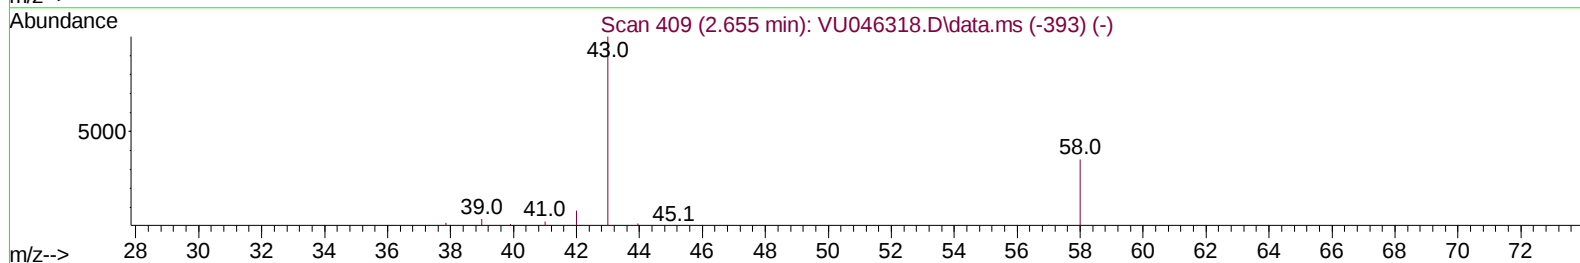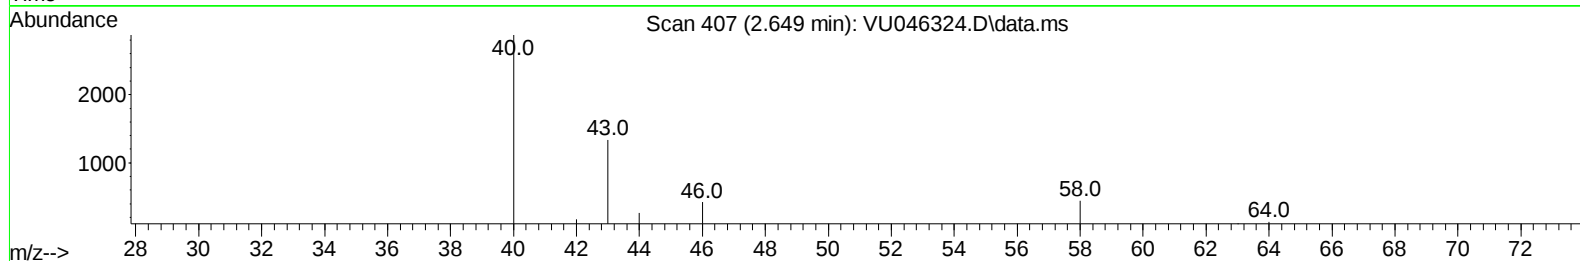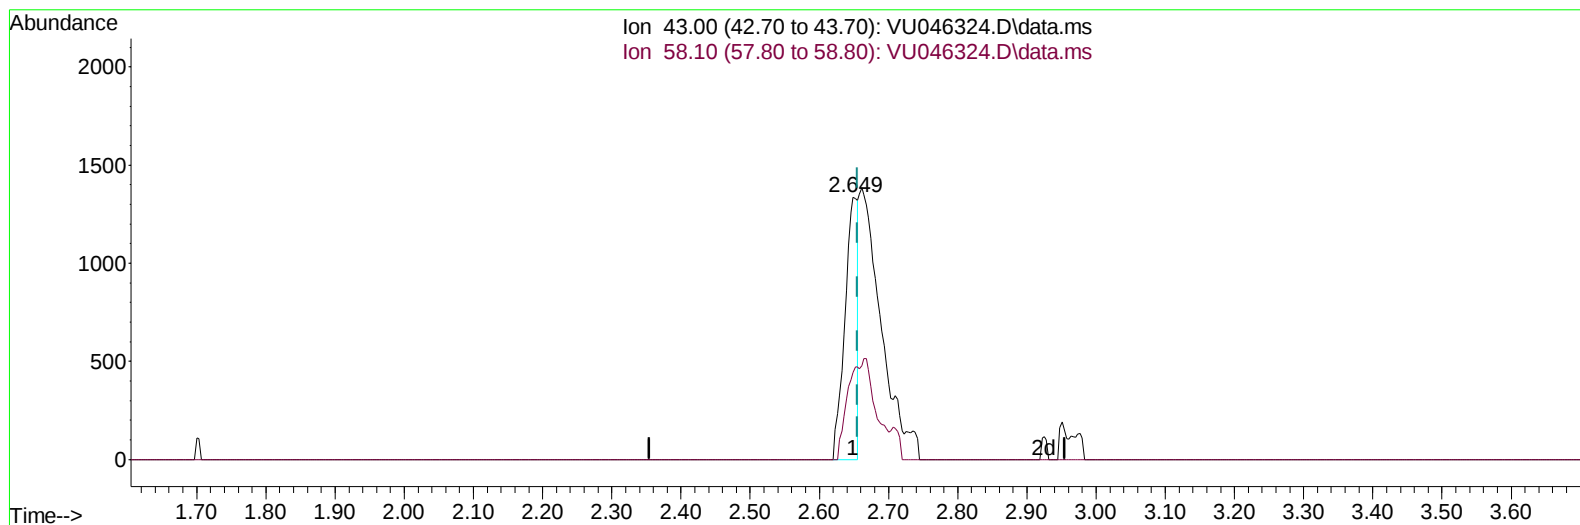

TIC: VU046324.D\data.ms

(13) Acetone (T)

2.649min (-0.006) 1.48 ug/L

response 1736

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.40	37.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046324.D
Acq On : 13 Dec 2021 18:35
Operator : SY/MD
Sample : M4971-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/14/2021
Supervised By :Mahesh Dadoda 12/14/2021

Quant Time: Dec 14 03:53:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 14 03:19:41 2021
Response via : Initial Calibration

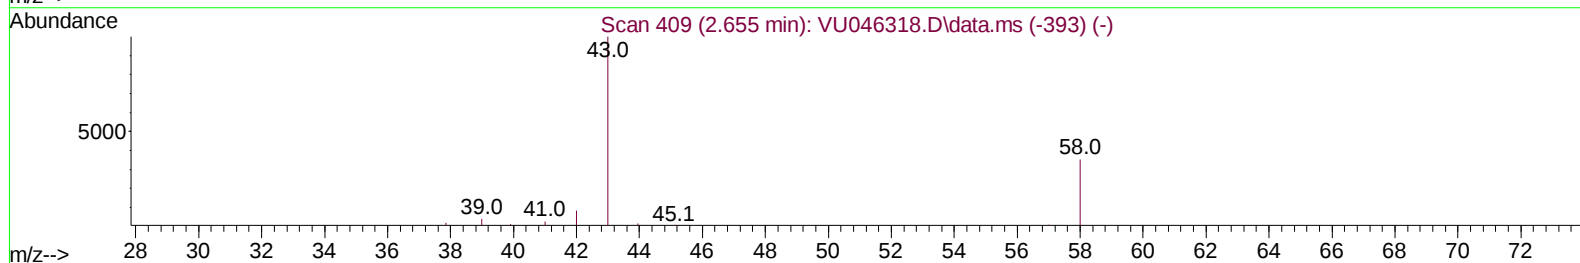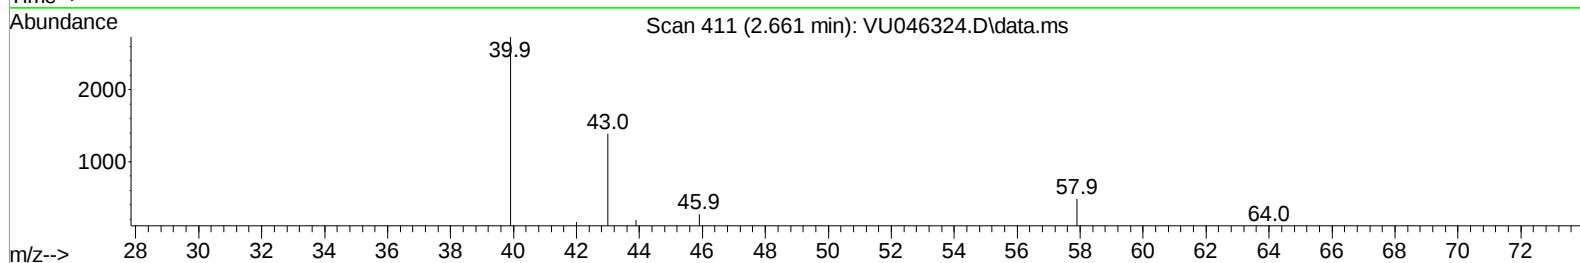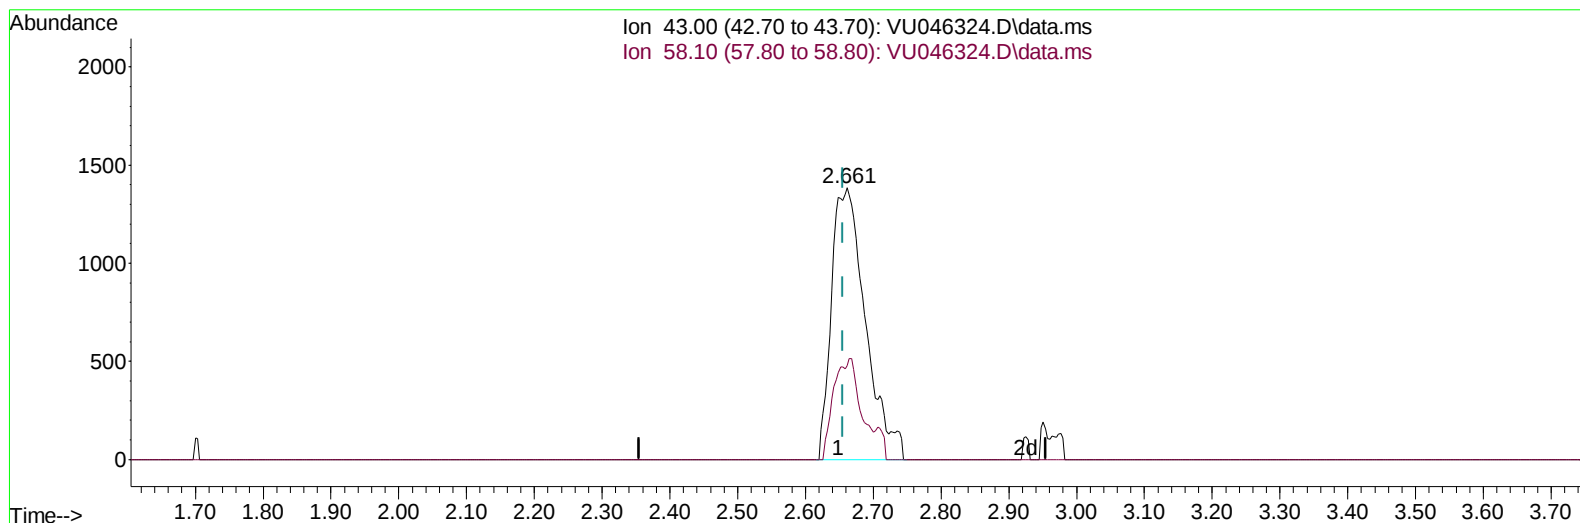

TIC: VU046324.D\data.ms

(13) Acetone (T)

2.661min (+ 0.006) 4.09 ug/L m

response 4806

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.40	13.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046324.D
 Acq On : 13 Dec 2021 18:35
 Operator : SY/MD
 Sample : M4971-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E8

Manual IntegrationsAPPROVED

Quant Time: Dec 14 03:53:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 14 03:19:41 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/14/2021
 Supervised By :Mahesh Dadoda 12/14/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	143671	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	153978	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	75810	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	57135	48.277	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	96.560%	
7) Chloroethane-d5	1.919	69	42298	46.549	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	93.100%	
11) 1,1-Dichloroethene-d2	2.571	63	71795	33.793	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	67.580%	
21) 2-Butanone-d5	4.639	46	86055	91.468	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.470%	
24) Chloroform-d	5.070	84	94329	47.729	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.460%	
26) 1,2-Dichloroethane-d4	5.706	65	65168	49.133	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	98.260%	
32) Benzene-d6	5.732	84	192764	43.678	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.360%	
36) 1,2-Dichloropropane-d6	6.693	67	61653	45.076	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.160%	
41) Toluene-d8	7.899	98	162913	40.543	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.080%	
43) trans-1,3-Dichloroprop...	8.182	79	28427	43.054	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.100%	
47) 2-Hexanone-d5	8.635	63	57253	88.285	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	88.290%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	95845	46.207	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	92.420%	
66) 1,2-Dichlorobenzene-d4	12.195	152	66017	45.218	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.440%	
Target Compounds						
					Qvalue	
13) Acetone	2.661	43	4806m	4.087	ug/L	
33) Benzene	5.777	78	3441	0.738	ug/L	100
42) Toluene	7.970	91	6890	1.378	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046324.D
Acq On : 13 Dec 2021 18:35
Operator : SY/MD
Sample : M4971-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E8

Manual IntegrationsAPPROVED

Quant Time: Dec 14 03:53:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 14 03:19:41 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/14/2021
Supervised By :Mahesh Dadoda 12/14/2021

