

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046332.D
 Acq On : 13 Dec 2021 21:35
 Operator : SY/MD
 Sample : M5023-06ME
 Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKY2ME

Quant Time: Dec 14 03:55:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 14 03:19:41 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 12/14/2021
 Supervised By : Mahesh Dadoda 12/14/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	177314	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	184189	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	88271	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	55364	37.904	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.800%
7) Chloroethane-d5	1.916	69	34803	31.034	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	62.060%#
11) 1,1-Dichloroethene-d2	2.549	63	64146	24.464	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	48.920%#
21) 2-Butanone-d5	4.661	46	66763	57.499	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	57.500%
24) Chloroform-d	5.066	84	90731	37.198	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.400%
26) 1,2-Dichloroethane-d4	5.703	65	65721	40.148	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.300%
32) Benzene-d6	5.726	84	191386	36.253	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.500%
36) 1,2-Dichloropropane-d6	6.693	67	60215	36.804	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	73.600%
41) Toluene-d8	7.899	98	167890	34.929	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	69.860%#
43) trans-1,3-Dichloroprop...	8.182	79	28645	36.268	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.540%
47) 2-Hexanone-d5	8.684	63	53872	69.446	ug/L	0.05
Spiked Amount	100.000	Range	45 - 130	Recovery	=	69.450%
56) 1,1,2,2-Tetrachloroeth...	10.770	84	87055	35.085	ug/L	0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	70.180%
66) 1,2-Dichlorobenzene-d4	12.201	152	62426	36.722	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.440%#
Target Compounds						
					Qvalue	
22) 2-Butanone	4.742	43	12112m	7.667	ug/L	
46) Tetrachloroethene	8.552	164	6532	6.052	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046332.D
Acq On : 13 Dec 2021 21:35
Operator : SY/MD
Sample : M5023-06ME
Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BGKY2ME

Quant Time: Dec 14 03:55:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 14 03:19:41 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/14/2021
Supervised By :Mahesh Dadoda 12/14/2021

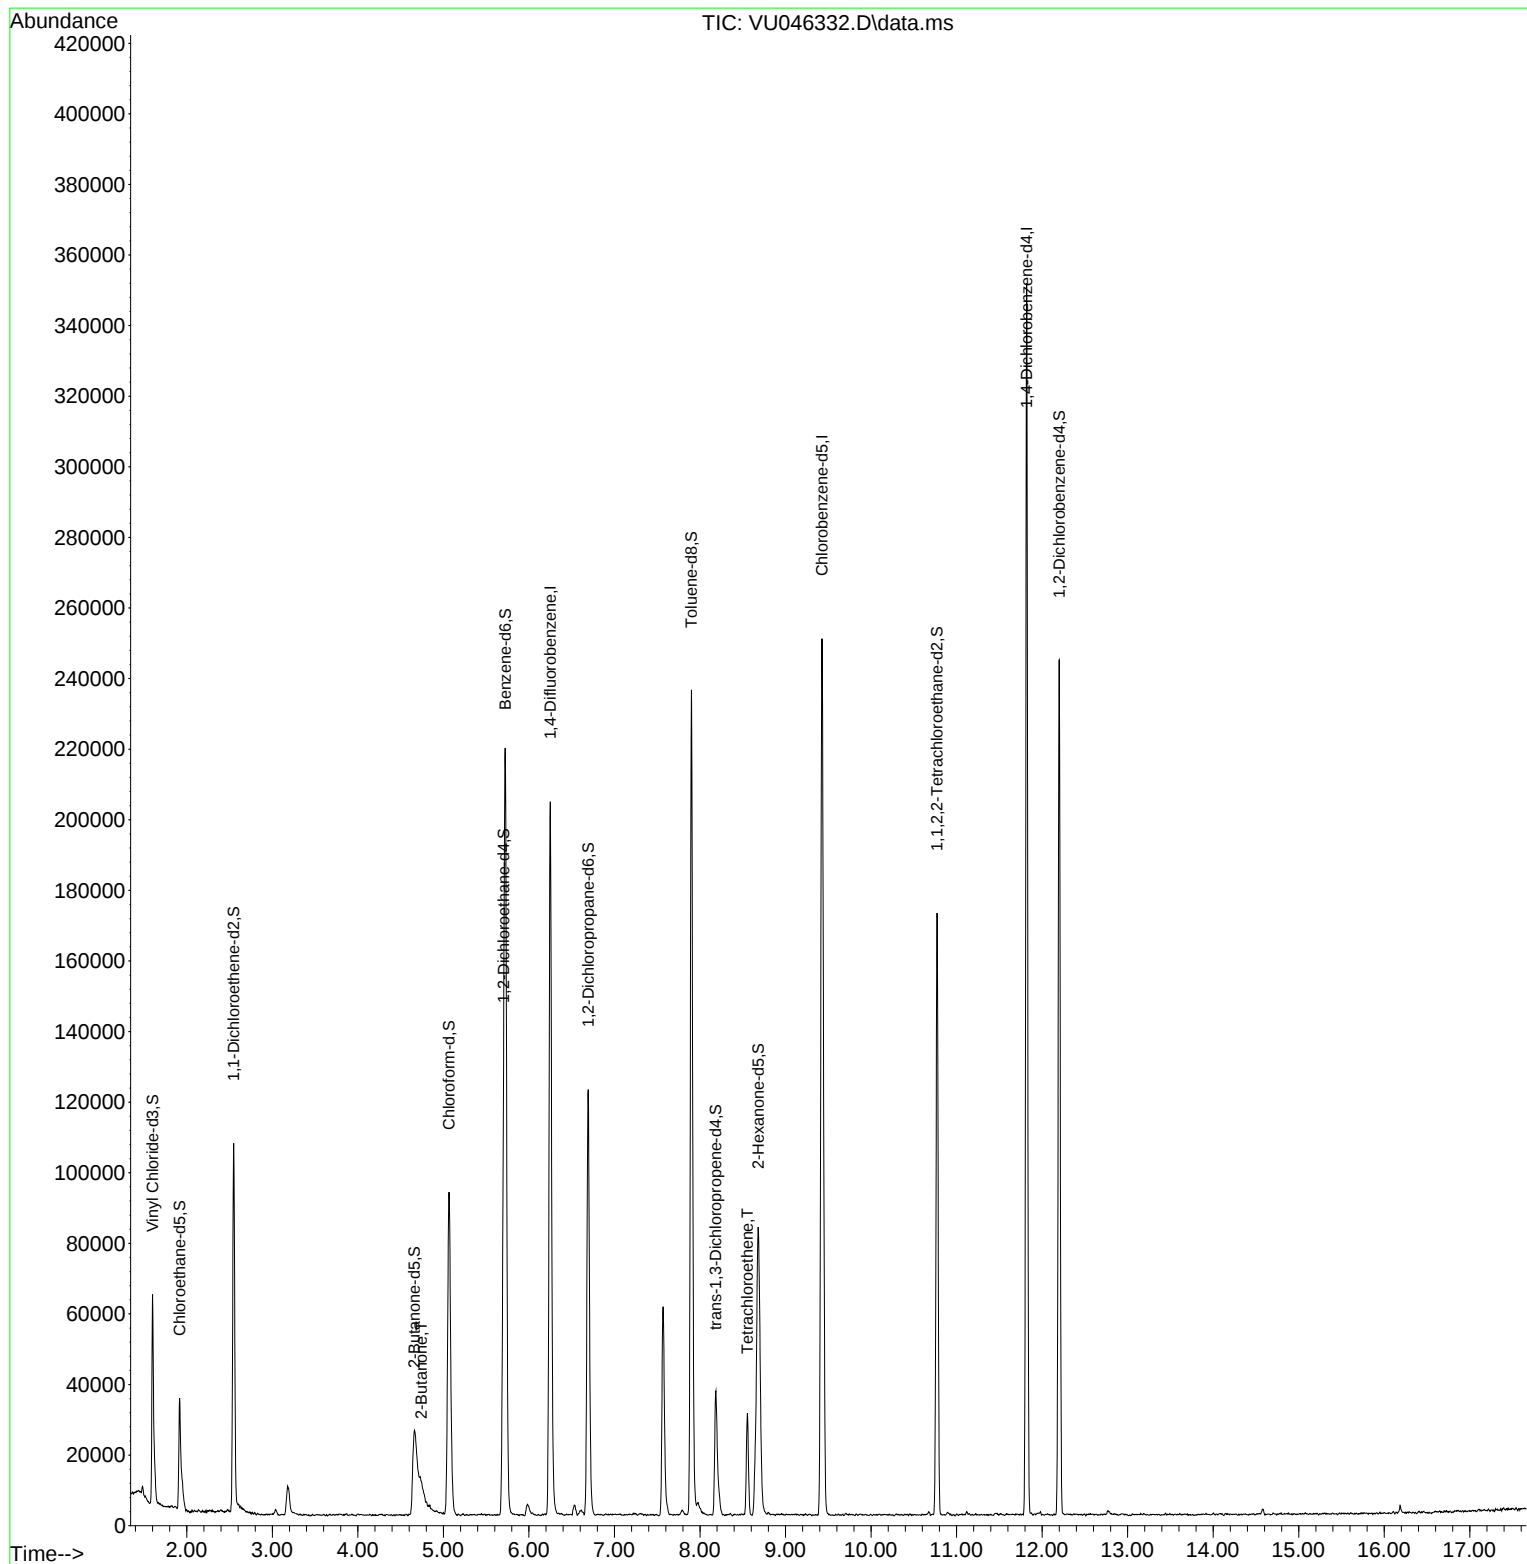

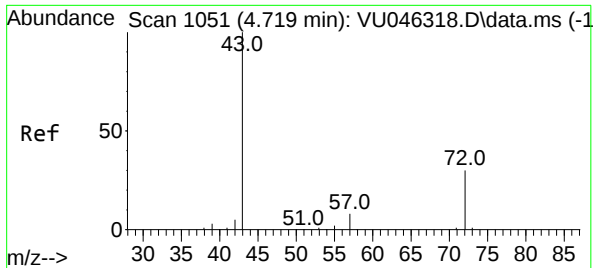

#22

2-Butanone

Concen: 7.667 ug/L m

RT: 4.742 min Scan# 1058

Delta R.T. 0.023 min

Lab File: VU046332.D

Acq: 13 Dec 2021 21:35

Instrument :

MSVOA_U

ClientSampleId :

BGKY2ME

Tgt Ion: 43 Resp: 1211

Ion Ratio Lower Upper

43 100





72 9.1 14.5 43.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/14/2021

Supervised By :Mahesh Dadoda 12/14/2021

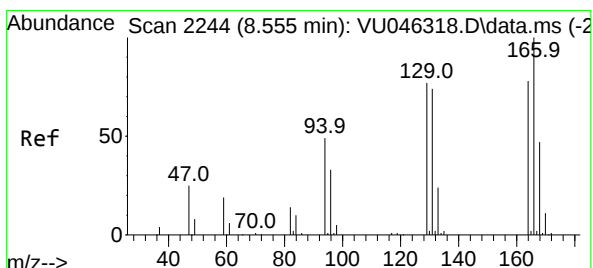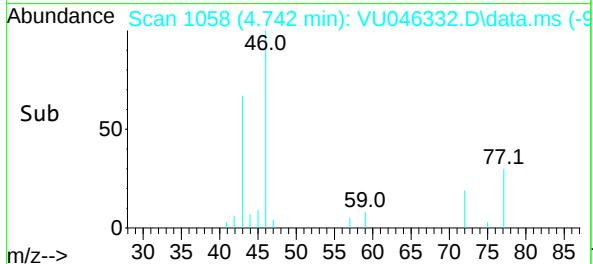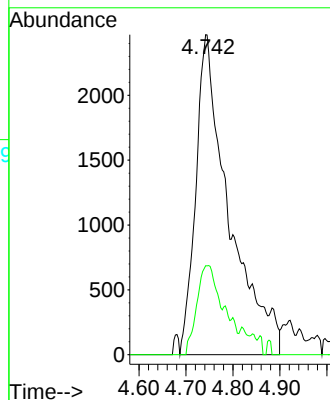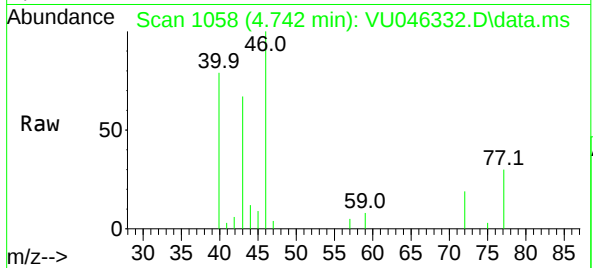

#46

Tetrachloroethene

Concen: 6.052 ug/L

RT: 8.552 min Scan# 2243

Delta R.T. -0.003 min

Lab File: VU046332.D

Acq: 13 Dec 2021 21:35

Tgt Ion:164 Resp: 6532

Ion Ratio Lower Upper

164 100

129 93.0 71.1 132.1

131 87.7 67.8 126.0

166 119.8 90.6 168.2

