

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046304.D
 Acq On : 13 Dec 2021 10:49
 Operator : SY/MD
 Sample : VU1213WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK057

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	96	rVB	100957	109144	17.02%	2.232%
2	1.919	173	180	194	rVB	69303	86632	13.51%	1.772%
3	2.366	316	319	323	rBV2	455	372	0.06%	0.008%
4	2.408	328	332	337	rVB2	653	797	0.12%	0.016%
5	2.575	372	384	400	rBV	146368	241780	37.71%	4.944%
6	3.048	528	531	537	rBV3	746	714	0.11%	0.015%
7	3.125	551	555	558	rBV	602	490	0.08%	0.010%
8	3.279	600	603	607	rBV	594	505	0.08%	0.010%
9	4.192	884	887	890	rBV	515	415	0.06%	0.008%
10	4.475	969	975	978	rBV	472	548	0.09%	0.011%
11	4.646	1012	1028	1065	rBV	46618	168802	26.33%	3.452%
12	5.067	1144	1159	1192	rVB	109349	259286	40.44%	5.302%
13	5.231	1206	1210	1213	rBV	503	401	0.06%	0.008%
14	5.575	1312	1317	1321	rBV	704	794	0.12%	0.016%
15	5.633	1332	1335	1338	rBV	426	337	0.05%	0.007%
16	5.729	1344	1365	1386	rBV2	236744	641129	100.00%	13.110%
17	6.253	1514	1528	1556	rBV	169821	320608	50.01%	6.556%
18	6.527	1606	1613	1623	rBV5	2359	4260	0.66%	0.087%
19	6.694	1652	1665	1687	rVV	145192	281996	43.98%	5.767%
20	6.813	1699	1702	1705	rBV2	489	433	0.07%	0.009%
21	6.887	1719	1725	1727	rBV2	393	436	0.07%	0.009%
22	6.932	1736	1739	1743	rBV	436	348	0.05%	0.007%
23	7.015	1762	1765	1767	rBV	480	302	0.05%	0.006%
24	7.401	1882	1885	1888	rBV	456	351	0.05%	0.007%
25	7.568	1925	1937	1963	rVB	77666	136253	21.25%	2.786%
26	7.826	2013	2017	2021	rBV	332	307	0.05%	0.006%
27	7.900	2027	2040	2057	rBV	288461	500521	78.07%	10.235%
28	8.182	2117	2128	2143	rVV	56006	92500	14.43%	1.892%
29	8.369	2183	2186	2190	rBV	412	317	0.05%	0.006%
30	8.459	2209	2214	2217	rBV	355	394	0.06%	0.008%
31	8.636	2257	2269	2293	rBV	178998	323883	50.52%	6.623%
32	8.832	2325	2330	2333	rBV	484	384	0.06%	0.008%
33	8.912	2347	2355	2365	rVB3	1202	2122	0.33%	0.043%
34	8.986	2372	2378	2381	rBV	512	518	0.08%	0.011%
35	9.054	2393	2399	2403	rBV2	548	452	0.07%	0.009%
36	9.089	2408	2410	2415	rVB	690	488	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046304.D
 Acq On : 13 Dec 2021 10:49
 Operator : SY/MD
 Sample : VU1213WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK057

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	9.115	2415	2418	2422	rBV	515	419	0.07%	0.009%
38	9.166	2427	2434	2437	rBV2	544	650	0.10%	0.013%
39	9.269	2463	2466	2468	rBV	536	381	0.06%	0.008%
40	9.420	2495	2513	2532	rBV	260334	428764	66.88%	8.768%
41	9.629	2575	2578	2581	rVB	555	334	0.05%	0.007%
42	9.652	2581	2585	2588	rBV2	552	497	0.08%	0.010%
43	9.690	2593	2597	2603	rBV4	612	630	0.10%	0.013%
44	9.867	2649	2652	2656	rVB2	639	500	0.08%	0.010%
45	9.893	2656	2660	2663	rBV	496	501	0.08%	0.010%
46	9.912	2663	2666	2670	rVB	434	360	0.06%	0.007%
47	9.948	2675	2677	2680	rBV	472	334	0.05%	0.007%
48	10.031	2698	2703	2705	rBV	641	498	0.08%	0.010%
49	10.247	2767	2770	2774	rVV	403	354	0.06%	0.007%
50	10.285	2778	2782	2787	rVV	632	634	0.10%	0.013%
51	10.317	2789	2792	2802	rVB	806	1058	0.17%	0.022%
52	10.362	2802	2806	2808	rBV	526	434	0.07%	0.009%
53	10.407	2814	2820	2824	rBV	380	398	0.06%	0.008%
54	10.671	2897	2902	2913	rVV6	1811	2809	0.44%	0.057%
55	10.758	2917	2929	2945	rVV	218501	347376	54.18%	7.103%
56	10.867	2960	2963	2966	rBV	998	872	0.14%	0.018%
57	10.919	2976	2979	2982	rBV	484	380	0.06%	0.008%
58	10.967	2991	2994	3000	rVB2	470	522	0.08%	0.011%
59	11.018	3007	3010	3018	rVB	640	702	0.11%	0.014%
60	11.079	3022	3029	3030	rBV2	350	396	0.06%	0.008%
61	11.247	3078	3081	3087	rVB	591	528	0.08%	0.011%
62	11.276	3087	3090	3097	rVB2	506	619	0.10%	0.013%
63	11.404	3126	3130	3135	rVB2	736	835	0.13%	0.017%
64	11.449	3135	3144	3145	rBV2	1277	1149	0.18%	0.023%
65	11.504	3158	3161	3170	rVB2	666	888	0.14%	0.018%
66	11.546	3170	3174	3177	rBV	777	593	0.09%	0.012%
67	11.587	3183	3187	3195	rBV2	426	529	0.08%	0.011%
68	11.639	3200	3203	3206	rBV	709	596	0.09%	0.012%
69	11.700	3216	3222	3226	rBV2	589	699	0.11%	0.014%
70	11.813	3245	3257	3272	rVV	273477	428042	66.76%	8.753%
71	11.973	3303	3307	3313	rVB4	1031	1308	0.20%	0.027%
72	12.076	3337	3339	3345	rVB	437	332	0.05%	0.007%
73	12.124	3351	3354	3358	rBV	424	308	0.05%	0.006%
74	12.195	3363	3376	3395	rBV	296185	472225	73.66%	9.656%
75	12.272	3397	3400	3402	rBV	507	302	0.05%	0.006%
76	12.308	3408	3411	3417	rBV2	331	424	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046304.D
 Acq On : 13 Dec 2021 10:49
 Operator : SY/MD
 Sample : VU1213WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK057

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.385	3431	3435	3440	rBV	464	432	0.07%	0.009%
78	12.581	3493	3496	3502	rVB2	566	419	0.07%	0.009%
79	12.690	3527	3530	3535	rBV	441	452	0.07%	0.009%
80	12.803	3563	3565	3569	rVB2	486	307	0.05%	0.006%
81	12.896	3591	3594	3599	rBV	399	372	0.06%	0.008%
82	13.327	3723	3728	3732	rBV	702	646	0.10%	0.013%
83	13.501	3777	3782	3785	rBV	382	361	0.06%	0.007%
84	13.571	3800	3804	3805	rBV2	527	355	0.06%	0.007%
85	13.620	3816	3819	3823	rBV	610	509	0.08%	0.010%
86	13.706	3842	3846	3850	rVB	524	482	0.08%	0.010%
87	13.806	3875	3877	3883	rVB	503	503	0.08%	0.010%
88	13.848	3883	3890	3893	rBV3	564	760	0.12%	0.016%
89	14.031	3944	3947	3949	rBV	482	339	0.05%	0.007%
90	14.092	3957	3966	3971	rBV2	754	1304	0.20%	0.027%
91	14.295	4026	4029	4033	rBV2	410	372	0.06%	0.008%
92	14.456	4076	4079	4083	rBV2	696	725	0.11%	0.015%
93	14.620	4126	4130	4135	rBV2	446	506	0.08%	0.010%
94	14.687	4148	4151	4155	rBV2	341	310	0.05%	0.006%
95	14.716	4158	4160	4165	rVB	486	358	0.06%	0.007%
96	15.028	4254	4257	4262	rVB	675	565	0.09%	0.012%
97	15.054	4262	4265	4268	rBV2	559	505	0.08%	0.010%
98	15.111	4280	4283	4287	rBV3	498	496	0.08%	0.010%
99	15.295	4338	4340	4346	rVB2	523	525	0.08%	0.011%
100	16.555	4730	4732	4738	rBV	593	435	0.07%	0.009%




Sum of corrected areas: 4890237

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046304.D
Acq On : 13 Dec 2021 10:49
Operator : SY/MD
Sample : VU1213WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK057

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

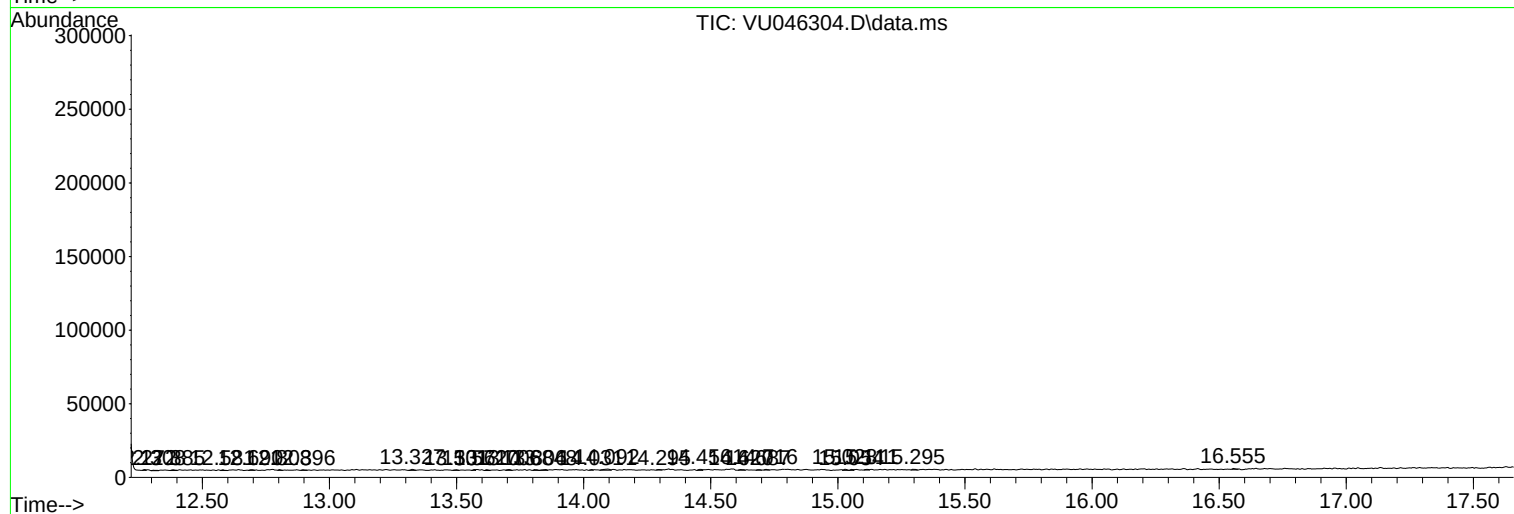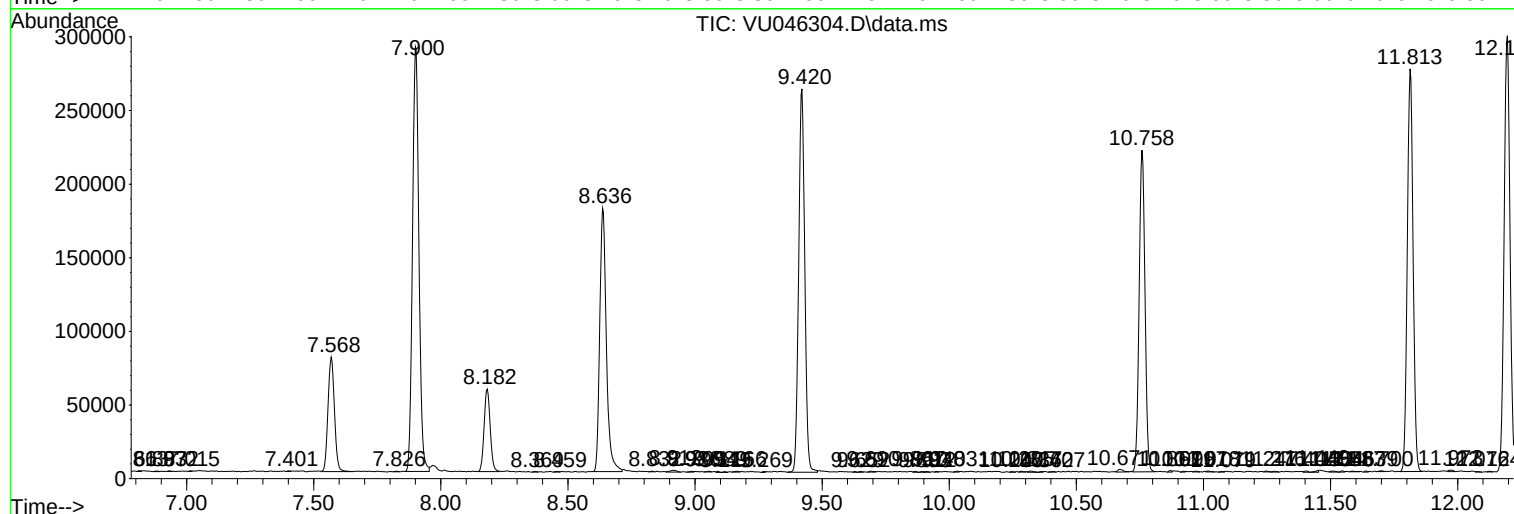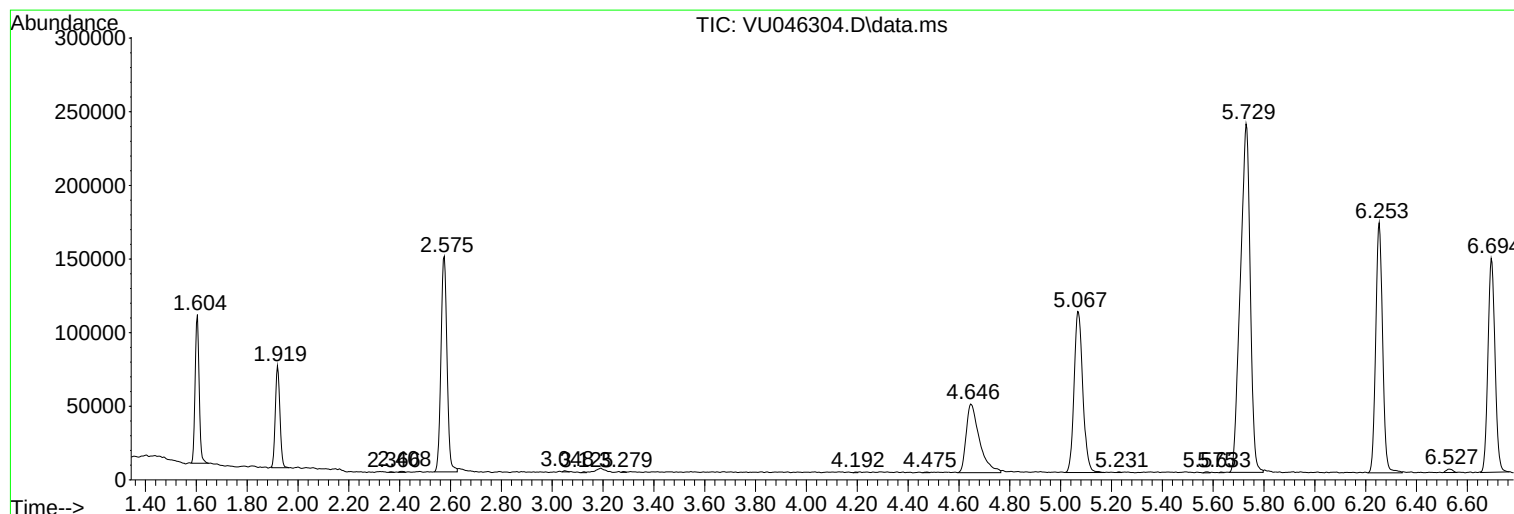

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046304.D
Acq On : 13 Dec 2021 10:49
Operator : SY/MD
Sample : VU1213WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK057

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046304.D
Acq On : 13 Dec 2021 10:49
Operator : SY/MD
Sample : VU1213WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK057

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc