

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046316.D
 Acq On : 13 Dec 2021 15:29
 Operator : SY/MD
 Sample : M5004-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	96	rVB	88976	97029	16.11%	2.063%
2	1.919	172	180	193	rVB	61173	77669	12.90%	1.652%
3	2.179	259	261	263	rVB	138	63	0.01%	0.001%
4	2.195	263	266	267	rBV2	147	78	0.01%	0.002%
5	2.208	267	270	275	rBV2	235	245	0.04%	0.005%
6	2.260	284	286	292	rBV2	395	352	0.06%	0.007%
7	2.314	300	303	308	rBV2	374	298	0.05%	0.006%
8	2.340	308	311	313	rBV	205	135	0.02%	0.003%
9	2.414	326	334	335	rBV2	456	495	0.08%	0.011%
10	2.453	343	346	348	rBV2	253	179	0.03%	0.004%
11	2.572	371	383	413	rBV	133131	220522	36.62%	4.689%
12	2.713	424	427	431	rBV	273	236	0.04%	0.005%
13	2.874	474	477	479	rBV	278	205	0.03%	0.004%
14	2.964	502	505	508	rBV2	245	193	0.03%	0.004%
15	2.983	508	511	514	rBV	224	120	0.02%	0.003%
16	3.002	514	517	521	rVB	383	312	0.05%	0.007%
17	3.025	521	524	526	rBV2	277	179	0.03%	0.004%
18	3.044	526	530	532	rBV2	902	674	0.11%	0.014%
19	3.109	546	550	553	rBV2	267	207	0.03%	0.004%
20	3.189	572	575	577	rBV	369	226	0.04%	0.005%
21	3.228	584	587	590	rBV2	204	125	0.02%	0.003%
22	3.337	618	621	623	rBV	283	179	0.03%	0.004%
23	3.424	646	648	651	rVB	173	88	0.01%	0.002%
24	3.449	651	656	658	rBV	262	293	0.05%	0.006%
25	3.507	671	674	677	rBV	272	207	0.03%	0.004%
26	3.771	753	756	758	rBV2	223	170	0.03%	0.004%
27	3.916	796	801	804	rBV2	295	373	0.06%	0.008%
28	3.990	820	824	827	rBV2	372	392	0.07%	0.008%
29	4.080	846	852	855	rBV2	334	362	0.06%	0.008%
30	4.231	895	899	906	rBV2	286	361	0.06%	0.008%
31	4.263	906	909	911	rVB	173	105	0.02%	0.002%
32	4.279	911	914	916	rBV	169	89	0.01%	0.002%
33	4.417	954	957	958	rBV	173	98	0.02%	0.002%
34	4.459	967	970	972	rBV2	238	141	0.02%	0.003%
35	4.510	984	986	990	rBV	332	314	0.05%	0.007%
36	4.575	1004	1006	1007	rBV	212	91	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046316.D
 Acq On : 13 Dec 2021 15:29
 Operator : SY/MD
 Sample : M5004-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	4.639	1012	1026	1059	rVV2	48824	143704	23.86%	3.056%
38	4.890	1101	1104	1108	rBV2	289	253	0.04%	0.005%
39	4.999	1135	1138	1140	rBV2	276	187	0.03%	0.004%
40	5.067	1143	1159	1183	rBV2	104662	243191	40.38%	5.171%
41	5.433	1269	1273	1275	rBV2	179	114	0.02%	0.002%
42	5.443	1275	1276	1278	rVB	187	45	0.01%	0.001%
43	5.469	1278	1284	1287	rBV2	410	557	0.09%	0.012%
44	5.562	1310	1313	1316	rVB	299	164	0.03%	0.003%
45	5.588	1316	1321	1324	rBV	357	331	0.05%	0.007%
46	5.607	1324	1327	1336	rVB2	443	545	0.09%	0.012%
47	5.645	1336	1339	1341	rBV2	248	144	0.02%	0.003%
48	5.729	1344	1365	1385	rBV2	222179	602194	100.00%	12.805%
49	5.893	1413	1416	1423	rVB	311	359	0.06%	0.008%
50	5.925	1423	1426	1428	rBV	266	159	0.03%	0.003%
51	6.089	1474	1477	1480	rBV	185	145	0.02%	0.003%
52	6.108	1480	1483	1487	rVV	273	203	0.03%	0.004%
53	6.131	1487	1490	1493	rVB2	302	170	0.03%	0.004%
54	6.160	1496	1499	1502	rBV2	203	148	0.02%	0.003%
55	6.250	1515	1527	1549	rBV	182202	344057	57.13%	7.316%
56	6.530	1608	1614	1626	rVB3	1712	3086	0.51%	0.066%
57	6.694	1651	1665	1683	rBV	138693	265249	44.05%	5.640%
58	6.887	1722	1725	1727	rBV	235	171	0.03%	0.004%
59	6.932	1736	1739	1742	rBV	334	204	0.03%	0.004%
60	7.060	1776	1779	1782	rBV2	494	277	0.05%	0.006%
61	7.147	1801	1806	1809	rBV2	380	389	0.06%	0.008%
62	7.282	1842	1848	1851	rBV	398	385	0.06%	0.008%
63	7.301	1851	1854	1856	rBV2	316	218	0.04%	0.005%
64	7.491	1910	1913	1914	rBV	252	144	0.02%	0.003%
65	7.568	1925	1937	1953	rBV	73977	127944	21.25%	2.721%
66	7.899	2027	2040	2058	rBV	272592	467633	77.65%	9.944%
67	8.179	2117	2127	2144	rBV	52026	86794	14.41%	1.846%
68	8.494	2222	2225	2228	rVB	367	227	0.04%	0.005%
69	8.517	2228	2232	2235	rBV	286	288	0.05%	0.006%
70	8.636	2254	2269	2295	rBV	166633	300366	49.88%	6.387%
71	9.057	2397	2400	2401	rBV	316	186	0.03%	0.004%
72	9.417	2499	2512	2535	rBV	278856	468460	77.79%	9.961%
73	9.800	2628	2631	2634	rVB	401	257	0.04%	0.005%
74	10.060	2709	2712	2715	rBV	364	302	0.05%	0.006%
75	10.160	2740	2743	2749	rBV	251	309	0.05%	0.007%
76	10.758	2917	2929	2945	rBV	205082	323396	53.70%	6.877%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046316.D
Acq On : 13 Dec 2021 15:29
Operator : SY/MD
Sample : M5004-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	10.893	2968	2971	2976	rVB3	783	580	0.10%	0.012%
78	11.256	3081	3084	3089	rBV	423	403	0.07%	0.009%
79	11.812	3242	3257	3273	rBV	304318	469951	78.04%	9.993%
80	12.195	3362	3376	3394	rBV	279466	445775	74.03%	9.479%
81	13.320	3723	3726	3728	rBV	382	247	0.04%	0.005%




Sum of corrected areas: 4702716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046316.D
Acq On : 13 Dec 2021 15:29
Operator : SY/MD
Sample : M5004-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

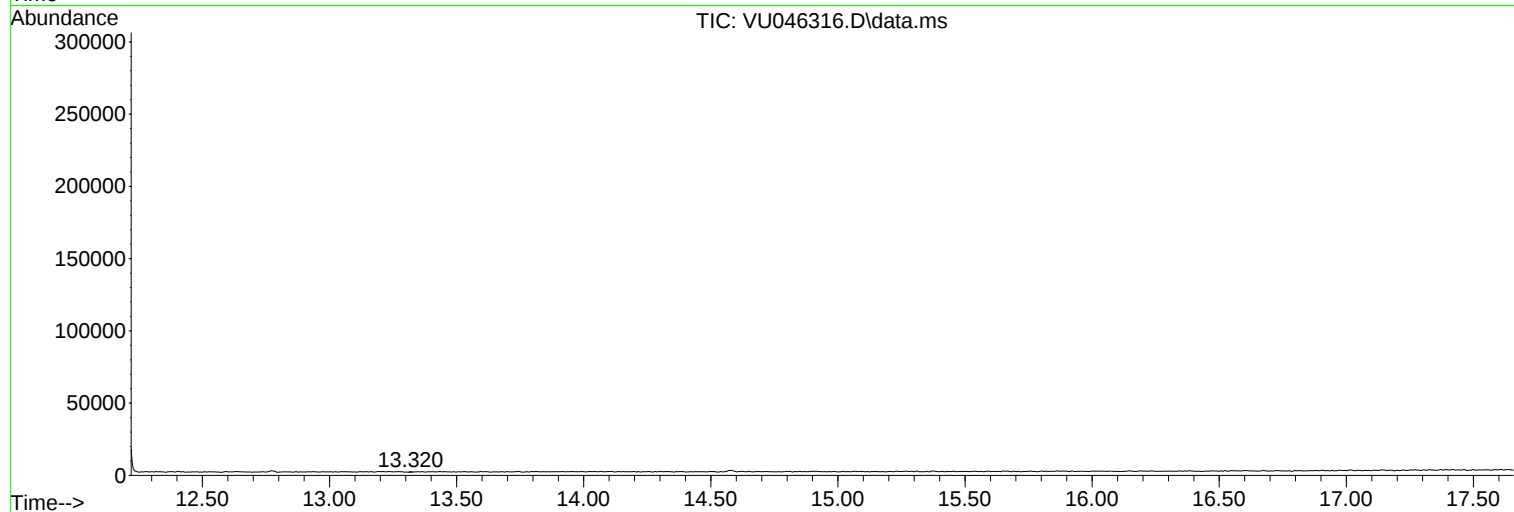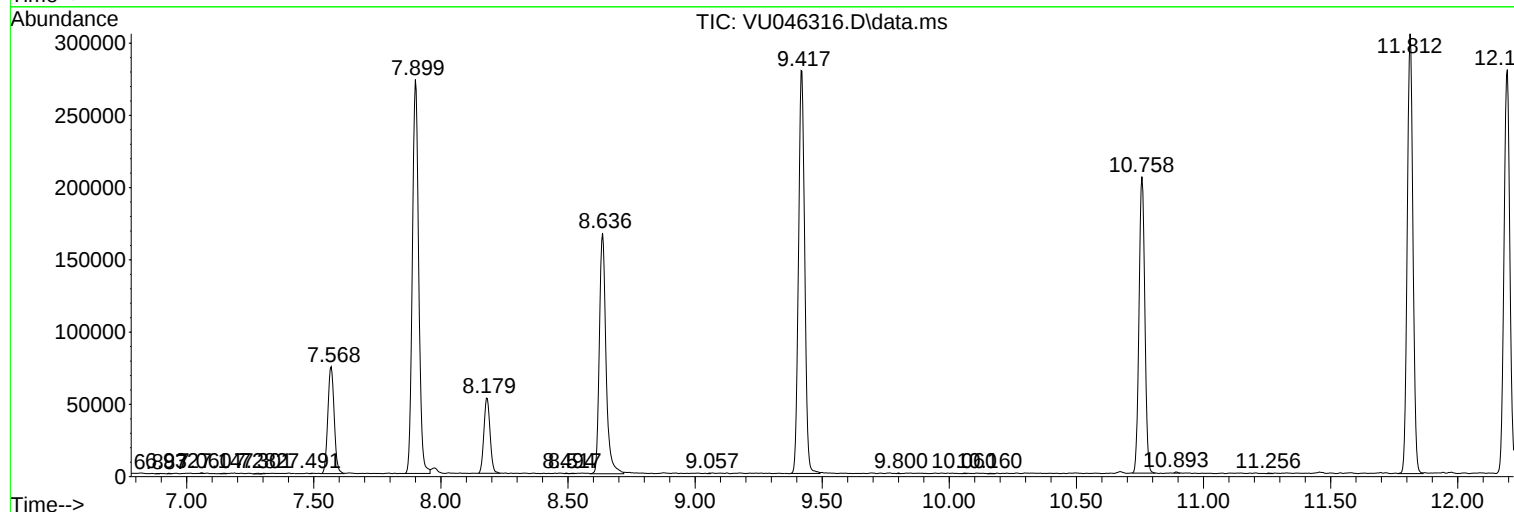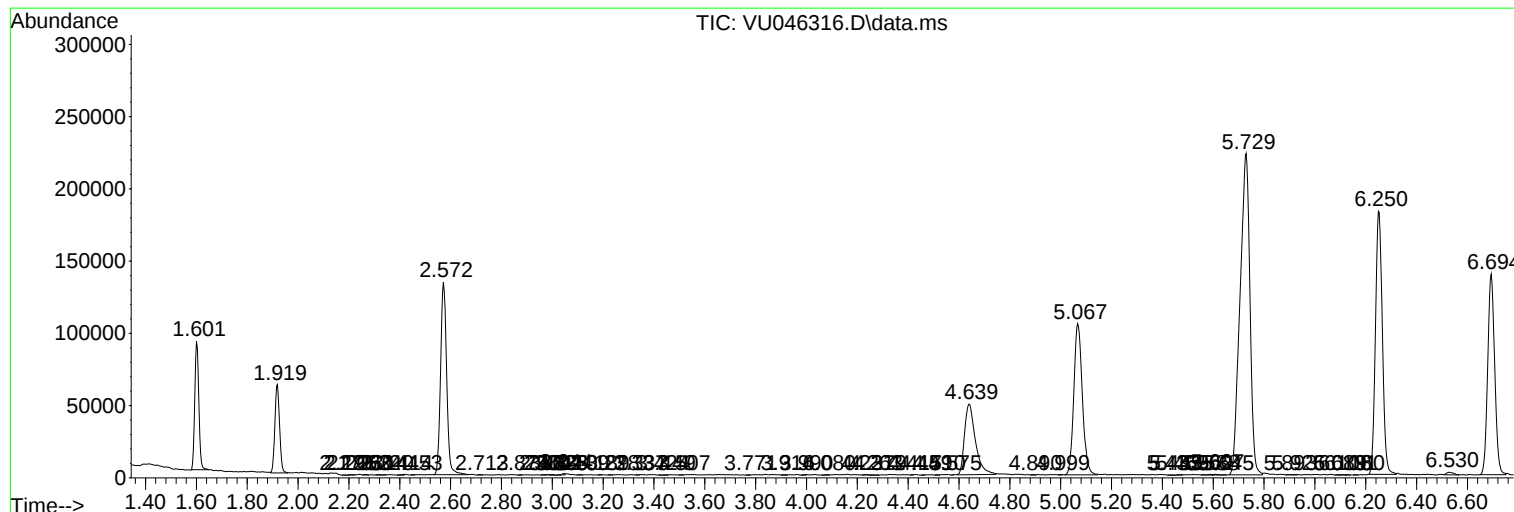

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046316.D
Acq On : 13 Dec 2021 15:29
Operator : SY/MD
Sample : M5004-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046316.D
Acq On : 13 Dec 2021 15:29
Operator : SY/MD
Sample : M5004-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc