

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046322.D
 Acq On : 13 Dec 2021 17:50
 Operator : SY/MD
 Sample : M4971-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

Signal : TIC: VU046322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	94	rVB	81975	89857	15.57%	1.961%
2	1.919	172	180	192	rVB	60092	75827	13.14%	1.655%
3	2.202	265	268	274	rVB2	462	420	0.07%	0.009%
4	2.234	274	278	279	rBV	460	283	0.05%	0.006%
5	2.285	291	294	297	rVB2	408	280	0.05%	0.006%
6	2.398	323	329	331	rBV2	459	407	0.07%	0.009%
7	2.572	371	383	401	rBV	121676	204199	35.39%	4.457%
8	2.803	452	455	458	rBV2	485	342	0.06%	0.007%
9	3.250	591	594	598	rBV	330	269	0.05%	0.006%
10	3.356	624	627	630	rBV	289	182	0.03%	0.004%
11	3.491	665	669	675	rBV2	635	775	0.13%	0.017%
12	3.520	675	678	679	rBV	130	78	0.01%	0.002%
13	3.777	753	758	762	rBV	563	534	0.09%	0.012%
14	3.906	792	798	803	rBV	481	525	0.09%	0.011%
15	4.015	828	832	836	rBV2	345	362	0.06%	0.008%
16	4.112	860	862	863	rBV2	338	165	0.03%	0.004%
17	4.150	870	874	880	rBV	382	498	0.09%	0.011%
18	4.218	892	895	897	rBV	254	161	0.03%	0.004%
19	4.308	918	923	928	rVB	525	577	0.10%	0.013%
20	4.404	951	953	959	rVB	436	401	0.07%	0.009%
21	4.436	959	963	966	rBV	337	337	0.06%	0.007%
22	4.517	984	988	997	rVB	494	635	0.11%	0.014%
23	4.575	1003	1006	1009	rBV2	342	259	0.04%	0.006%
24	4.639	1013	1026	1061	rVV2	49873	153571	26.61%	3.352%
25	4.993	1134	1136	1139	rVB	455	245	0.04%	0.005%
26	5.012	1139	1142	1143	rBV	274	142	0.02%	0.003%
27	5.067	1143	1159	1183	rVV	107990	248745	43.11%	5.430%
28	5.414	1263	1267	1274	rBV2	288	403	0.07%	0.009%
29	5.472	1280	1285	1290	rBV2	442	601	0.10%	0.013%
30	5.729	1343	1365	1395	rBV2	208126	577014	100.00%	12.595%
31	6.025	1454	1457	1458	rBV2	235	125	0.02%	0.003%
32	6.163	1497	1500	1503	rBV2	336	260	0.05%	0.006%
33	6.198	1507	1511	1513	rBV	573	447	0.08%	0.010%
34	6.253	1514	1528	1545	rBV	178985	332933	57.70%	7.267%
35	6.530	1607	1614	1623	rBV5	1603	2596	0.45%	0.057%
36	6.620	1637	1642	1644	rBV	335	288	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046322.D
 Acq On : 13 Dec 2021 17:50
 Operator : SY/MD
 Sample : M4971-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.694	1652	1665	1682	rBV	130884	252932	43.83%	5.521%
38	6.941	1739	1742	1745	rBV	314	242	0.04%	0.005%
39	6.977	1750	1753	1757	rBV2	232	193	0.03%	0.004%
40	7.137	1799	1803	1806	rBV2	356	292	0.05%	0.006%
41	7.157	1806	1809	1814	rVV	440	378	0.07%	0.008%
42	7.250	1835	1838	1839	rBV	261	169	0.03%	0.004%
43	7.350	1866	1869	1877	rVB2	524	617	0.11%	0.013%
44	7.411	1885	1888	1895	rBV	400	375	0.06%	0.008%
45	7.568	1925	1937	1954	rBV	72527	123791	21.45%	2.702%
46	7.655	1959	1964	1966	rBV2	282	285	0.05%	0.006%
47	7.700	1976	1978	1985	rVB	280	275	0.05%	0.006%
48	7.899	2026	2040	2055	rBV	250921	432511	74.96%	9.441%
49	8.047	2083	2086	2092	rVB2	623	458	0.08%	0.010%
50	8.182	2117	2128	2141	rBV	49923	83314	14.44%	1.819%
51	8.295	2160	2163	2166	rVB	399	250	0.04%	0.005%
52	8.314	2166	2169	2171	rVB	338	191	0.03%	0.004%
53	8.330	2171	2174	2176	rBV2	278	202	0.04%	0.004%
54	8.362	2181	2184	2186	rBV	249	185	0.03%	0.004%
55	8.417	2197	2201	2204	rBV2	397	318	0.06%	0.007%
56	8.475	2211	2219	2232	rVB2	5100	8674	1.50%	0.189%
57	8.636	2257	2269	2296	rBV	160500	283689	49.17%	6.193%
58	8.787	2308	2316	2328	rBV4	9898	18265	3.17%	0.399%
59	8.870	2340	2342	2344	rBV	214	137	0.02%	0.003%
60	8.944	2361	2365	2369	rBV2	396	333	0.06%	0.007%
61	9.083	2405	2408	2411	rBV	285	232	0.04%	0.005%
62	9.420	2500	2513	2534	rBV	273757	453100	78.52%	9.891%
63	9.774	2620	2623	2627	rBV	366	309	0.05%	0.007%
64	10.028	2699	2702	2705	rVB	355	197	0.03%	0.004%
65	10.343	2797	2800	2808	rVB4	659	757	0.13%	0.017%
66	10.758	2918	2929	2942	rBV	194425	306828	53.18%	6.698%
67	10.893	2963	2971	2981	rVB2	9146	13583	2.35%	0.296%
68	11.002	2998	3005	3007	rBV2	629	791	0.14%	0.017%
69	11.298	3090	3097	3102	rBV2	704	1010	0.18%	0.022%
70	11.472	3140	3151	3162	rBV5	3188	5910	1.02%	0.129%
71	11.574	3180	3183	3186	rBV2	448	292	0.05%	0.006%
72	11.693	3215	3220	3225	rVB4	987	1169	0.20%	0.026%
73	11.812	3245	3257	3275	rVB	293926	459965	79.71%	10.040%
74	12.060	3327	3334	3343	rBV5	4164	6627	1.15%	0.145%
75	12.195	3364	3376	3391	rVB	262653	417748	72.40%	9.119%
76	12.549	3480	3486	3492	rBV4	1016	1375	0.24%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046322.D
Acq On : 13 Dec 2021 17:50
Operator : SY/MD
Sample : M4971-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis

77	12.774	3547	3556	3564	rBV3	2894	4729	0.82%	0.103%
78	12.889	3586	3592	3600	rBV4	3269	3715	0.64%	0.081%




Sum of corrected areas: 4581156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046322.D
Acq On : 13 Dec 2021 17:50
Operator : SY/MD
Sample : M4971-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

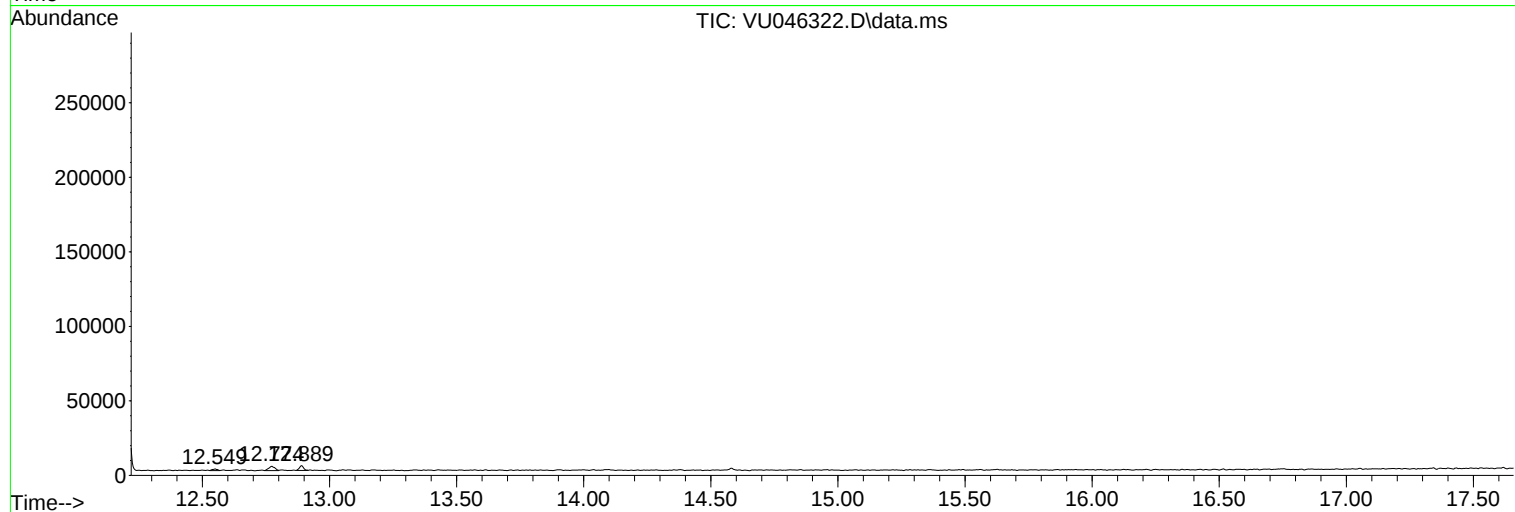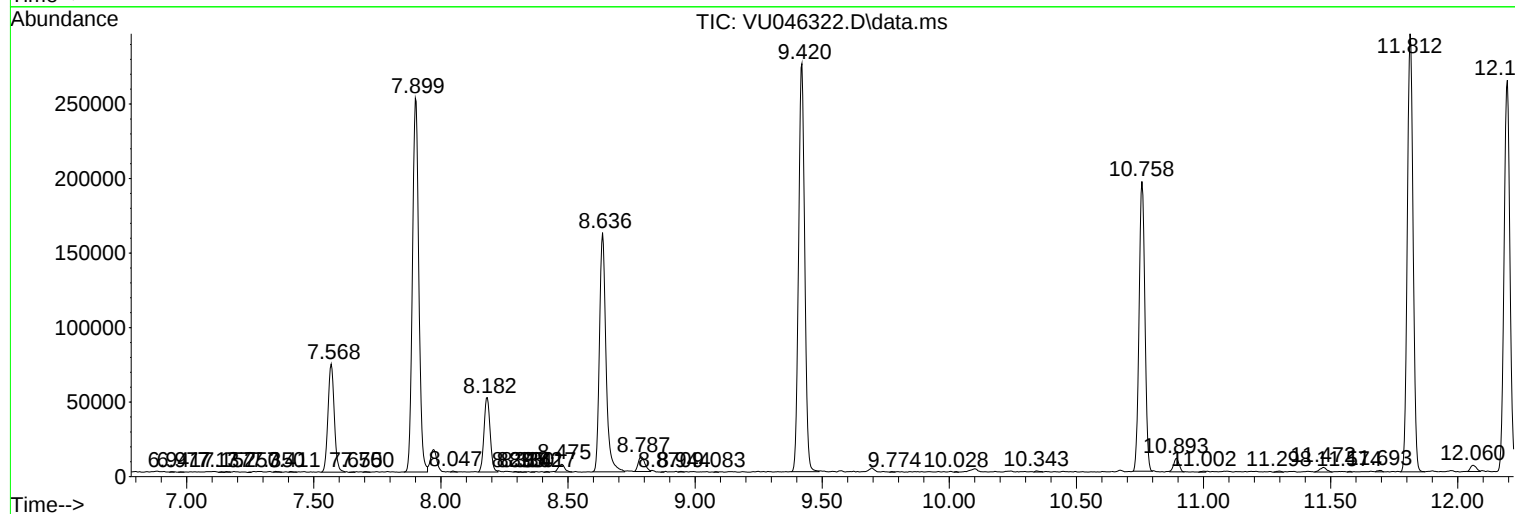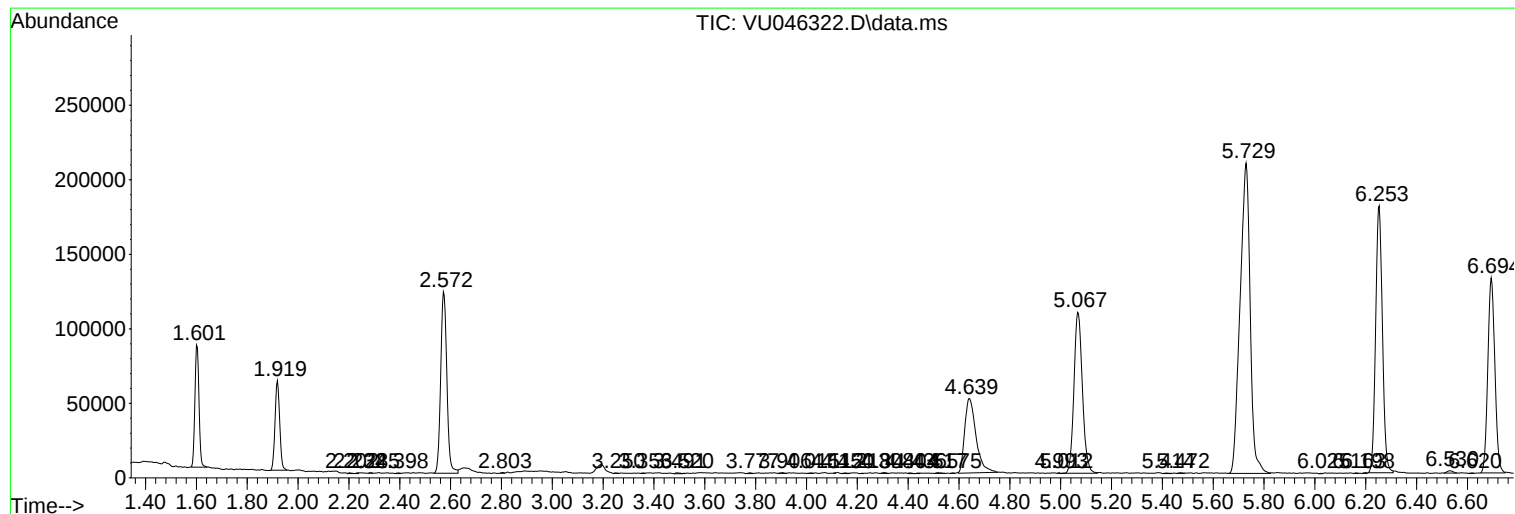

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046322.D
Acq On : 13 Dec 2021 17:50
Operator : SY/MD
Sample : M4971-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046322.D
Acq On : 13 Dec 2021 17:50
Operator : SY/MD
Sample : M4971-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc