

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046323.D
 Acq On : 13 Dec 2021 18:13
 Operator : SY/MD
 Sample : M4971-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	103	rVB	78354	89864	16.26%	2.006%
2	1.919	172	180	193	rVB	57938	72391	13.10%	1.616%
3	2.212	268	271	276	rVB3	296	296	0.05%	0.007%
4	2.253	281	284	288	rVV2	477	381	0.07%	0.009%
5	2.276	288	291	298	rVB2	385	465	0.08%	0.010%
6	2.318	298	304	305	rBV2	434	412	0.07%	0.009%
7	2.337	308	310	316	rVB2	650	499	0.09%	0.011%
8	2.401	324	330	334	rBB2	360	361	0.07%	0.008%
9	2.572	370	383	399	rBV	117424	195065	35.29%	4.354%
10	2.745	435	437	443	rVB2	599	500	0.09%	0.011%
11	2.890	477	482	486	rBV2	515	601	0.11%	0.013%
12	2.951	493	501	502	rBV2	584	646	0.12%	0.014%
13	3.192	566	576	587	rBV4	2122	4696	0.85%	0.105%
14	3.337	614	621	627	rVB	528	880	0.16%	0.020%
15	3.382	632	635	639	rVV2	337	297	0.05%	0.007%
16	3.411	639	644	653	rVV2	453	623	0.11%	0.014%
17	3.482	658	666	668	rBV	289	334	0.06%	0.007%
18	3.594	691	701	704	rBV2	447	666	0.12%	0.015%
19	3.639	711	715	724	rVB	419	641	0.12%	0.014%
20	3.883	789	791	796	rVB	436	362	0.07%	0.008%
21	4.205	887	891	896	rVB2	328	292	0.05%	0.007%
22	4.314	922	925	929	rVB	455	343	0.06%	0.008%
23	4.346	931	935	937	rBV2	421	355	0.06%	0.008%
24	4.427	954	960	963	rBV	397	453	0.08%	0.010%
25	4.639	1012	1026	1064	rBV	44815	141966	25.69%	3.169%
26	4.877	1093	1100	1105	rBV3	354	524	0.09%	0.012%
27	5.067	1140	1159	1183	rBV	102583	237060	42.89%	5.291%
28	5.343	1239	1245	1247	rBV	356	365	0.07%	0.008%
29	5.430	1266	1272	1274	rBV	460	396	0.07%	0.009%
30	5.729	1343	1365	1397	rBV2	199693	552678	100.00%	12.336%
31	5.928	1420	1427	1432	rBV	341	491	0.09%	0.011%
32	5.964	1432	1438	1443	rVB2	279	353	0.06%	0.008%
33	6.192	1505	1509	1512	rBV	351	317	0.06%	0.007%
34	6.253	1513	1528	1549	rBV	177132	335246	60.66%	7.483%
35	6.440	1581	1586	1588	rBV	354	310	0.06%	0.007%
36	6.456	1588	1591	1596	rVB2	465	437	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046323.D
 Acq On : 13 Dec 2021 18:13
 Operator : SY/MD
 Sample : M4971-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.533	1607	1615	1623	rBV3	1722	2681	0.49%	0.060%
38	6.694	1651	1665	1682	rVV	124894	243983	44.15%	5.446%
39	6.899	1723	1729	1734	rVB3	535	725	0.13%	0.016%
40	6.996	1756	1759	1762	rBV	599	451	0.08%	0.010%
41	7.083	1782	1786	1790	rBV	379	466	0.08%	0.010%
42	7.231	1828	1832	1835	rBV	409	313	0.06%	0.007%
43	7.282	1844	1848	1853	rBV	288	346	0.06%	0.008%
44	7.459	1898	1903	1906	rBV	270	312	0.06%	0.007%
45	7.568	1925	1937	1951	rVV	65920	116112	21.01%	2.592%
46	7.690	1970	1975	1978	rBV	539	560	0.10%	0.012%
47	7.739	1983	1990	1993	rBV	524	529	0.10%	0.012%
48	7.899	2027	2040	2055	rBV	237516	412580	74.65%	9.209%
49	7.973	2057	2063	2075	rVB2	8884	14010	2.53%	0.313%
50	8.092	2095	2100	2104	rBV	562	523	0.09%	0.012%
51	8.182	2117	2128	2143	rBV	47330	78503	14.20%	1.752%
52	8.449	2207	2211	2212	rBV	640	409	0.07%	0.009%
53	8.475	2212	2219	2226	rVB4	3486	5617	1.02%	0.125%
54	8.636	2256	2269	2294	rVV	156051	280577	50.77%	6.263%
55	8.790	2308	2317	2330	rBV4	9013	14951	2.71%	0.334%
56	8.977	2371	2375	2381	rVB2	441	437	0.08%	0.010%
57	9.022	2381	2389	2391	rBV	408	561	0.10%	0.013%
58	9.231	2450	2454	2458	rVB2	454	373	0.07%	0.008%
59	9.272	2458	2467	2468	rBV	330	406	0.07%	0.009%
60	9.420	2499	2513	2537	rBV	275643	455218	82.37%	10.161%
61	9.559	2552	2556	2558	rBV	413	294	0.05%	0.007%
62	9.575	2558	2561	2567	rVB	505	464	0.08%	0.010%
63	9.694	2592	2598	2603	rBV2	1243	1612	0.29%	0.036%
64	9.835	2639	2642	2646	rVB	467	316	0.06%	0.007%
65	10.208	2753	2758	2761	rVB2	342	359	0.06%	0.008%
66	10.234	2761	2766	2772	rBV4	717	1066	0.19%	0.024%
67	10.349	2790	2802	2806	rBV3	833	1299	0.24%	0.029%
68	10.671	2896	2902	2910	rBV3	857	1070	0.19%	0.024%
69	10.758	2917	2929	2945	rVV	191851	302549	54.74%	6.753%
70	10.893	2963	2971	2982	rVB2	5752	8694	1.57%	0.194%
71	10.967	2991	2994	3002	rVB2	365	457	0.08%	0.010%
72	11.005	3002	3006	3010	rBV	461	477	0.09%	0.011%
73	11.275	3084	3090	3093	rVB	366	364	0.07%	0.008%
74	11.295	3093	3096	3100	rVB2	553	395	0.07%	0.009%
75	11.324	3100	3105	3108	rBV	283	302	0.05%	0.007%
76	11.468	3142	3150	3160	rVB5	2420	4151	0.75%	0.093%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046323.D
 Acq On : 13 Dec 2021 18:13
 Operator : SY/MD
 Sample : M4971-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.693	3214	3220	3228	rBV5	749	1029	0.19%	0.023%
78	11.812	3245	3257	3275	rVB	295003	456284	82.56%	10.184%
79	11.886	3275	3280	3281	rBV	409	313	0.06%	0.007%
80	11.970	3303	3306	3317	rVB4	853	1175	0.21%	0.026%
81	12.063	3325	3335	3345	rBV5	4249	7655	1.39%	0.171%
82	12.195	3362	3376	3390	rBV	253861	403257	72.96%	9.001%
83	12.317	3410	3414	3418	rBV2	549	532	0.10%	0.012%
84	12.777	3549	3557	3567	rVB3	2377	3694	0.67%	0.082%
85	12.828	3571	3573	3578	rVB	497	308	0.06%	0.007%
86	12.890	3584	3592	3598	rBV4	2700	3146	0.57%	0.070%
87	13.002	3624	3627	3631	rBV2	467	411	0.07%	0.009%
88	13.102	3651	3658	3662	rBV	486	591	0.11%	0.013%
89	13.176	3678	3681	3684	rBV	431	358	0.06%	0.008%
90	13.491	3775	3779	3782	rBV	376	325	0.06%	0.007%
91	13.603	3811	3814	3818	rBV2	434	342	0.06%	0.008%
92	13.764	3860	3864	3868	rVV	365	469	0.08%	0.010%
93	14.005	3935	3939	3942	rBV	458	432	0.08%	0.010%
94	14.086	3954	3964	3967	rBV2	994	1609	0.29%	0.036%
95	14.214	4001	4004	4008	rVB2	467	348	0.06%	0.008%
96	14.340	4040	4043	4047	rBV2	436	357	0.06%	0.008%
97	14.996	4242	4247	4249	rBV2	371	330	0.06%	0.007%
98	16.028	4564	4568	4571	rBV2	578	552	0.10%	0.012%
99	16.343	4663	4666	4667	rBV2	475	296	0.05%	0.007%
100	17.066	4889	4891	4893	rBV	561	311	0.06%	0.007%




Sum of corrected areas: 4480202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046323.D
Acq On : 13 Dec 2021 18:13
Operator : SY/MD
Sample : M4971-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

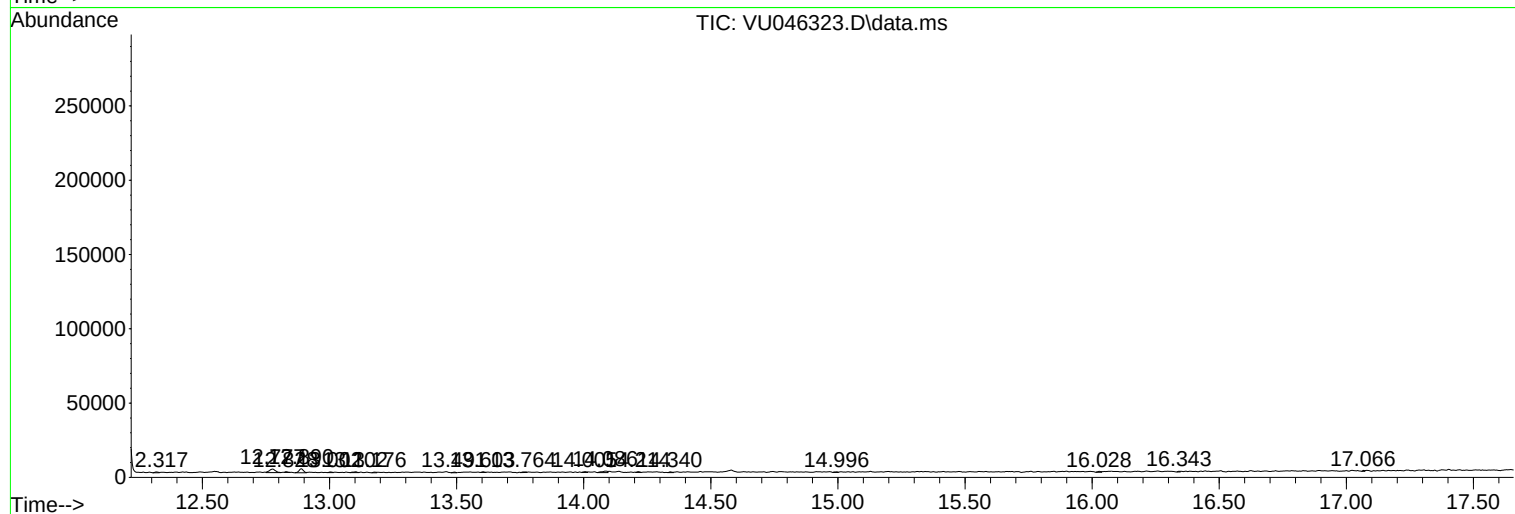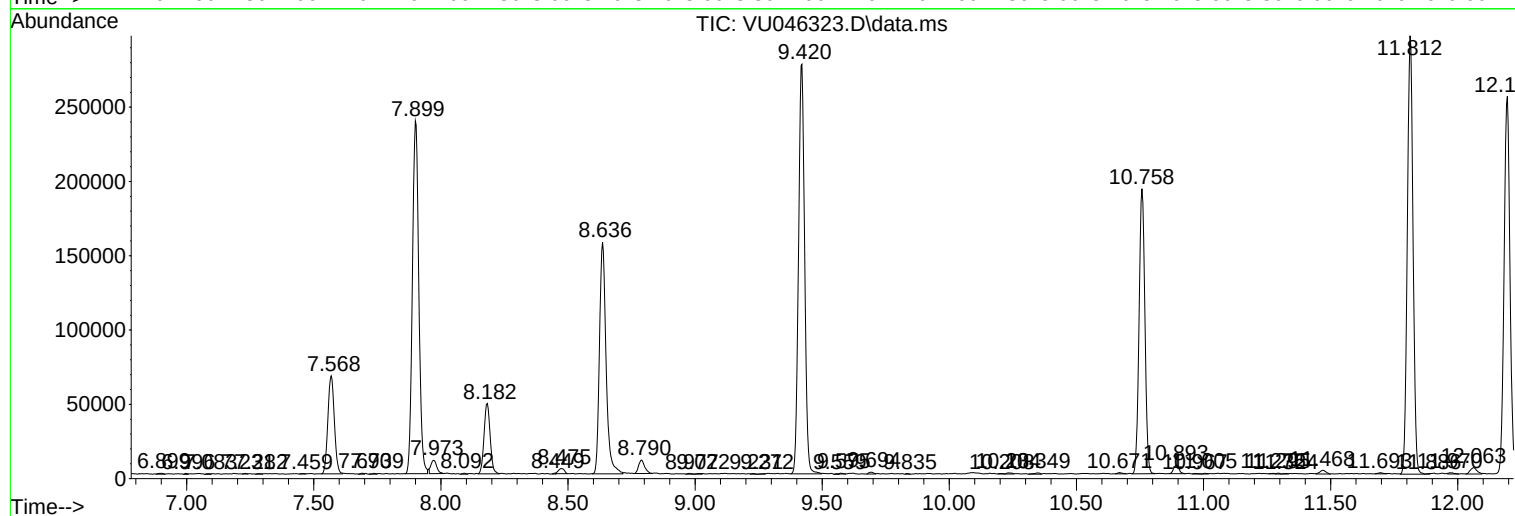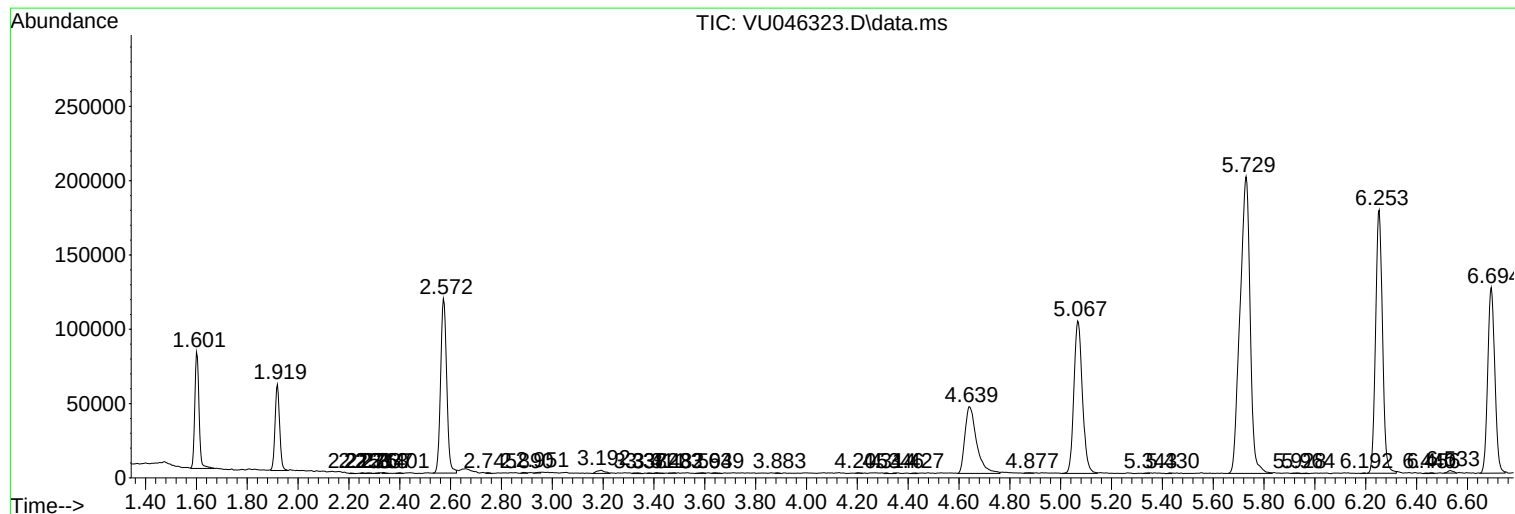

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046323.D
Acq On : 13 Dec 2021 18:13
Operator : SY/MD
Sample : M4971-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046323.D
Acq On : 13 Dec 2021 18:13
Operator : SY/MD
Sample : M4971-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc