

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046332.D
 Acq On : 13 Dec 2021 21:35
 Operator : SY/MD
 Sample : M5023-06ME
 Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKY2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	59152	86989	15.64%	1.888%
2	1.916	172	179	202	rVB	31980	61653	11.08%	1.338%
3	2.549	364	376	392	rBV	104319	173002	31.10%	3.754%
4	2.919	489	491	492	rBV	203	88	0.02%	0.002%
5	3.179	561	572	591	rBV2	8105	20942	3.76%	0.454%
6	3.369	627	631	633	rBV	377	281	0.05%	0.006%
7	3.423	646	648	654	rVB	378	278	0.05%	0.006%
8	3.452	654	657	659	rBV2	198	117	0.02%	0.003%
9	3.469	659	662	666	rBV	442	294	0.05%	0.006%
10	3.632	710	713	717	rVB2	398	251	0.05%	0.005%
11	3.658	717	721	723	rBV2	314	259	0.05%	0.006%
12	3.835	773	776	778	rBV	297	136	0.02%	0.003%
13	3.854	778	782	783	rBV	338	220	0.04%	0.005%
14	4.002	821	828	833	rBV2	544	876	0.16%	0.019%
15	4.169	877	880	883	rBV	348	229	0.04%	0.005%
16	4.189	883	886	889	rVV	290	191	0.03%	0.004%
17	4.205	889	891	893	rVV	259	120	0.02%	0.003%
18	4.218	893	895	900	rVV2	117	97	0.02%	0.002%
19	4.311	922	924	926	rVB2	216	100	0.02%	0.002%
20	4.330	926	930	934	rBV2	358	422	0.08%	0.009%
21	4.388	945	948	954	rVB2	380	356	0.06%	0.008%
22	4.420	954	958	962	rBV	338	281	0.05%	0.006%
23	4.446	962	966	969	rBV	362	331	0.06%	0.007%
24	4.517	985	988	992	rVB	262	168	0.03%	0.004%
25	4.539	992	995	997	rVB	284	129	0.02%	0.003%
26	4.565	997	1003	1005	rBV2	424	452	0.08%	0.010%
27	4.597	1010	1013	1016	rBV2	509	463	0.08%	0.010%
28	4.661	1018	1033	1051	rBV2	23777	91062	16.37%	1.976%
29	5.067	1143	1159	1185	rVB	91438	226458	40.71%	4.914%
30	5.173	1188	1192	1196	rBV	408	378	0.07%	0.008%
31	5.407	1261	1265	1268	rBV	263	295	0.05%	0.006%
32	5.507	1292	1296	1298	rBV2	274	195	0.04%	0.004%
33	5.629	1331	1334	1337	rBV	312	170	0.03%	0.004%
34	5.722	1343	1363	1383	rBV2	217262	556293	100.00%	12.072%
35	5.902	1414	1419	1421	rBV2	270	278	0.05%	0.006%
36	5.983	1434	1444	1458	rBV6	3235	8692	1.56%	0.189%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046332.D
 Acq On : 13 Dec 2021 21:35
 Operator : SY/MD
 Sample : M5023-06ME
 Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKY2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.108	1480	1483	1488	rVB	312	267	0.05%	0.006%
38	6.131	1488	1490	1493	rVB2	134	58	0.01%	0.001%
39	6.160	1493	1499	1502	rBV3	462	416	0.07%	0.009%
40	6.250	1513	1527	1554	rBV	201752	409426	73.60%	8.885%
41	6.529	1606	1614	1620	rBV6	2792	5095	0.92%	0.111%
42	6.597	1627	1635	1637	rBV2	1157	1340	0.24%	0.029%
43	6.693	1650	1665	1691	rVB	120557	249111	44.78%	5.406%
44	7.115	1793	1796	1799	rBV2	309	189	0.03%	0.004%
45	7.221	1826	1829	1831	rBV3	429	292	0.05%	0.006%
46	7.298	1845	1853	1858	rBV3	558	950	0.17%	0.021%
47	7.349	1866	1869	1870	rBV	258	143	0.03%	0.003%
48	7.385	1876	1880	1883	rBV	331	267	0.05%	0.006%
49	7.481	1906	1910	1912	rBV	333	308	0.06%	0.007%
50	7.568	1924	1937	1961	rBV2	59109	121773	21.89%	2.642%
51	7.693	1973	1976	1978	rBV	215	143	0.03%	0.003%
52	7.899	2026	2040	2058	rBV	233584	437235	78.60%	9.488%
53	8.185	2117	2129	2153	rBV2	35143	80545	14.48%	1.748%
54	8.295	2161	2163	2166	rBV	224	171	0.03%	0.004%
55	8.391	2190	2193	2195	rBV	307	208	0.04%	0.005%
56	8.555	2233	2244	2259	rVB	28879	49318	8.87%	1.070%
57	8.681	2262	2283	2315	rBV2	81593	251385	45.19%	5.455%
58	8.893	2346	2349	2350	rBV	351	203	0.04%	0.004%
59	9.217	2447	2450	2452	rBV	275	171	0.03%	0.004%
60	9.234	2452	2455	2462	rVB2	501	496	0.09%	0.011%
61	9.269	2463	2466	2467	rBV2	288	161	0.03%	0.003%
62	9.320	2478	2482	2485	rBV	337	301	0.05%	0.007%
63	9.426	2500	2515	2536	rBV	248352	545775	98.11%	11.843%
64	9.584	2561	2564	2568	rBV	335	276	0.05%	0.006%
65	9.642	2579	2582	2585	rBV	199	112	0.02%	0.002%
66	9.703	2594	2601	2607	rBV2	692	958	0.17%	0.021%
67	9.745	2612	2614	2618	rBV	359	251	0.05%	0.005%
68	9.825	2635	2639	2645	rBV2	501	545	0.10%	0.012%
69	10.031	2698	2703	2706	rBV2	347	354	0.06%	0.008%
70	10.295	2777	2785	2790	rBV	598	922	0.17%	0.020%
71	10.391	2811	2815	2817	rBV	398	279	0.05%	0.006%
72	10.449	2829	2833	2835	rBV2	451	369	0.07%	0.008%
73	10.481	2840	2843	2846	rBV	243	151	0.03%	0.003%
74	10.597	2875	2879	2883	rBV	430	411	0.07%	0.009%
75	10.716	2910	2916	2920	rBV	379	517	0.09%	0.011%
76	10.770	2920	2933	2948	rVV	170517	285189	51.27%	6.189%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046332.D
 Acq On : 13 Dec 2021 21:35
 Operator : SY/MD
 Sample : M5023-06ME
 Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKY2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	10.931	2980	2983	2988	rVB2	524	354	0.06%	0.008%
78	10.960	2988	2992	2994	rBV2	300	247	0.04%	0.005%
79	11.002	2999	3005	3009	rBV	617	741	0.13%	0.016%
80	11.034	3012	3015	3017	rBV	324	223	0.04%	0.005%
81	11.118	3036	3041	3046	rBV4	912	1038	0.19%	0.023%
82	11.378	3119	3122	3124	rBV2	347	240	0.04%	0.005%
83	11.452	3139	3145	3146	rBV2	546	552	0.10%	0.012%
84	11.581	3180	3185	3188	rBV2	523	456	0.08%	0.010%
85	11.693	3217	3220	3222	rBV2	366	226	0.04%	0.005%
86	11.819	3247	3259	3274	rBV	348851	533592	95.92%	11.579%
87	11.905	3282	3286	3287	rBB	72	96	0.02%	0.002%
88	12.201	3364	3378	3398	rVB	242272	389651	70.04%	8.455%
89	12.484	3463	3466	3467	rBV	267	154	0.03%	0.003%
90	12.523	3474	3478	3482	rBV	536	539	0.10%	0.012%
91	12.970	3614	3617	3619	rBV	269	155	0.03%	0.003%
92	13.719	3846	3850	3853	rBV2	277	248	0.04%	0.005%
93	14.143	3976	3982	3986	rBV2	575	727	0.13%	0.016%
94	14.298	4028	4030	4034	rBV	315	214	0.04%	0.005%
95	14.751	4168	4171	4173	rBV	316	189	0.03%	0.004%




Sum of corrected areas: 4608269

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046332.D
Acq On : 13 Dec 2021 21:35
Operator : SY/MD
Sample : M5023-06ME
Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKY2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

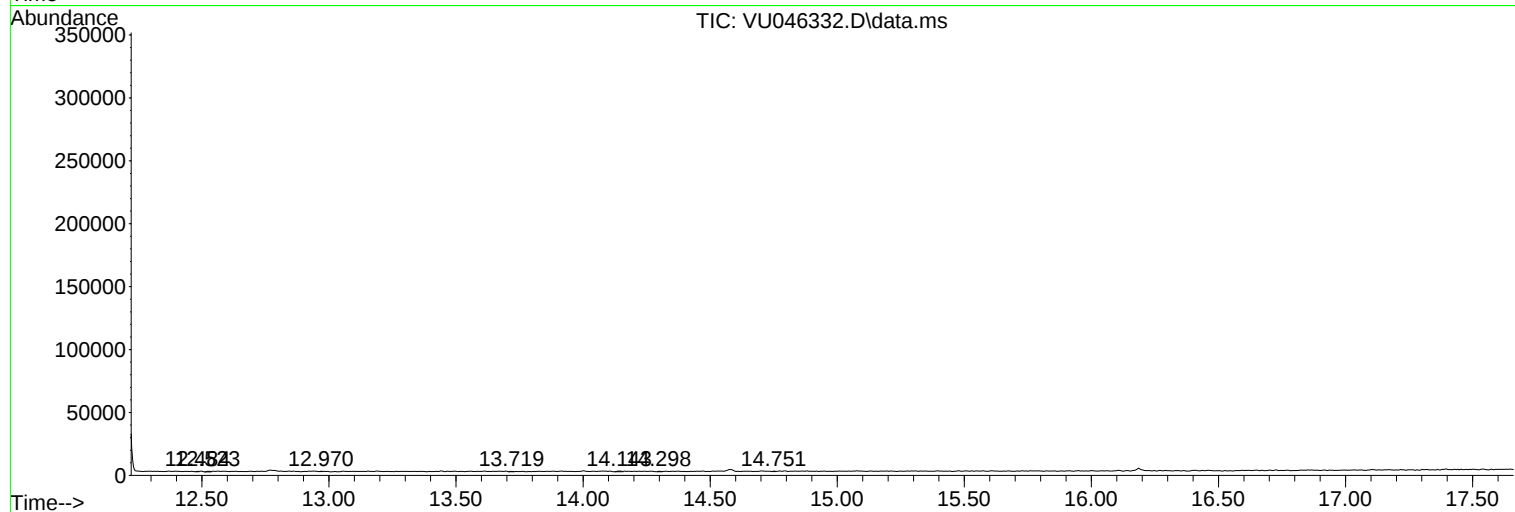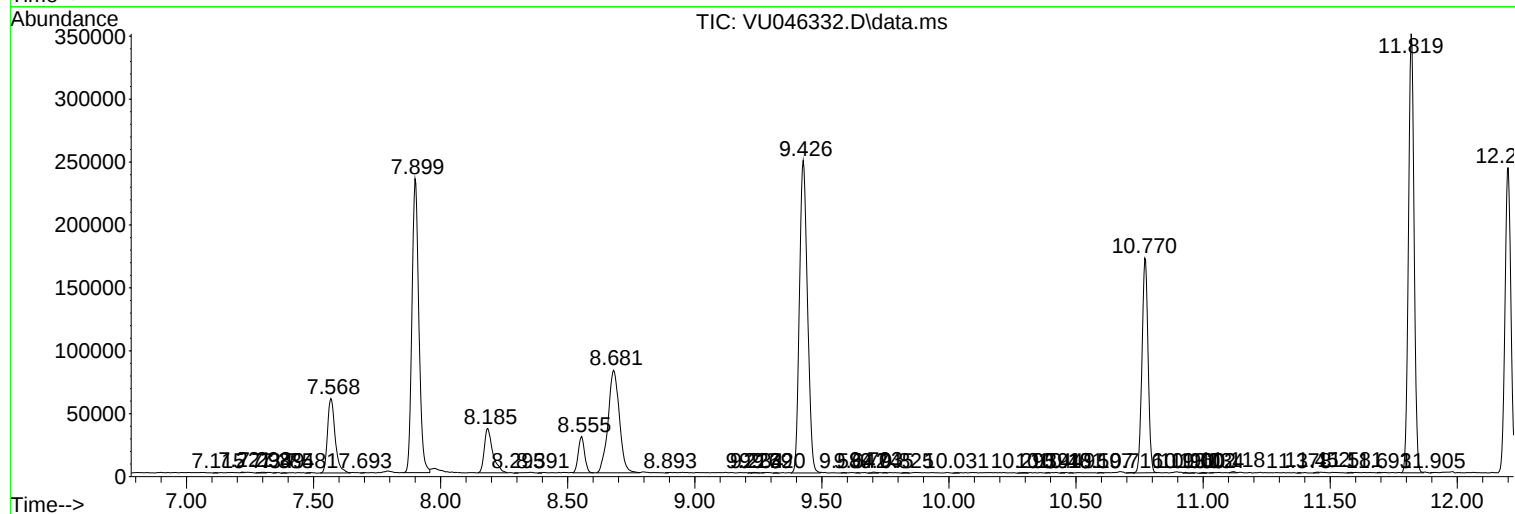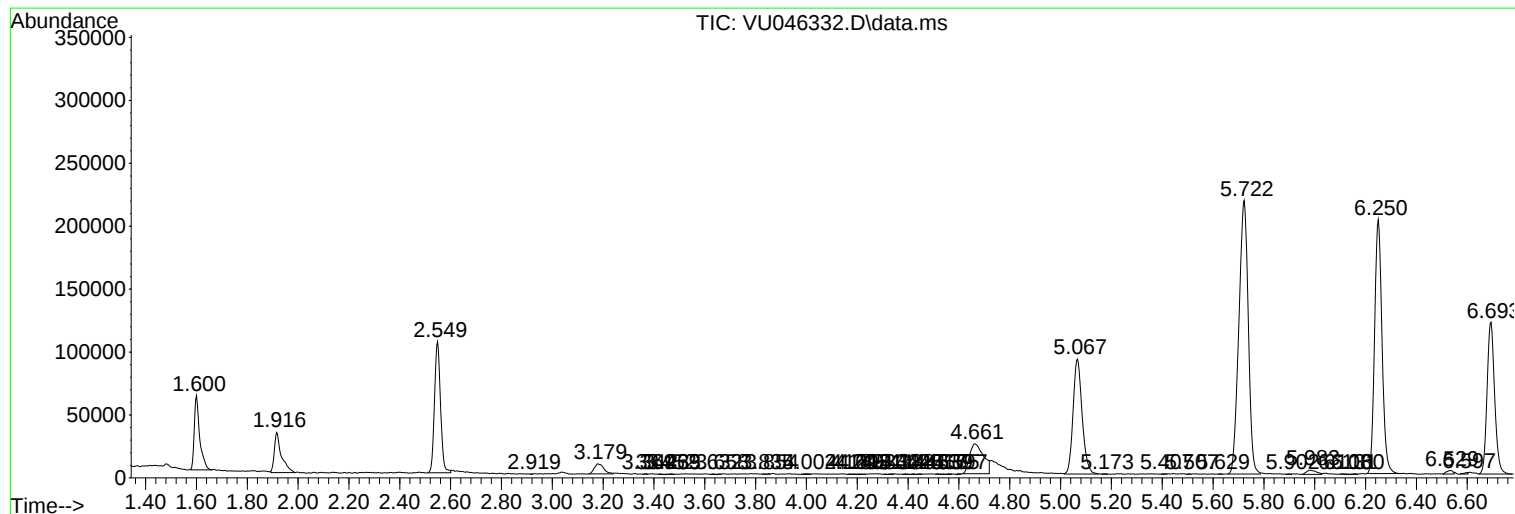

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046332.D
Acq On : 13 Dec 2021 21:35
Operator : SY/MD
Sample : M5023-06ME
Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKY2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046332.D
Acq On : 13 Dec 2021 21:35
Operator : SY/MD
Sample : M5023-06ME
Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKY2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc