

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046337.D
 Acq On : 13 Dec 2021 23:27
 Operator : SY/MD
 Sample : M5062-03 20X
 Misc : 6.77g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	75	81	98	rVB	73841	82118	15.56%	1.866%
2	1.919	172	180	193	rVB	52579	66691	12.64%	1.515%
3	2.289	288	295	298	rBV2	562	547	0.10%	0.012%
4	2.440	335	342	347	rBV	489	745	0.14%	0.017%
5	2.497	357	360	365	rVV2	322	332	0.06%	0.008%
6	2.571	371	383	409	rBV	113438	187701	35.58%	4.264%
7	2.825	458	462	464	rBV	463	333	0.06%	0.008%
8	2.896	480	484	490	rBV	430	408	0.08%	0.009%
9	3.051	520	532	542	rBV4	2737	5195	0.98%	0.118%
10	3.124	552	555	560	rBV	301	299	0.06%	0.007%
11	3.189	565	575	588	rVV2	3745	7938	1.50%	0.180%
12	3.240	588	591	596	rVB3	409	298	0.06%	0.007%
13	3.391	631	638	642	rBV	390	491	0.09%	0.011%
14	3.542	682	685	689	rVB2	460	314	0.06%	0.007%
15	3.568	689	693	698	rBV2	422	427	0.08%	0.010%
16	3.652	716	719	724	rVB	532	488	0.09%	0.011%
17	3.681	724	728	731	rBV	356	324	0.06%	0.007%
18	3.697	731	733	737	rVB2	575	406	0.08%	0.009%
19	3.719	737	740	742	rBV2	479	310	0.06%	0.007%
20	3.870	785	787	791	rVV3	499	380	0.07%	0.009%
21	4.121	860	865	868	rBV2	293	322	0.06%	0.007%
22	4.362	937	940	945	rVB2	362	335	0.06%	0.008%
23	4.391	945	949	956	rBV2	387	500	0.09%	0.011%
24	4.423	956	959	964	rVB	490	421	0.08%	0.010%
25	4.452	964	968	970	rBV2	354	266	0.05%	0.006%
26	4.536	990	994	999	rVB2	337	341	0.06%	0.008%
27	4.565	999	1003	1005	rBV2	430	360	0.07%	0.008%
28	4.642	1013	1027	1061	rBV2	40259	133741	25.35%	3.038%
29	4.864	1093	1096	1099	rVB	343	242	0.05%	0.005%
30	5.067	1144	1159	1180	rBV2	91496	215170	40.78%	4.888%
31	5.157	1184	1187	1194	rVB3	474	471	0.09%	0.011%
32	5.208	1198	1203	1209	rBV2	354	483	0.09%	0.011%
33	5.321	1226	1238	1250	rVV3	4982	10135	1.92%	0.230%
34	5.401	1255	1263	1266	rBV	439	577	0.11%	0.013%
35	5.465	1277	1283	1286	rBV	254	334	0.06%	0.008%
36	5.613	1327	1329	1335	rVB2	340	273	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046337.D
 Acq On : 13 Dec 2021 23:27
 Operator : SY/MD
 Sample : M5062-03 20X
 Misc : 6.77g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	5.645	1335	1339	1342	rBV	465	391	0.07%	0.009%
38	5.729	1342	1365	1387	rBV2	197589	527617	100.00%	11.987%
39	6.140	1489	1493	1496	rBV	291	262	0.05%	0.006%
40	6.253	1512	1528	1551	rBV	186943	356730	67.61%	8.104%
41	6.539	1607	1617	1627	rBV7	2445	4866	0.92%	0.111%
42	6.693	1651	1665	1683	rVV	122559	235987	44.73%	5.361%
43	7.108	1790	1794	1797	rBV2	312	318	0.06%	0.007%
44	7.259	1839	1841	1844	rVV2	467	267	0.05%	0.006%
45	7.430	1890	1894	1899	rBV	431	464	0.09%	0.011%
46	7.568	1924	1937	1953	rBV	63389	110598	20.96%	2.513%
47	7.722	1982	1985	1988	rVB	465	282	0.05%	0.006%
48	7.787	2000	2005	2008	rBV2	485	459	0.09%	0.010%
49	7.899	2028	2040	2058	rBV	231873	397894	75.41%	9.040%
50	7.973	2058	2063	2072	rVB2	3264	4817	0.91%	0.109%
51	8.050	2082	2087	2091	rBV2	355	373	0.07%	0.008%
52	8.182	2117	2128	2142	rVV	45484	75331	14.28%	1.711%
53	8.555	2235	2244	2257	rBV2	15570	25354	4.81%	0.576%
54	8.636	2257	2269	2292	rBV	148265	270389	51.25%	6.143%
55	8.909	2349	2354	2356	rBV2	1016	854	0.16%	0.019%
56	8.970	2369	2373	2377	rBV2	324	312	0.06%	0.007%
57	9.099	2410	2413	2417	rVB	467	312	0.06%	0.007%
58	9.420	2500	2513	2532	rVV	290767	476076	90.23%	10.816%
59	9.533	2546	2548	2554	rVB2	491	342	0.06%	0.008%
60	9.587	2562	2565	2570	rBV	390	416	0.08%	0.009%
61	9.729	2605	2609	2613	rBV	447	447	0.08%	0.010%
62	9.783	2622	2626	2630	rBV	366	395	0.07%	0.009%
63	10.079	2715	2718	2725	rVB2	250	341	0.06%	0.008%
64	10.214	2755	2760	2763	rBV2	493	485	0.09%	0.011%
65	10.282	2778	2781	2784	rBV	326	256	0.05%	0.006%
66	10.385	2810	2813	2816	rVB	389	241	0.05%	0.005%
67	10.510	2847	2852	2857	rBV2	320	438	0.08%	0.010%
68	10.603	2878	2881	2884	rBV2	380	253	0.05%	0.006%
69	10.671	2898	2902	2909	rVB2	1209	1382	0.26%	0.031%
70	10.758	2917	2929	2946	rVV	186824	296978	56.29%	6.747%
71	10.893	2968	2971	2976	rBV	465	399	0.08%	0.009%
72	10.938	2982	2985	2989	rBV	413	405	0.08%	0.009%
73	11.198	3063	3066	3070	rBV	310	249	0.05%	0.006%
74	11.333	3103	3108	3112	rVB	567	609	0.12%	0.014%
75	11.365	3112	3118	3121	rBV	319	373	0.07%	0.008%
76	11.465	3145	3149	3151	rVV4	501	444	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046337.D
 Acq On : 13 Dec 2021 23:27
 Operator : SY/MD
 Sample : M5062-03 20X
 Misc : 6.77g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.754	3237	3239	3243	rVV	355	272	0.05%	0.006%
78	11.812	3245	3257	3275	rVV	309655	481318	91.22%	10.935%
79	11.934	3291	3295	3296	rBV	410	269	0.05%	0.006%
80	11.967	3301	3305	3311	rVB4	674	784	0.15%	0.018%
81	12.108	3346	3349	3352	rBV2	330	259	0.05%	0.006%
82	12.195	3363	3376	3393	rVB	246233	395192	74.90%	8.978%
83	12.262	3393	3397	3402	rBV3	290	333	0.06%	0.008%
84	12.288	3402	3405	3410	rVB2	338	298	0.06%	0.007%
85	12.320	3410	3415	3417	rBV	326	339	0.06%	0.008%
86	12.777	3549	3557	3564	rBV3	982	1713	0.32%	0.039%
87	12.912	3596	3599	3602	rBV	424	354	0.07%	0.008%
88	12.983	3618	3621	3626	rVB	586	496	0.09%	0.011%
89	13.201	3685	3689	3694	rBV	366	420	0.08%	0.010%
90	13.770	3862	3866	3868	rBV2	473	397	0.08%	0.009%
91	14.356	4043	4048	4051	rBV2	352	391	0.07%	0.009%
92	14.577	4109	4117	4118	rBV3	1058	1268	0.24%	0.029%
93	14.635	4132	4135	4141	rVB	394	276	0.05%	0.006%
94	14.796	4182	4185	4187	rBV2	367	263	0.05%	0.006%
95	14.918	4220	4223	4229	rBV2	307	334	0.06%	0.008%
96	14.986	4242	4244	4250	rVB	452	337	0.06%	0.008%
97	15.420	4373	4379	4382	rBV2	581	743	0.14%	0.017%
98	15.497	4400	4403	4411	rVB2	487	600	0.11%	0.014%
99	15.536	4412	4415	4418	rBV	471	385	0.07%	0.009%
100	16.146	4602	4605	4612	rVB2	510	553	0.10%	0.013%




Sum of corrected areas: 4401716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046337.D
Acq On : 13 Dec 2021 23:27
Operator : SY/MD
Sample : M5062-03 20X
Misc : 6.77g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

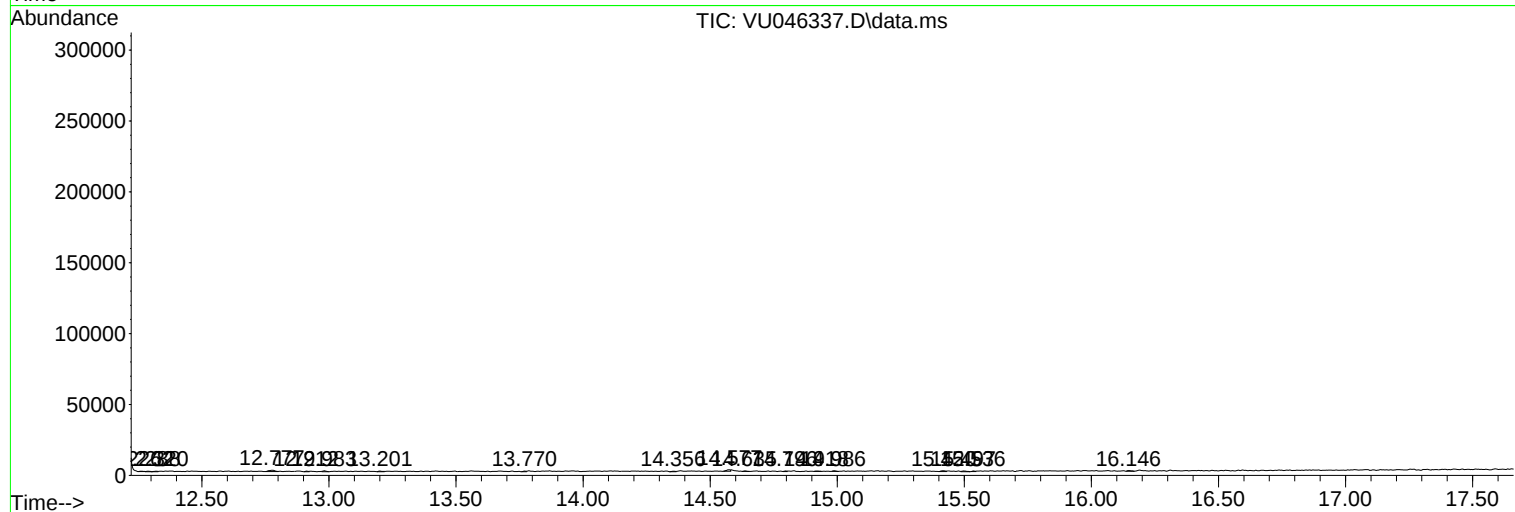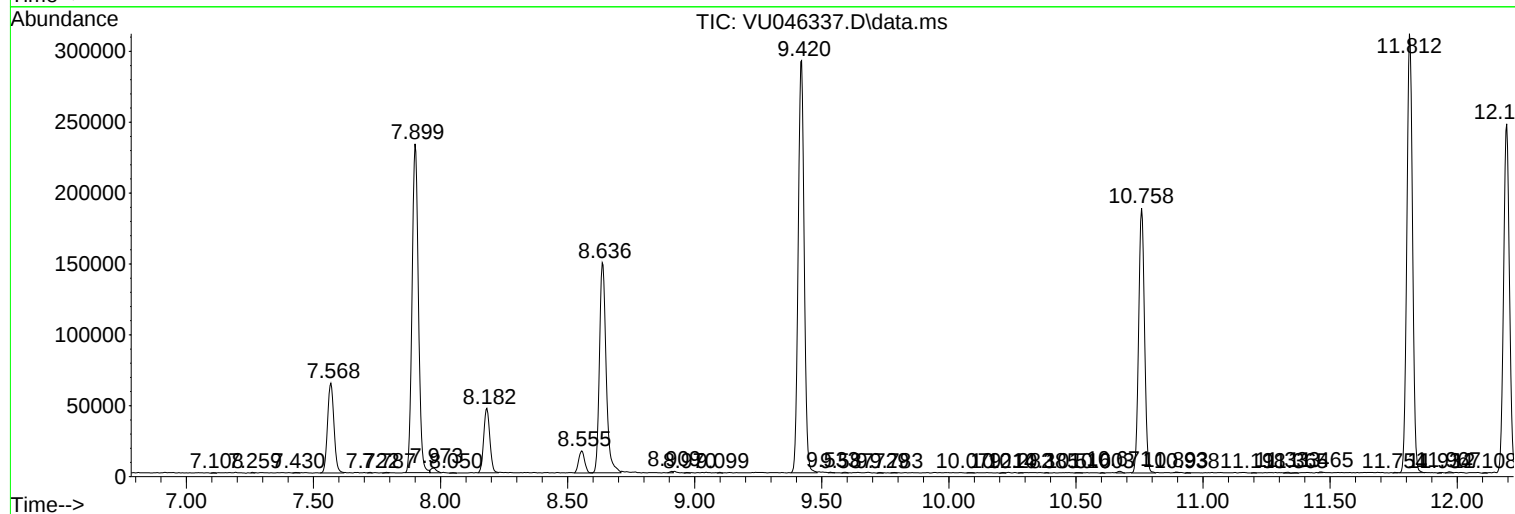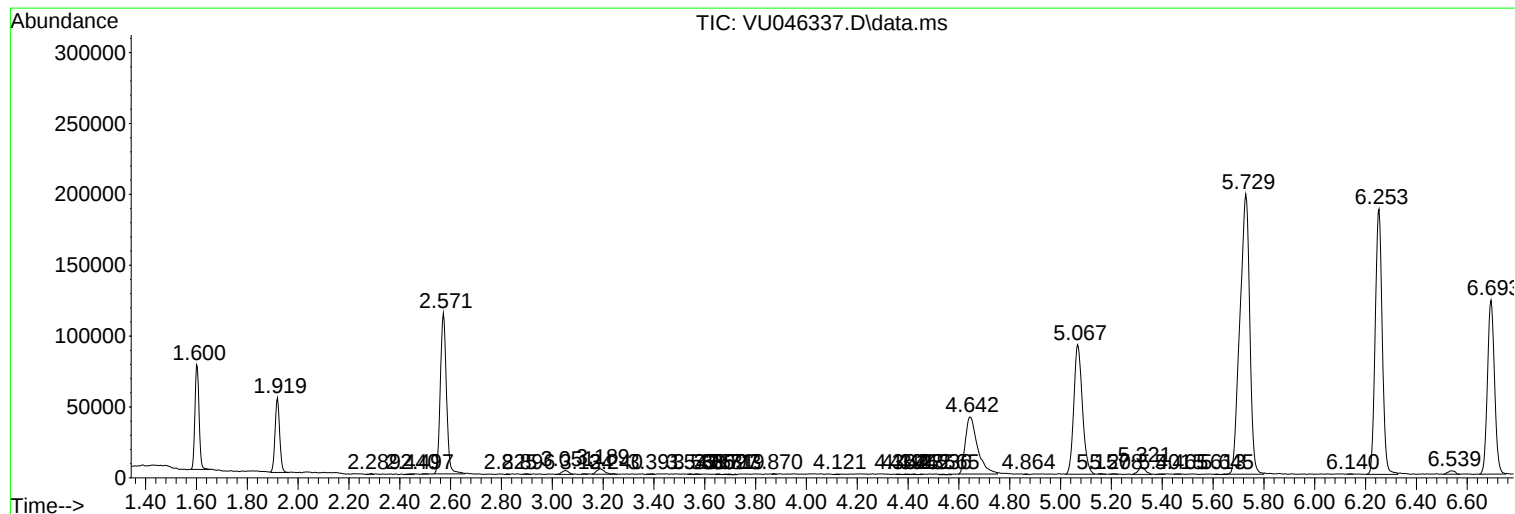

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046337.D
Acq On : 13 Dec 2021 23:27
Operator : SY/MD
Sample : M5062-03 20X
Misc : 6.77g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046337.D
Acq On : 13 Dec 2021 23:27
Operator : SY/MD
Sample : M5062-03 20X
Misc : 6.77g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------