

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046341.D
 Acq On : 14 Dec 2021 00:57
 Operator : SY/MD
 Sample : M5023-20ME 20X
 Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKZ8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	75	81	101	rVB	56469	81537	3.48%	1.181%
2	2.549	366	376	400	rBV3	103684	188579	8.06%	2.732%
3	2.816	455	459	464	rBV5	577	568	0.02%	0.008%
4	2.948	497	500	505	rBV3	512	558	0.02%	0.008%
5	3.041	519	529	531	rBV3	1317	1838	0.08%	0.027%
6	3.182	562	573	592	rVB2	11118	26447	1.13%	0.383%
7	3.407	640	643	645	rBV2	310	219	0.01%	0.003%
8	3.729	739	743	745	rBV2	282	258	0.01%	0.004%
9	3.800	763	765	767	rBV2	191	97	0.00%	0.001%
10	3.864	774	785	800	rVB2	17870	41750	1.78%	0.605%
11	3.989	820	824	827	rBV	281	226	0.01%	0.003%
12	4.009	827	830	832	rBV	264	148	0.01%	0.002%
13	4.070	846	849	851	rBV	221	125	0.01%	0.002%
14	4.134	866	869	876	rBV2	309	502	0.02%	0.007%
15	4.253	903	906	909	rVB	418	228	0.01%	0.003%
16	4.308	921	923	926	rBV	224	137	0.01%	0.002%
17	4.362	935	940	944	rBV	464	496	0.02%	0.007%
18	4.584	1005	1009	1011	rBV	291	183	0.01%	0.003%
19	4.665	1017	1034	1052	rBV	26758	100157	4.28%	1.451%
20	5.067	1144	1159	1191	rVB2	82160	221982	9.49%	3.216%
21	5.179	1191	1194	1198	rBV	352	265	0.01%	0.004%
22	5.205	1198	1202	1207	rBV2	268	300	0.01%	0.004%
23	5.304	1230	1233	1235	rBV2	164	86	0.00%	0.001%
24	5.443	1273	1276	1277	rBV	204	122	0.01%	0.002%
25	5.481	1285	1288	1291	rBV2	237	171	0.01%	0.002%
26	5.600	1322	1325	1329	rBV2	284	273	0.01%	0.004%
27	5.722	1343	1363	1384	rBV2	209394	539309	23.05%	7.813%
28	5.877	1405	1411	1413	rBV	467	431	0.02%	0.006%
29	5.935	1426	1429	1434	rBV	299	248	0.01%	0.004%
30	5.980	1434	1443	1447	rBV3	3552	5469	0.23%	0.079%
31	6.063	1467	1469	1473	rVB	368	250	0.01%	0.004%
32	6.250	1512	1527	1554	rBV	205293	425683	18.19%	6.167%
33	6.401	1572	1574	1577	rBV	288	216	0.01%	0.003%
34	6.439	1582	1586	1589	rBV2	280	246	0.01%	0.004%
35	6.542	1604	1618	1633	rBV	141396	275029	11.75%	3.984%
36	6.693	1651	1665	1691	rVB	113296	242561	10.37%	3.514%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046341.D
 Acq On : 14 Dec 2021 00:57
 Operator : SY/MD
 Sample : M5023-20ME 20X
 Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKZ8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.800	1696	1698	1702	rVV2	358	260	0.01%	0.004%
38	6.835	1706	1709	1712	rBV2	244	173	0.01%	0.003%
39	6.893	1724	1727	1728	rBV	302	178	0.01%	0.003%
40	6.957	1744	1747	1748	rBV2	170	102	0.00%	0.001%
41	7.012	1760	1764	1766	rBV	372	249	0.01%	0.004%
42	7.079	1782	1785	1787	rBV	228	150	0.01%	0.002%
43	7.121	1796	1798	1801	rBV	219	99	0.00%	0.001%
44	7.198	1820	1822	1825	rBV	384	210	0.01%	0.003%
45	7.224	1828	1830	1831	rBV	429	217	0.01%	0.003%
46	7.327	1859	1862	1865	rBV2	208	149	0.01%	0.002%
47	7.423	1888	1892	1896	rBV2	257	274	0.01%	0.004%
48	7.523	1920	1923	1925	rBV2	244	155	0.01%	0.002%
49	7.568	1925	1937	1965	rVV3	55636	118582	5.07%	1.718%
50	7.899	2027	2040	2058	rBV	219078	425533	18.18%	6.165%
51	8.185	2118	2129	2153	rBV2	30005	78277	3.35%	1.134%
52	8.417	2197	2201	2206	rBV2	441	470	0.02%	0.007%
53	8.555	2229	2244	2264	rBV	1331151	2340055	100.00%	33.901%
54	9.153	2427	2430	2434	rBV	354	282	0.01%	0.004%
55	9.359	2491	2494	2495	rBV	142	80	0.00%	0.001%
56	9.426	2500	2515	2535	rVV	238428	560697	23.96%	8.123%
57	9.552	2551	2554	2557	rBV	288	187	0.01%	0.003%
58	9.693	2595	2598	2599	rBV2	264	160	0.01%	0.002%
59	9.970	2680	2684	2687	rBV	202	190	0.01%	0.003%
60	10.224	2760	2763	2765	rBV	231	133	0.01%	0.002%
61	10.471	2837	2840	2842	rBV	264	207	0.01%	0.003%
62	10.510	2849	2852	2854	rBV	460	302	0.01%	0.004%
63	10.668	2896	2901	2902	rBV2	892	696	0.03%	0.010%
64	10.713	2911	2915	2919	rBV	447	383	0.02%	0.006%
65	10.774	2921	2934	2949	rVB	165688	283934	12.13%	4.113%
66	10.838	2949	2954	2957	rBV	565	453	0.02%	0.007%
67	11.063	3018	3024	3027	rBV2	407	447	0.02%	0.006%
68	11.118	3036	3041	3047	rVB4	1217	1216	0.05%	0.018%
69	11.282	3089	3092	3097	rBV2	438	433	0.02%	0.006%
70	11.333	3105	3108	3112	rBV	256	227	0.01%	0.003%
71	11.385	3118	3124	3126	rBV	272	327	0.01%	0.005%
72	11.822	3247	3260	3274	rBV	346437	544714	23.28%	7.892%
73	11.909	3285	3287	3294	rBV2	359	368	0.02%	0.005%
74	12.147	3358	3361	3362	rBV2	197	112	0.00%	0.002%
75	12.201	3365	3378	3397	rVB	238399	382131	16.33%	5.536%
76	12.278	3398	3402	3403	rBV	430	327	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046341.D
 Acq On : 14 Dec 2021 00:57
 Operator : SY/MD
 Sample : M5023-20ME 20X
 Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKZ8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	12.973	3616	3618	3619	rBV2	316	148	0.01%	0.002%
78	13.208	3686	3691	3692	rBV2	389	354	0.02%	0.005%
79	13.401	3749	3751	3753	rBV2	277	177	0.01%	0.003%
80	13.532	3789	3792	3794	rBV	361	277	0.01%	0.004%
81	13.684	3836	3839	3841	rBV	370	230	0.01%	0.003%
82	13.905	3906	3908	3911	rBV2	392	248	0.01%	0.004%
83	14.561	4109	4112	4113	rBV	694	405	0.02%	0.006%
84	15.577	4425	4428	4436	rBV2	499	855	0.04%	0.012%




Sum of corrected areas: 6902527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046341.D
Acq On : 14 Dec 2021 00:57
Operator : SY/MD
Sample : M5023-20ME 20X
Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKZ8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

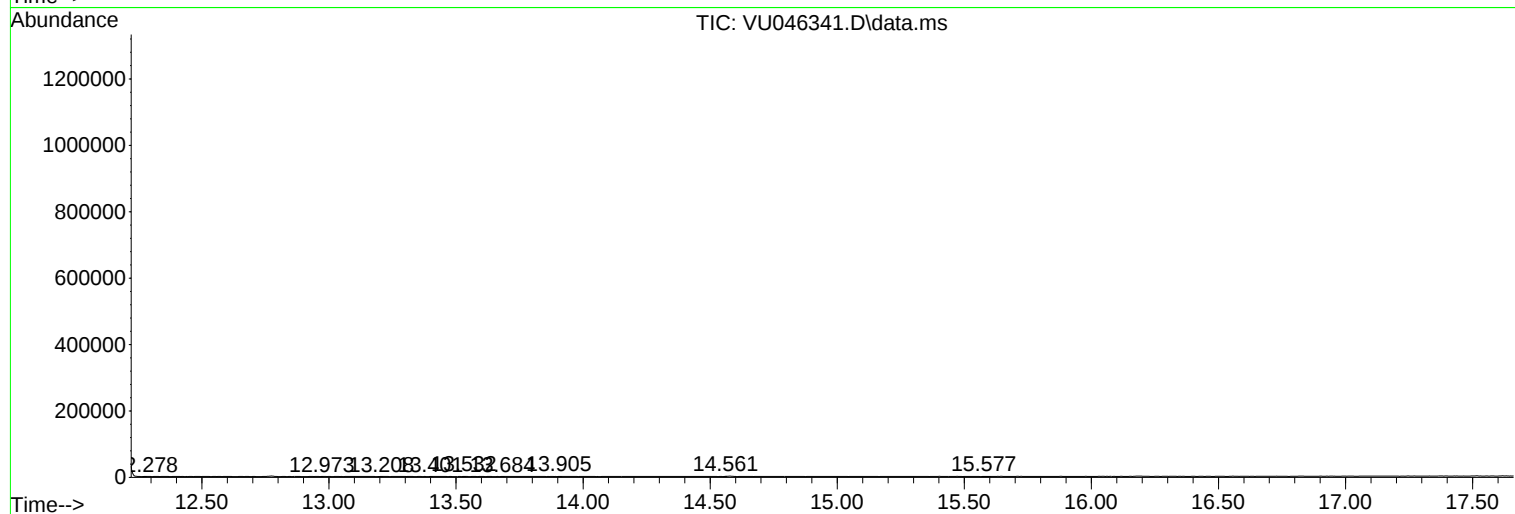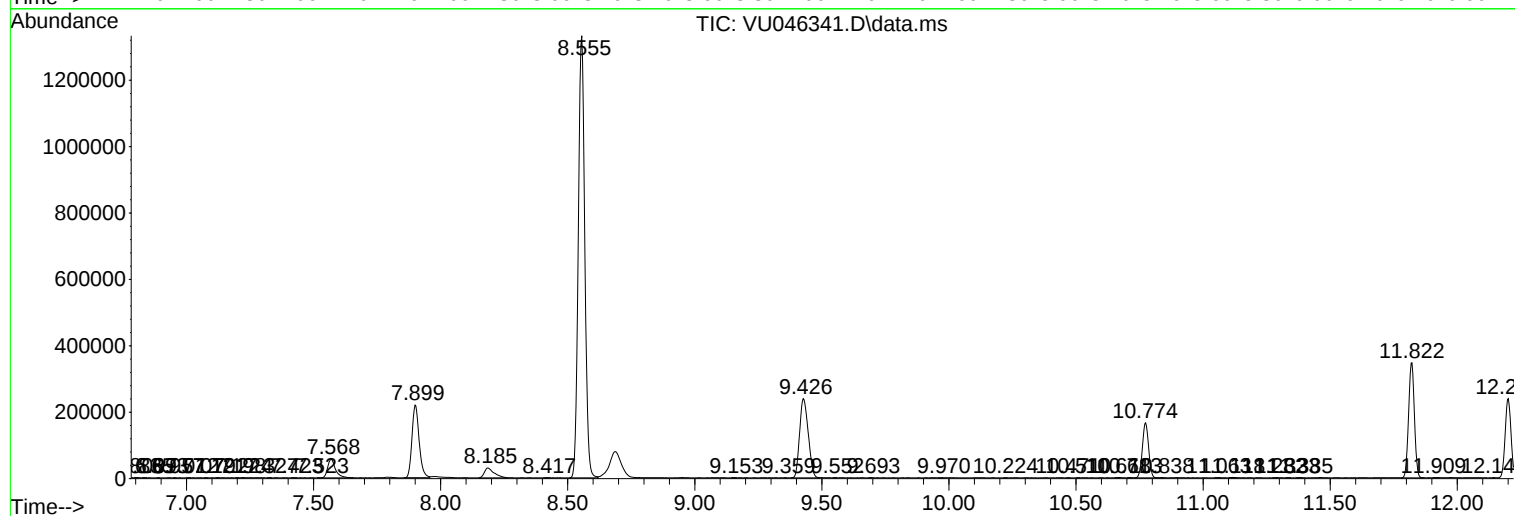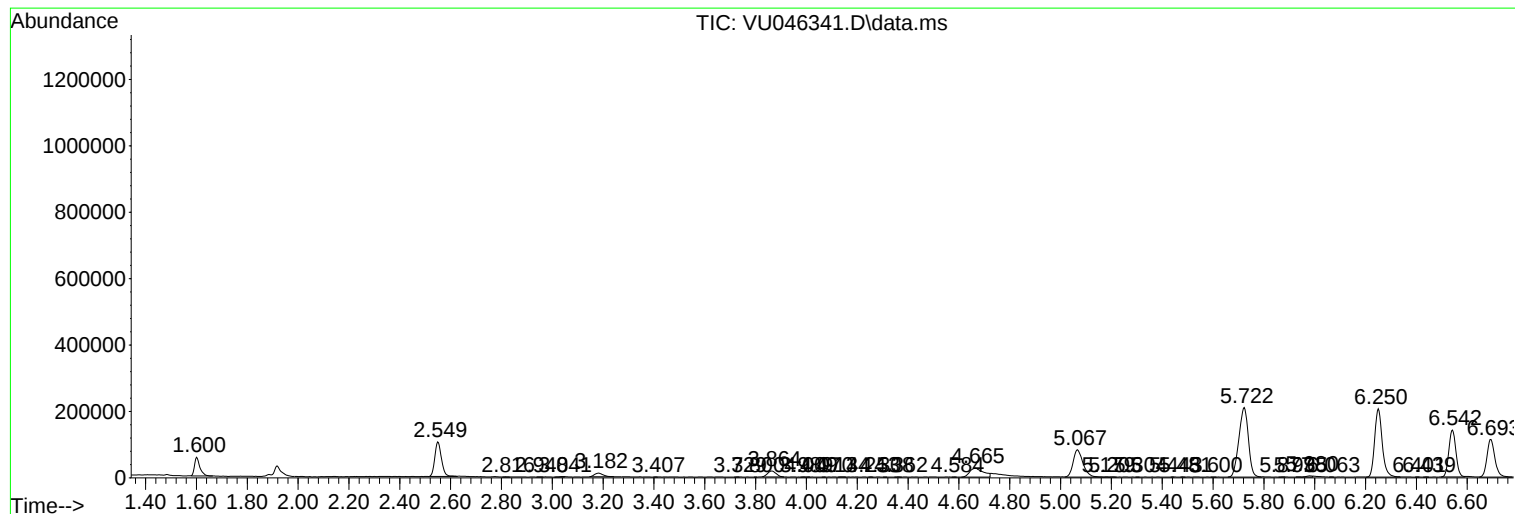

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046341.D
Acq On : 14 Dec 2021 00:57
Operator : SY/MD
Sample : M5023-20ME 20X
Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKZ8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046341.D
Acq On : 14 Dec 2021 00:57
Operator : SY/MD
Sample : M5023-20ME 20X
Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKZ8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc