

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046342.D
 Acq On : 14 Dec 2021 01:19
 Operator : SY/MD
 Sample : M4975-06DL 400X
 Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKT0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	95	rVB	81724	91383	0.75%	0.542%
2	1.919	173	180	192	rVB	58047	73417	0.60%	0.435%
3	2.240	277	280	283	rVB	421	282	0.00%	0.002%
4	2.263	283	287	288	rBV	318	217	0.00%	0.001%
5	2.404	328	331	335	rBV	461	279	0.00%	0.002%
6	2.572	371	383	405	rBV	123016	209761	1.73%	1.244%
7	3.057	526	534	539	rVB3	983	1546	0.01%	0.009%
8	3.108	543	550	552	rBV	351	416	0.00%	0.002%
9	3.125	552	555	558	rBV2	367	267	0.00%	0.002%
10	3.195	563	577	588	rBV2	3216	7124	0.06%	0.042%
11	3.565	688	692	695	rBV	340	296	0.00%	0.002%
12	3.645	713	717	722	rBV2	422	447	0.00%	0.003%
13	3.671	722	725	727	rVV	178	105	0.00%	0.001%
14	3.700	732	734	735	rVV	258	136	0.00%	0.001%
15	3.723	739	741	746	rVB2	367	225	0.00%	0.001%
16	3.755	746	751	753	rBV2	289	305	0.00%	0.002%
17	3.867	783	786	788	rBV	221	167	0.00%	0.001%
18	3.883	788	791	797	rVV2	302	321	0.00%	0.002%
19	4.018	830	833	834	rBV2	189	112	0.00%	0.001%
20	4.060	842	846	851	rBV2	396	443	0.00%	0.003%
21	4.112	859	862	863	rBV	169	112	0.00%	0.001%
22	4.125	864	866	871	rVV	390	297	0.00%	0.002%
23	4.160	874	877	881	rBV2	342	281	0.00%	0.002%
24	4.250	902	905	911	rBV	525	604	0.00%	0.004%
25	4.305	919	922	926	rBV	359	249	0.00%	0.001%
26	4.327	926	929	932	rBV	467	268	0.00%	0.002%
27	4.520	985	989	991	rBV	271	231	0.00%	0.001%
28	4.571	1001	1005	1008	rBV2	254	263	0.00%	0.002%
29	4.642	1012	1027	1065	rVV	45507	146156	1.20%	0.867%
30	4.999	1134	1138	1139	rBV	195	141	0.00%	0.001%
31	5.067	1143	1159	1186	rVV	100629	229272	1.89%	1.360%
32	5.321	1220	1238	1258	rBV2	136703	305448	2.52%	1.811%
33	5.462	1280	1282	1288	rBV2	231	252	0.00%	0.001%
34	5.549	1307	1309	1311	rBV	237	148	0.00%	0.001%
35	5.594	1320	1323	1329	rBV2	435	586	0.00%	0.003%
36	5.729	1344	1365	1383	rBV2	207026	562378	4.63%	3.335%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046342.D
 Acq On : 14 Dec 2021 01:19
 Operator : SY/MD
 Sample : M4975-06DL 400X
 Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKT0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	5.957	1429	1436	1438	rBV	387	344	0.00%	0.002%
38	6.031	1456	1459	1462	rBV	338	250	0.00%	0.001%
39	6.176	1501	1504	1505	rBV	208	119	0.00%	0.001%
40	6.253	1515	1528	1559	rVB	179264	341188	2.81%	2.023%
41	6.546	1606	1619	1638	rVB	64768	120442	0.99%	0.714%
42	6.645	1648	1650	1651	rBV	236	110	0.00%	0.001%
43	6.694	1651	1665	1692	rVB	129867	251811	2.07%	1.493%
44	6.835	1705	1709	1710	rBV	203	151	0.00%	0.001%
45	6.903	1726	1730	1733	rBV	333	297	0.00%	0.002%
46	6.954	1743	1746	1749	rVB2	251	139	0.00%	0.001%
47	6.973	1749	1752	1755	rVB	275	169	0.00%	0.001%
48	7.009	1760	1763	1765	rBV	228	137	0.00%	0.001%
49	7.050	1773	1776	1780	rBV	442	279	0.00%	0.002%
50	7.150	1801	1807	1810	rBV2	334	416	0.00%	0.002%
51	7.169	1810	1813	1814	rBV	257	165	0.00%	0.001%
52	7.256	1837	1840	1842	rBV	349	242	0.00%	0.001%
53	7.333	1861	1864	1867	rBV2	352	274	0.00%	0.002%
54	7.411	1885	1888	1891	rVB	256	150	0.00%	0.001%
55	7.430	1891	1894	1896	rBV	310	224	0.00%	0.001%
56	7.568	1923	1937	1951	rBV	68298	119108	0.98%	0.706%
57	7.700	1974	1978	1981	rBV2	336	298	0.00%	0.002%
58	7.777	1999	2002	2004	rBV2	191	118	0.00%	0.001%
59	7.793	2004	2007	2011	rVV	260	187	0.00%	0.001%
60	7.899	2024	2040	2055	rBV	252285	435496	3.59%	2.583%
61	8.182	2117	2128	2142	rBV	48201	79669	0.66%	0.472%
62	8.279	2155	2158	2161	rBV	389	286	0.00%	0.002%
63	8.475	2217	2219	2223	rBV	251	177	0.00%	0.001%
64	8.558	2228	2245	2260	rBV	7207792	12141871	100.00%	72.009%
65	8.854	2334	2337	2344	rBV2	306	422	0.00%	0.003%
66	8.912	2350	2355	2363	rBV2	1391	1784	0.01%	0.011%
67	8.992	2376	2380	2382	rBV2	413	285	0.00%	0.002%
68	9.057	2396	2400	2402	rBV	317	243	0.00%	0.001%
69	9.192	2439	2442	2444	rBV	219	162	0.00%	0.001%
70	9.417	2500	2512	2533	rBV	284824	471013	3.88%	2.793%
71	9.568	2552	2559	2569	rVB2	1438	2401	0.02%	0.014%
72	9.613	2569	2573	2577	rBV	322	291	0.00%	0.002%
73	9.693	2588	2598	2610	rVB	14214	22335	0.18%	0.132%
74	9.812	2630	2635	2641	rBV2	411	627	0.01%	0.004%
75	9.854	2645	2648	2653	rVB2	443	464	0.00%	0.003%
76	9.886	2653	2658	2663	rBV2	504	562	0.00%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046342.D
 Acq On : 14 Dec 2021 01:19
 Operator : SY/MD
 Sample : M4975-06DL 400X
 Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKT0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	9.912	2663	2666	2668	rBV	284	187	0.00%	0.001%
78	9.970	2682	2684	2687	rVB2	224	108	0.00%	0.001%
79	10.102	2717	2725	2735	rBV3	3182	4717	0.04%	0.028%
80	10.208	2754	2758	2763	rBV	573	452	0.00%	0.003%
81	10.237	2763	2767	2771	rVV	359	282	0.00%	0.002%
82	10.282	2779	2781	2783	rBV2	258	146	0.00%	0.001%
83	10.298	2783	2786	2787	rBV	352	226	0.00%	0.001%
84	10.565	2866	2869	2875	rBV2	276	295	0.00%	0.002%
85	10.661	2895	2899	2900	rBV	409	278	0.00%	0.002%
86	10.758	2917	2929	2946	rVB	197218	312109	2.57%	1.851%
87	10.822	2946	2949	2952	rBV	227	177	0.00%	0.001%
88	11.150	3048	3051	3058	rBV2	269	267	0.00%	0.002%
89	11.327	3104	3106	3109	rBV	232	150	0.00%	0.001%
90	11.626	3196	3199	3201	rBV2	355	238	0.00%	0.001%
91	11.690	3216	3219	3221	rBV2	296	194	0.00%	0.001%
92	11.812	3245	3257	3275	rBV	302628	481163	3.96%	2.854%
93	12.131	3354	3356	3360	rBV2	398	249	0.00%	0.001%
94	12.195	3364	3376	3391	rVV	268355	428908	3.53%	2.544%
95	12.420	3443	3446	3451	rBV2	382	338	0.00%	0.002%
96	12.767	3548	3554	3556	rBV2	896	935	0.01%	0.006%
97	13.140	3668	3670	3675	rBV2	268	236	0.00%	0.001%
98	13.645	3820	3827	3829	rBV	476	517	0.00%	0.003%
99	13.696	3840	3843	3847	rBV	503	424	0.00%	0.003%
100	13.748	3856	3859	3867	rBV	382	477	0.00%	0.003%




Sum of corrected areas: 16861714

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046342.D
Acq On : 14 Dec 2021 01:19
Operator : SY/MD
Sample : M4975-06DL 400X
Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

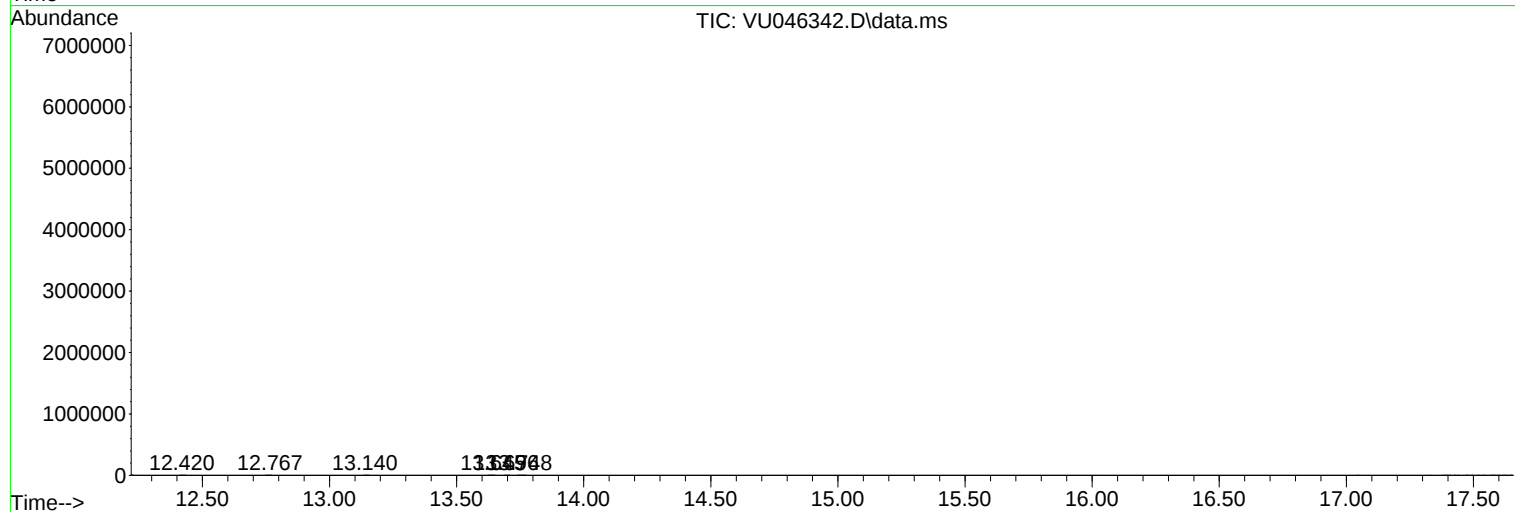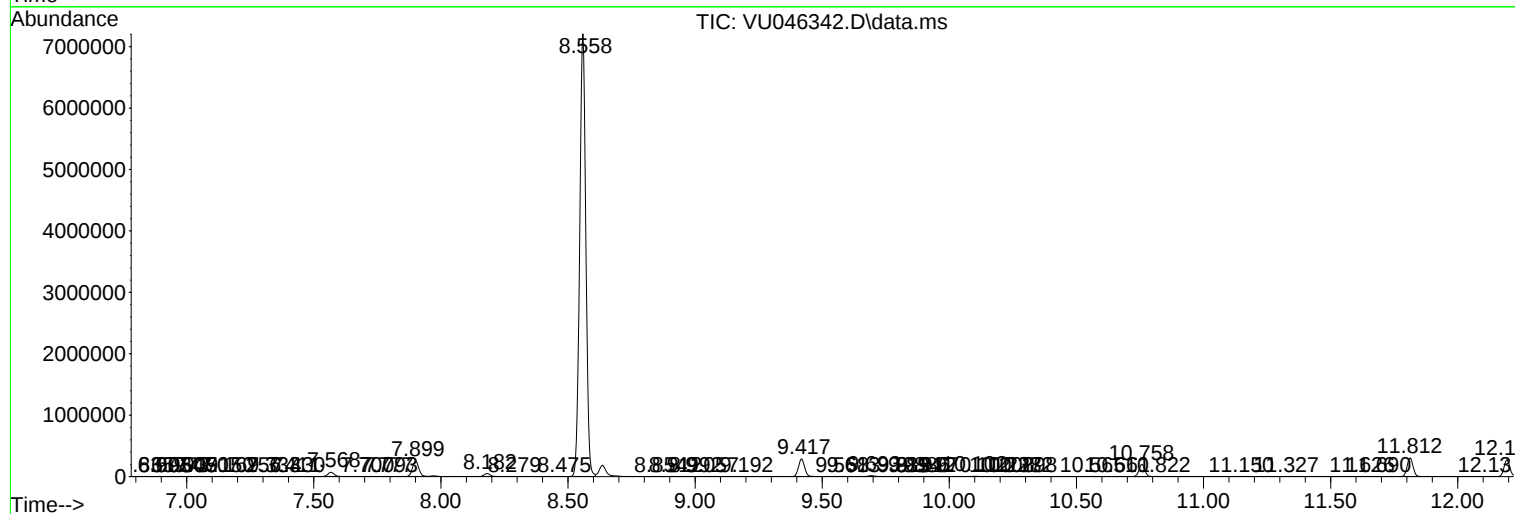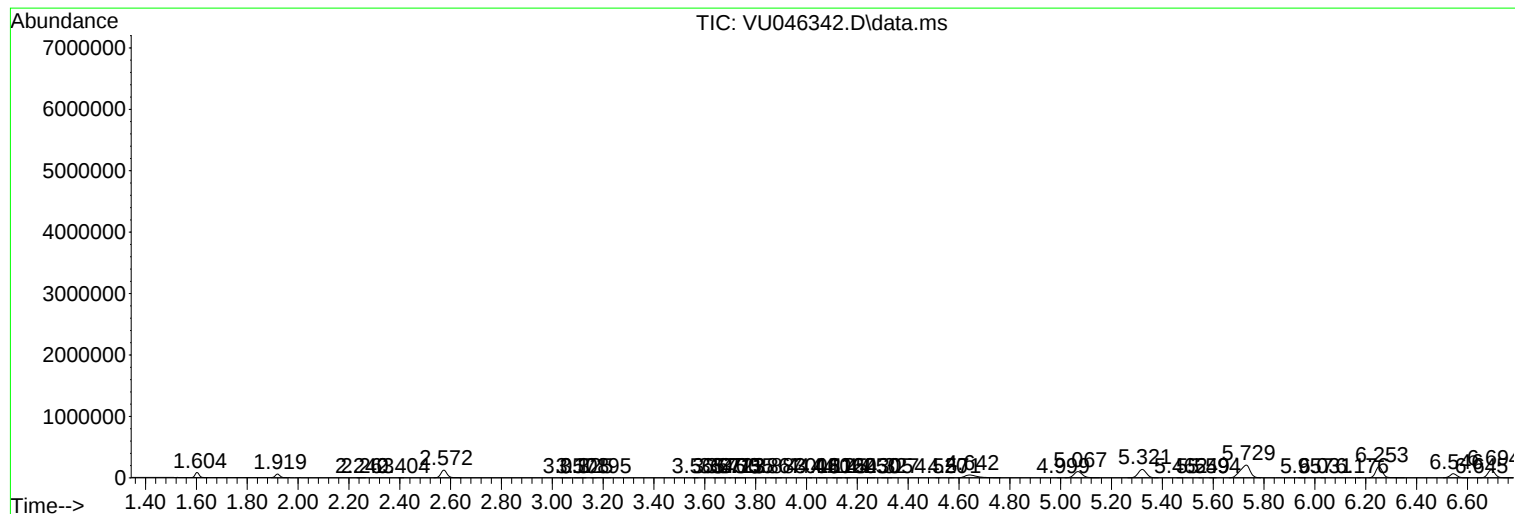

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046342.D
Acq On : 14 Dec 2021 01:19
Operator : SY/MD
Sample : M4975-06DL 400X
Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046342.D
Acq On : 14 Dec 2021 01:19
Operator : SY/MD
Sample : M4975-06DL 400X
Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc