

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046343.D
 Acq On : 14 Dec 2021 01:42
 Operator : SY/MD
 Sample : VIBLK010
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	98	rVB	72815	79535	15.14%	1.841%
2	1.919	172	180	192	rVB	56224	70325	13.38%	1.628%
3	2.221	269	274	276	rBV	483	406	0.08%	0.009%
4	2.321	301	305	308	rVB3	342	300	0.06%	0.007%
5	2.501	353	361	364	rBV2	327	527	0.10%	0.012%
6	2.575	372	384	416	rBV	110728	186021	35.40%	4.305%
7	2.777	443	447	450	rBV2	255	264	0.05%	0.006%
8	2.848	466	469	476	rVB2	331	308	0.06%	0.007%
9	2.960	501	504	510	rVB2	334	268	0.05%	0.006%
10	3.057	523	534	544	rVB2	4722	8606	1.64%	0.199%
11	3.131	549	557	561	rBV2	354	559	0.11%	0.013%
12	3.189	564	575	589	rVV3	2271	4707	0.90%	0.109%
13	3.259	594	597	602	rVV2	263	281	0.05%	0.007%
14	3.340	616	622	623	rBV	490	428	0.08%	0.010%
15	3.417	640	646	651	rBV2	458	581	0.11%	0.013%
16	3.465	657	661	664	rVV2	430	402	0.08%	0.009%
17	3.787	758	761	767	rVV2	431	522	0.10%	0.012%
18	3.960	808	815	818	rBV	433	521	0.10%	0.012%
19	4.108	856	861	863	rBV	293	266	0.05%	0.006%
20	4.121	863	865	870	rVB	397	301	0.06%	0.007%
21	4.337	926	932	935	rBV2	282	312	0.06%	0.007%
22	4.642	1013	1027	1058	rBV2	42080	138727	26.40%	3.211%
23	5.070	1144	1160	1183	rVV	92663	216738	41.25%	5.016%
24	5.214	1201	1205	1208	rBV2	350	278	0.05%	0.006%
25	5.411	1262	1266	1268	rBV2	321	281	0.05%	0.007%
26	5.729	1344	1365	1387	rBV2	192330	525423	100.00%	12.161%
27	5.925	1419	1426	1427	rBV	308	334	0.06%	0.008%
28	6.012	1447	1453	1456	rBV2	373	418	0.08%	0.010%
29	6.153	1493	1497	1501	rVB2	322	276	0.05%	0.006%
30	6.182	1501	1506	1509	rBV	359	293	0.06%	0.007%
31	6.253	1514	1528	1544	rBV	174437	330344	62.87%	7.646%
32	6.427	1578	1582	1587	rBV2	243	279	0.05%	0.006%
33	6.533	1608	1615	1625	rVB6	2102	3406	0.65%	0.079%
34	6.619	1639	1642	1644	rBV	387	321	0.06%	0.007%
35	6.693	1652	1665	1691	rVB	119836	233468	44.43%	5.403%
36	7.018	1763	1766	1769	rBV2	359	274	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046343.D
 Acq On : 14 Dec 2021 01:42
 Operator : SY/MD
 Sample : VIBLK010
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.173	1809	1814	1818	rVV	317	409	0.08%	0.009%
38	7.195	1818	1821	1825	rVB2	468	336	0.06%	0.008%
39	7.230	1828	1832	1835	rBV2	314	263	0.05%	0.006%
40	7.372	1871	1876	1878	rBV	380	321	0.06%	0.007%
41	7.484	1907	1911	1916	rVV	395	383	0.07%	0.009%
42	7.517	1916	1921	1925	rVB2	499	561	0.11%	0.013%
43	7.568	1925	1937	1957	rBV2	63745	110317	21.00%	2.553%
44	7.664	1962	1967	1971	rBV	373	310	0.06%	0.007%
45	7.697	1971	1977	1979	rBV2	286	311	0.06%	0.007%
46	7.799	2006	2009	2014	rBV	219	262	0.05%	0.006%
47	7.828	2015	2018	2023	rVB	422	318	0.06%	0.007%
48	7.899	2027	2040	2056	rBV	228000	396919	75.54%	9.186%
49	8.082	2092	2097	2100	rBV	249	270	0.05%	0.006%
50	8.182	2117	2128	2142	rBV	44907	73806	14.05%	1.708%
51	8.295	2158	2163	2166	rBV2	503	407	0.08%	0.009%
52	8.320	2168	2171	2180	rVV2	290	403	0.08%	0.009%
53	8.388	2189	2192	2198	rBV2	351	369	0.07%	0.009%
54	8.430	2198	2205	2211	rVV	521	606	0.12%	0.014%
55	8.462	2211	2215	2220	rBV	441	384	0.07%	0.009%
56	8.555	2234	2244	2257	rVB	17071	28338	5.39%	0.656%
57	8.635	2257	2269	2292	rBV	153771	274547	52.25%	6.354%
58	8.912	2350	2355	2362	rVB3	753	993	0.19%	0.023%
59	8.944	2362	2365	2373	rBV	260	319	0.06%	0.007%
60	9.047	2394	2397	2403	rVB	375	289	0.06%	0.007%
61	9.420	2497	2513	2543	rBV	271776	456231	86.83%	10.559%
62	9.889	2657	2659	2664	rVB	384	312	0.06%	0.007%
63	10.568	2865	2870	2874	rBV2	284	261	0.05%	0.006%
64	10.632	2883	2890	2894	rBV	406	465	0.09%	0.011%
65	10.674	2900	2903	2908	rVB3	769	527	0.10%	0.012%
66	10.758	2917	2929	2946	rVB	185388	297784	56.68%	6.892%
67	10.841	2949	2955	2958	rBV2	298	312	0.06%	0.007%
68	10.880	2964	2967	2969	rBV	489	362	0.07%	0.008%
69	11.127	3040	3044	3048	rVV	443	357	0.07%	0.008%
70	11.150	3048	3051	3056	rVB	460	341	0.06%	0.008%
71	11.455	3142	3146	3151	rBV3	384	418	0.08%	0.010%
72	11.812	3245	3257	3273	rVV	296086	455308	86.66%	10.538%
73	11.918	3283	3290	3293	rBV	501	666	0.13%	0.015%
74	12.195	3363	3376	3392	rVV	246802	396552	75.47%	9.178%
75	12.256	3393	3395	3401	rVB	386	289	0.06%	0.007%
76	12.568	3489	3492	3496	rVV	394	262	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
 Data File : VU046343.D
 Acq On : 14 Dec 2021 01:42
 Operator : SY/MD
 Sample : VIBLK010
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.597	3498	3501	3505	rVB	412	284	0.05%	0.007%
78	12.764	3550	3553	3563	rVB3	998	1508	0.29%	0.035%
79	12.854	3575	3581	3583	rBV2	422	393	0.07%	0.009%
80	13.031	3633	3636	3639	rBV	374	277	0.05%	0.006%
81	13.555	3796	3799	3804	rBV2	317	283	0.05%	0.007%
82	13.767	3862	3865	3870	rBV2	364	334	0.06%	0.008%
83	13.809	3874	3878	3883	rBV	432	369	0.07%	0.009%
84	13.960	3919	3925	3930	rBV	350	445	0.08%	0.010%
85	14.011	3937	3941	3945	rVV	361	354	0.07%	0.008%
86	14.105	3966	3970	3972	rBV	336	282	0.05%	0.007%
87	14.153	3981	3985	3988	rBV	454	372	0.07%	0.009%
88	14.240	4010	4012	4016	rVB	503	314	0.06%	0.007%
89	14.404	4060	4063	4065	rBV2	428	286	0.05%	0.007%
90	14.577	4108	4117	4127	rVB2	1506	2433	0.46%	0.056%
91	14.770	4172	4177	4178	rBV	559	511	0.10%	0.012%
92	15.204	4310	4312	4318	rVB	493	377	0.07%	0.009%
93	15.362	4358	4361	4367	rBV2	535	520	0.10%	0.012%
94	15.391	4368	4370	4375	rBV	296	271	0.05%	0.006%
95	15.497	4400	4403	4406	rBV	411	320	0.06%	0.007%
96	15.818	4499	4503	4508	rBV2	485	513	0.10%	0.012%
97	15.889	4518	4525	4533	rBV3	495	1126	0.21%	0.026%
98	15.925	4533	4536	4539	rBV	326	263	0.05%	0.006%
99	16.175	4611	4614	4616	rBV2	538	412	0.08%	0.010%
100	17.159	4917	4920	4922	rBV3	494	294	0.06%	0.007%




Sum of corrected areas: 4320729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046343.D
Acq On : 14 Dec 2021 01:42
Operator : SY/MD
Sample : VIBLK010
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK010

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

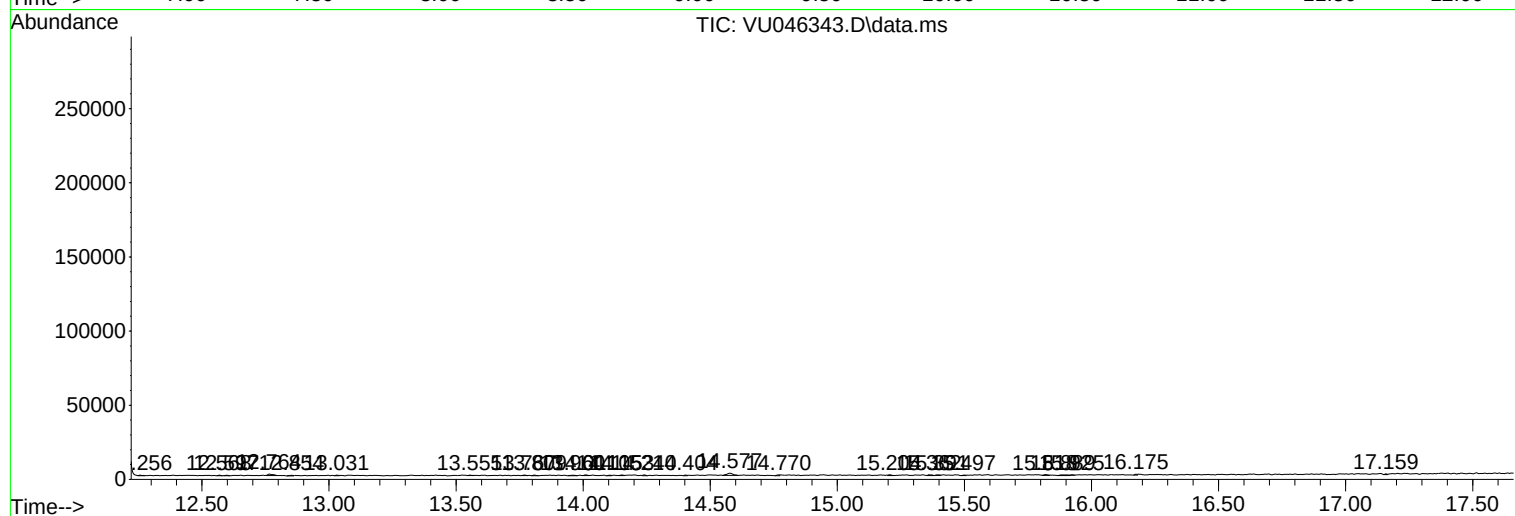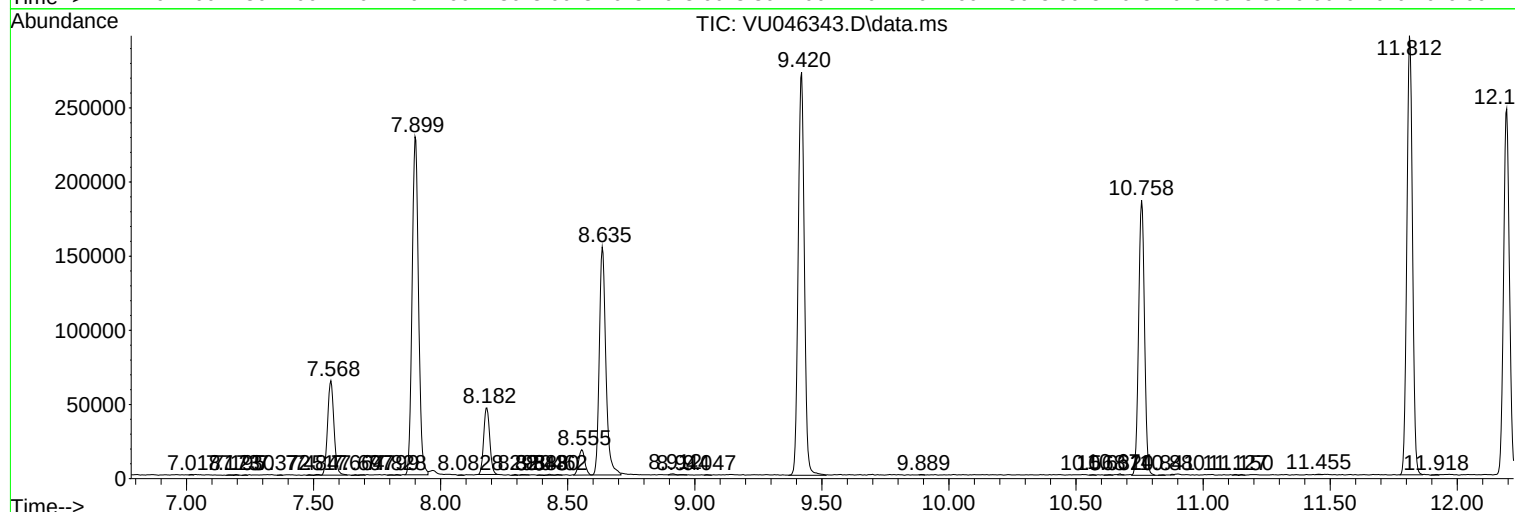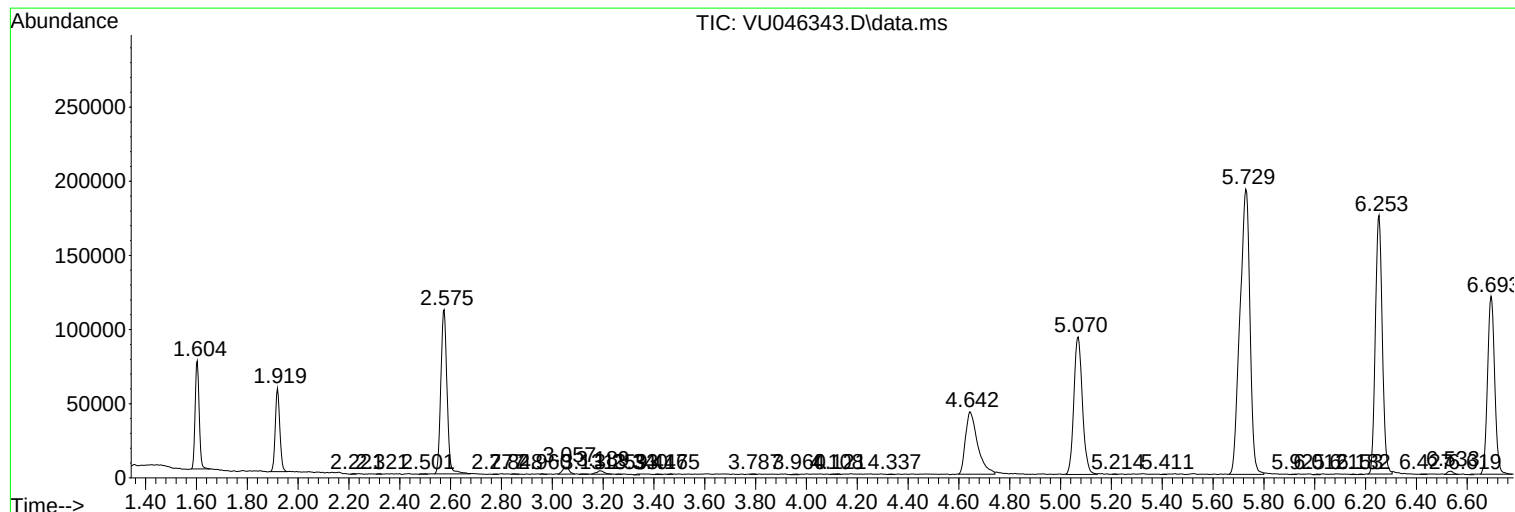

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046343.D
Acq On : 14 Dec 2021 01:42
Operator : SY/MD
Sample : VIBLK010
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK010

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046343.D
Acq On : 14 Dec 2021 01:42
Operator : SY/MD
Sample : VIBLK010
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK010

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------