
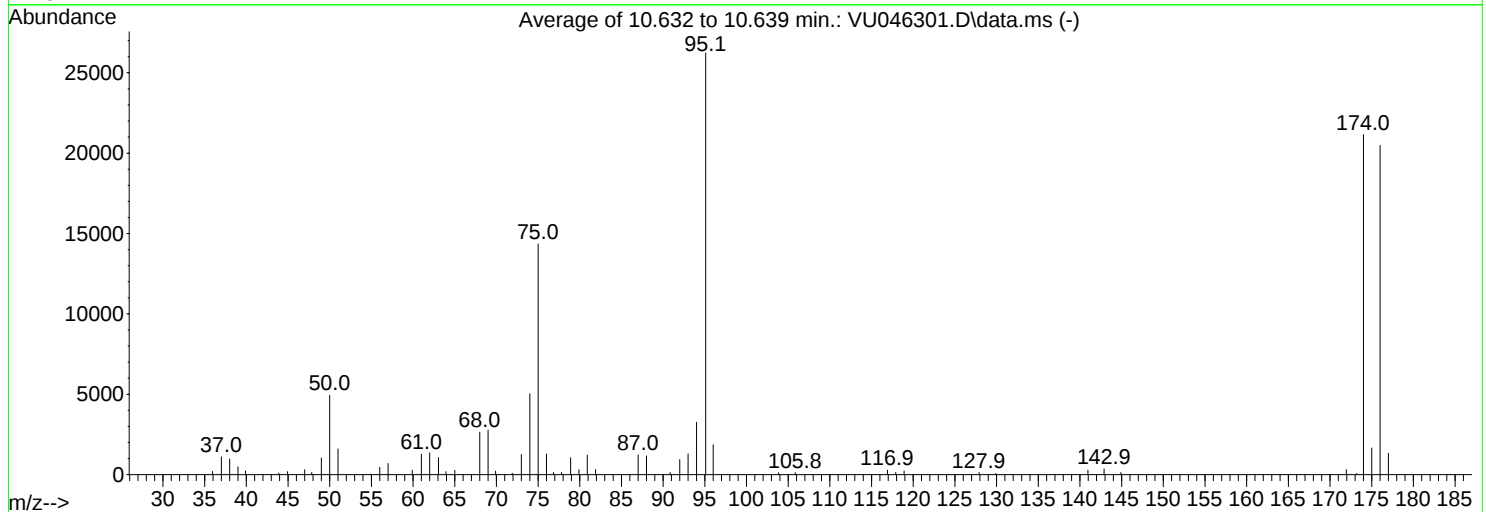


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121321\
Data File : VU046301.D
Acq On : 13 Dec 2021 09:20
Operator : SY/MD
Sample : BFB030
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB030

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis
Last Update : Fri Dec 17 03:50:47 2021

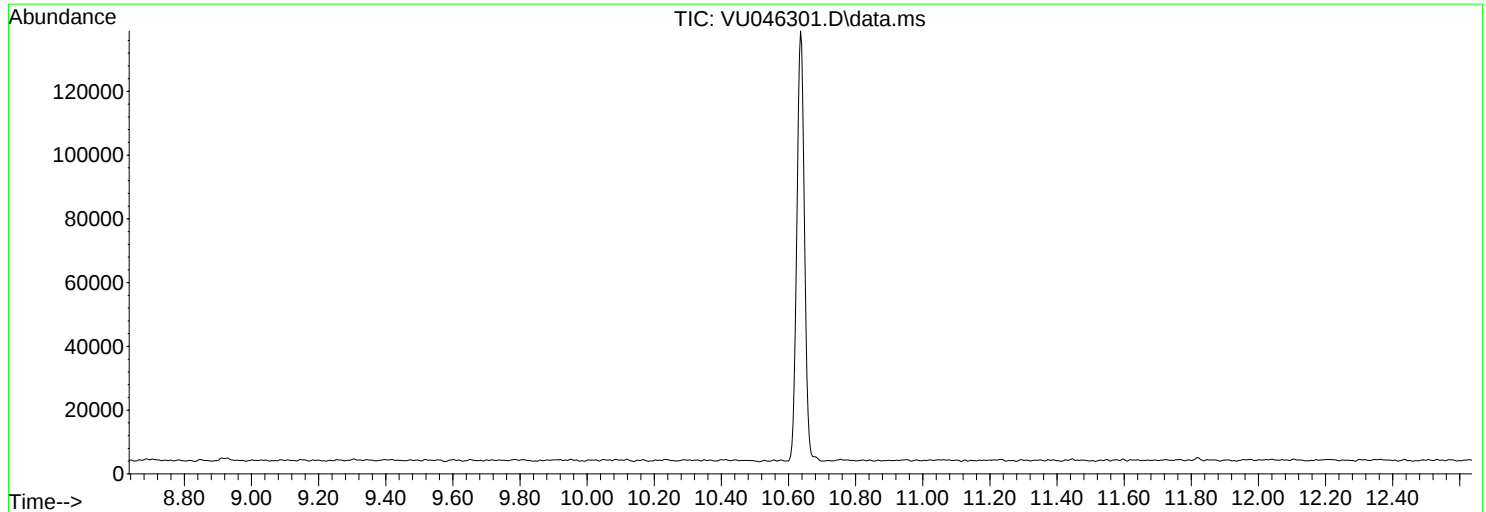

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	4941	PASS
75	95	30	80	54.7	14356	PASS
95	95	100	100	100.0	26240	PASS
96	95	5	9	7.1	1866	PASS
173	174	0.00	2	0.3	71	PASS
174	95	50	120	80.6	21155	PASS
175	174	5	9	7.9	1667	PASS
176	174	95	101	96.8	20485	PASS
177	176	5	9	6.5	1327	PASS

m/z	Abundance
39.90	3853.0
44.00	224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	215.0
37.00	1088.0
38.00	982.0
39.00	483.0
39.90	3937.0
43.90	338.0
44.90	191.0
47.00	298.0
47.90	128.0
49.00	1035.0
50.00	4870.0
51.00	1512.0
54.90	102.0
56.00	427.0
57.00	692.0
59.90	267.0
61.00	1258.0
62.00	1367.0
63.00	1071.0
63.90	191.0
65.00	246.0
68.00	2521.0
69.00	2730.0
69.90	214.0
73.00	1176.0
74.00	4810.0
75.00	14157.0
76.00	1271.0
76.90	140.0
77.80	120.0
78.90	1040.0
79.90	320.0
80.90	1170.0
81.90	308.0
87.00	1160.0
88.00	1193.0
90.90	122.0
92.00	965.0
93.00	1255.0
94.00	3266.0
95.10	25656.0
96.00	1825.0
103.90	116.0
105.80	132.0
116.90	301.0
117.90	105.0
118.90	218.0
127.90	126.0
141.00	277.0
142.90	336.0
144.90	134.0
171.90	286.0
173.20	212.0
174.00	20168.0
175.00	1590.0
176.00	19416.0
177.00	1352.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	192.0
37.00	1128.0
38.00	1020.0
39.00	495.0
39.90	4078.0
43.90	324.0
45.00	181.0
47.00	311.0
47.80	146.0
49.00	1083.0
50.00	5148.0
51.00	1667.0
56.00	477.0
57.00	711.0
59.90	286.0
61.00	1294.0
62.00	1383.0
63.10	1082.0
64.00	202.0
65.00	280.0
68.00	2697.0
69.00	2869.0
69.90	230.0
71.90	123.0
73.00	1321.0
74.00	5213.0
75.00	14737.0
76.00	1345.0
76.80	131.0
77.80	146.0
78.90	1099.0
79.90	317.0
80.90	1266.0
81.90	332.0
87.00	1259.0
88.00	1210.0
90.80	137.0
92.00	968.0
93.00	1325.0
94.00	3364.0
95.10	27024.0
96.00	1954.0
103.80	121.0
105.90	121.0
116.90	291.0
117.90	145.0
118.90	246.0
127.90	144.0
129.90	102.0
140.90	285.0
142.90	373.0
144.90	131.0
172.00	315.0
174.00	21800.0
175.00	1772.0
176.00	21136.0
177.00	1363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
36.00	183.0
37.00	1094.0
38.00	919.0
39.00	479.0
39.90	4219.0
43.90	305.0
45.00	197.0
47.00	311.0
47.90	155.0
49.00	976.0
50.00	4804.0
51.00	1622.0
56.00	460.0
57.00	701.0
59.90	251.0
61.00	1262.0
62.00	1304.0
63.10	1038.0
64.00	188.0
65.00	276.0
68.00	2684.0
69.00	2735.0
69.90	227.0
71.90	149.0
73.00	1275.0
74.00	5092.0
75.00	14173.0
76.00	1242.0
76.80	109.0
77.80	121.0
78.90	1022.0
79.90	296.0
80.90	1217.0
81.90	329.0
87.00	1298.0
88.00	1098.0
90.80	116.0
92.00	861.0
93.00	1296.0
94.00	3148.0
95.10	26040.0
96.00	1819.0
103.80	124.0
105.90	127.0
116.90	240.0
117.90	158.0
118.90	221.0
127.90	121.0
129.90	104.0
140.90	271.0
142.90	352.0
144.90	112.0
172.00	314.0
174.00	21496.0
175.00	1640.0
176.00	20904.0
177.00	1266.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030