

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
 Data File : VU052372.D
 Acq On : 13 Dec 2022 13:15
 Operator : JC/MD
 Sample : N6030-03 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL32DL

Quant Time: Dec 14 03:19:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 14 03:17:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.246	114	245531	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	247599	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	108672	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	86805	3.635	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.915	69	78889	4.253	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.000%
11) 1,1-Dichloroethene-d2	2.568	65	36300	4.240	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.800%
20) 2-Butanone-d5	4.639	46	271605	62.740	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.480%
24) Chloroform-d	5.060	84	172641	4.920	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	5.700	65	92788	5.235	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.600%
32) Benzene-d6	5.726	84	358247	4.874	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	6.687	67	118728	5.219	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.400%
41) Toluene-d8	7.896	98	288297	4.335	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	8.179	79	37420	4.514	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.200%
46) 2-Hexanone-d5	8.632	63	196424	55.911	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.820%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	103871	5.266	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	12.188	152	110411	5.307	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.200%
Target Compounds						
					Qvalue	
16) Methylene chloride	3.044	84	11032	0.458	ug/L	99
22) cis-1,2-Dichloroethene	4.661	96	5235	0.261	ug/L	93
34) Trichloroethene	6.539	95	52328	2.604	ug/L	98
35) Methylcyclohexane	6.687	83	26423	0.914	ug/L #	20
37) 1,2-Dichloropropane	6.687	63	11284	0.541	ug/L #	88
48) 2-Hexanone	8.632	43	24926	3.120	ug/L #	74
61) 1,2,3-Trichloropropane	11.809	75	12965	1.042	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052372.D
Acq On : 13 Dec 2022 13:15
Operator : JC/MD
Sample : N6030-03 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL32DL

Quant Time: Dec 14 03:19:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 14 03:17:56 2022
Response via : Initial Calibration




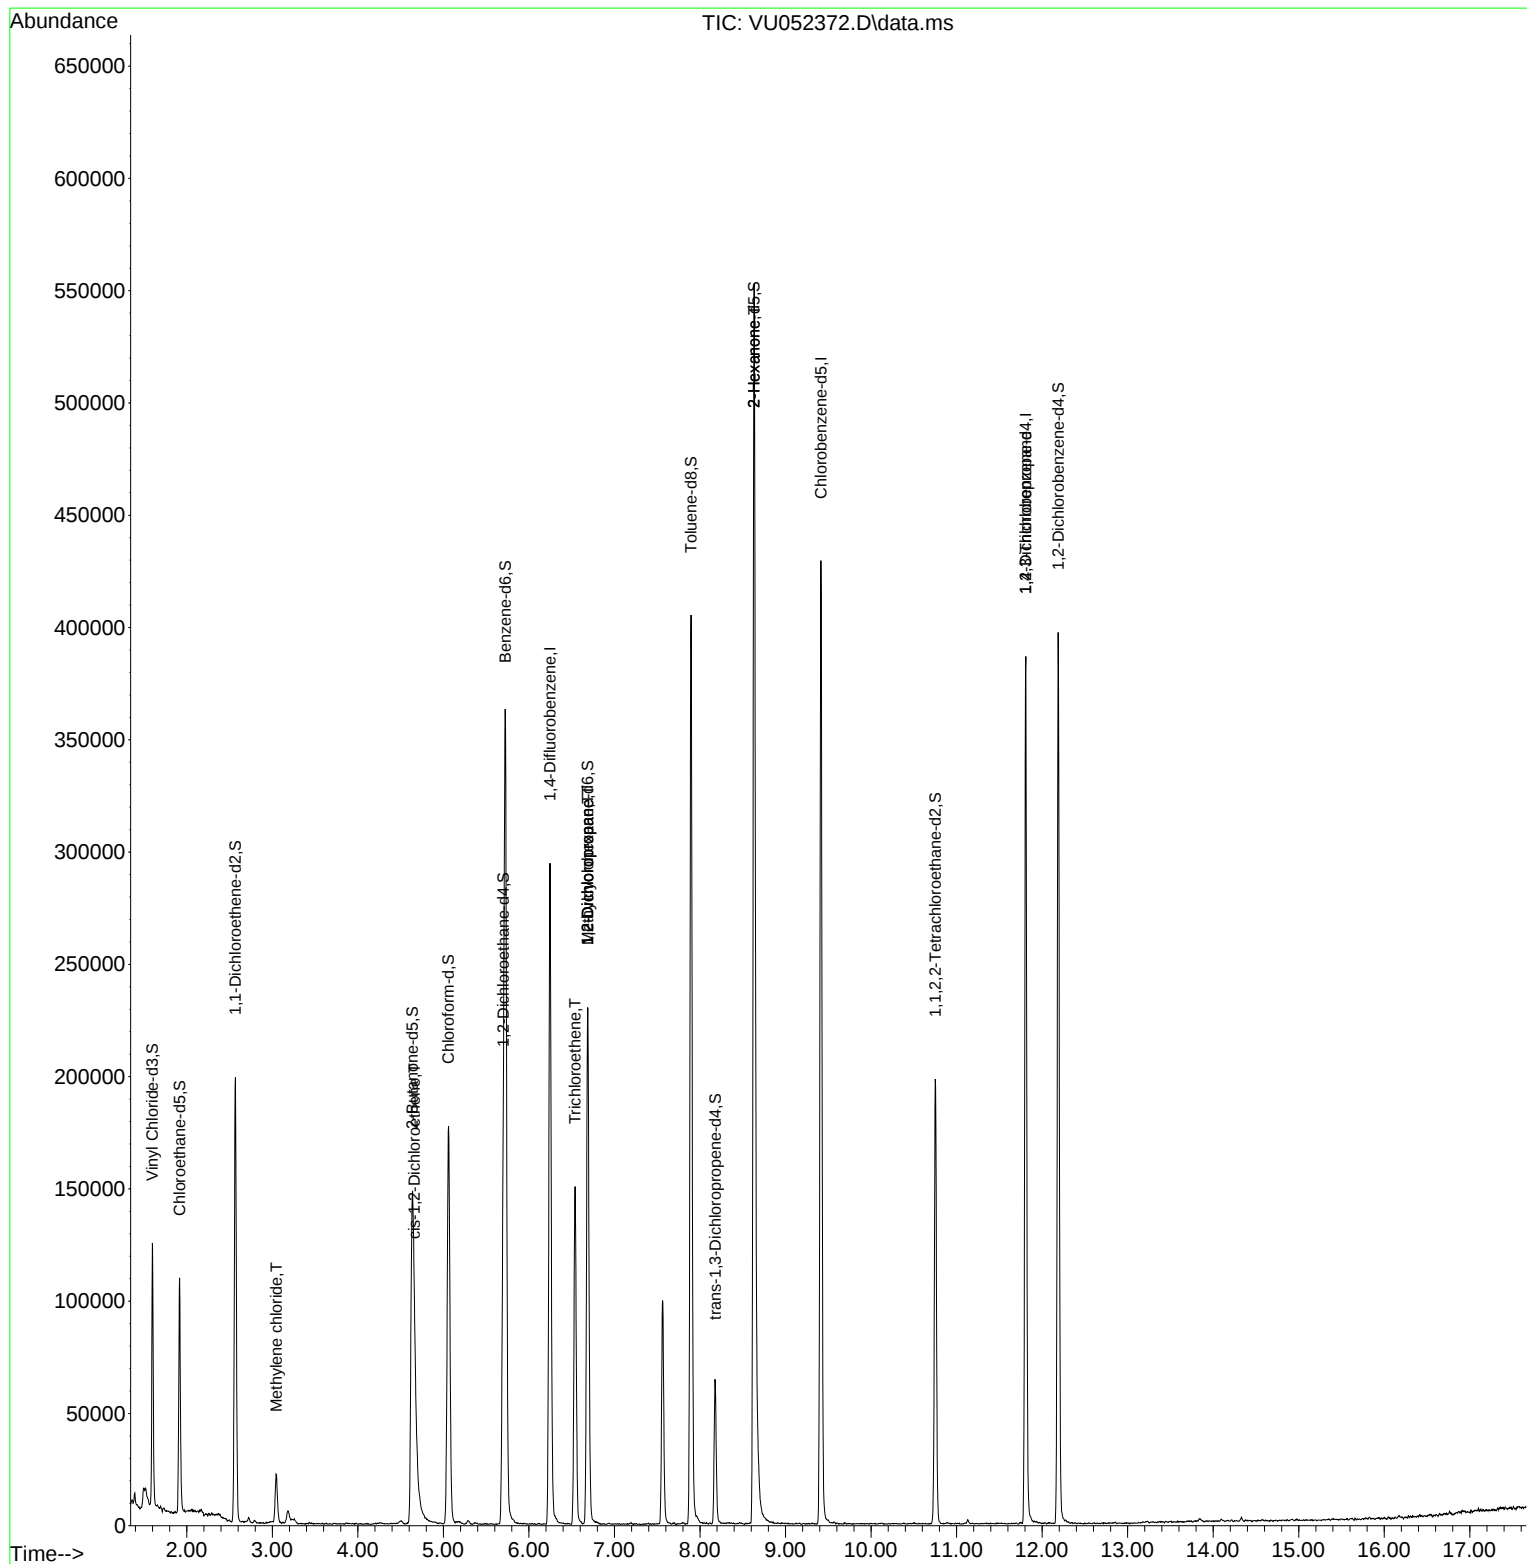


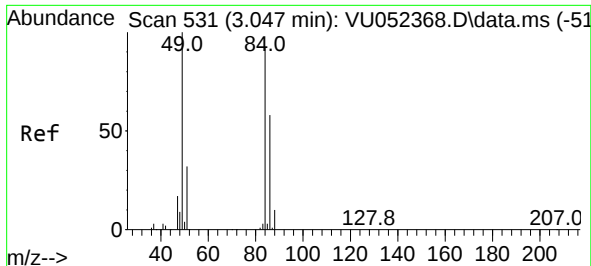

#16
Methylene chloride
Concen: 0.458 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU052372.D
Acq: 13 Dec 2022 13:15




Instrument :
MSVOA_U
ClientSampleId :
COL32DL


Tgt Ion: 84 Resp: 11032
Ion Ratio Lower Upper
84 100
86 62.3 43.8 81.4
49 107.5 75.9 141.1

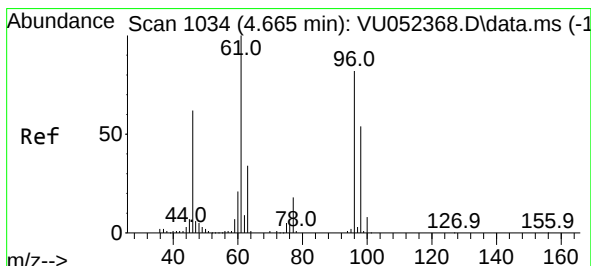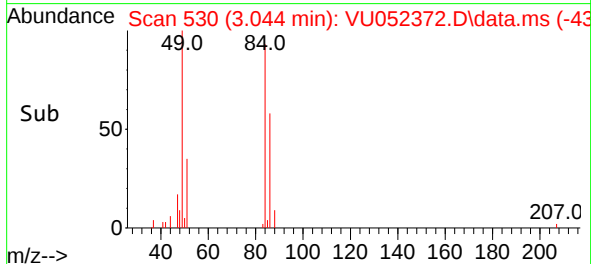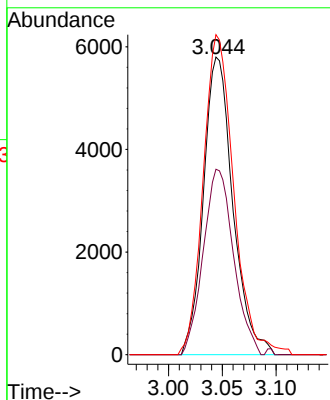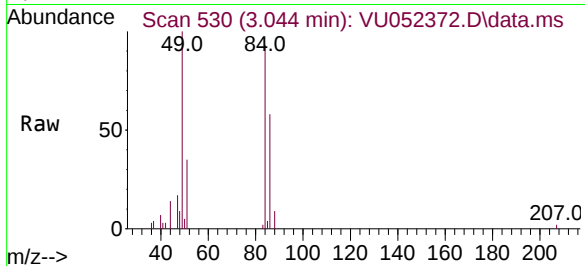

#22
cis-1,2-Dichloroethene
Concen: 0.261 ug/L
RT: 4.661 min Scan# 1033
Delta R.T. -0.003 min
Lab File: VU052372.D
Acq: 13 Dec 2022 13:15

Tgt Ion: 96 Resp: 5235
Ion Ratio Lower Upper
96 100
61 133.8 85.1 158.1
98 61.7 42.8 79.6


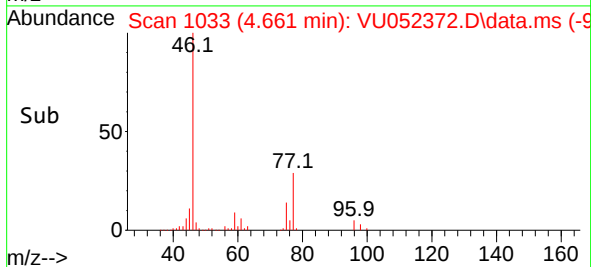
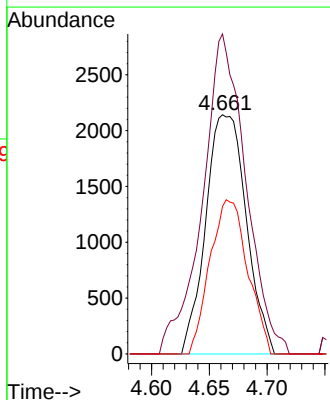
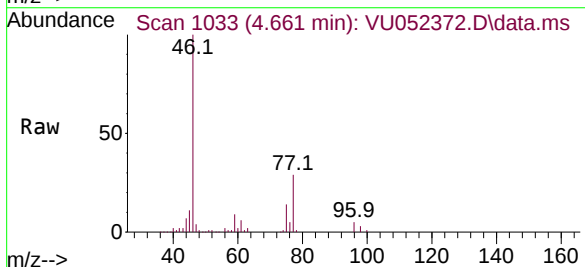


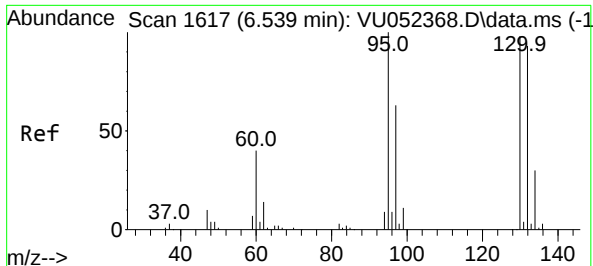

#34
Trichloroethene
Concen: 2.604 ug/L
RT: 6.539 min Scan# 1617
Delta R.T. -0.000 min
Lab File: VU052372.D
Acq: 13 Dec 2022 13:15




Instrument :
MSVOA_U
ClientSampleId :
COL32DL


Tgt Ion: 95 Resp: 52328
Ion Ratio Lower Upper
95 100
97 65.7 43.7 81.1
132 93.9 64.3 119.3
130 97.2 67.3 124.9

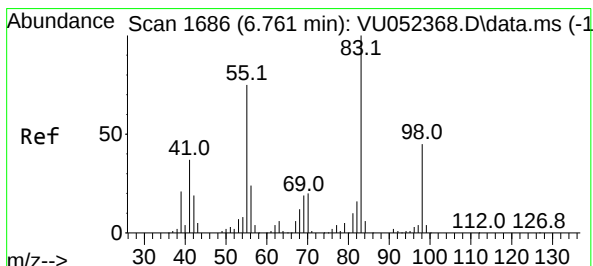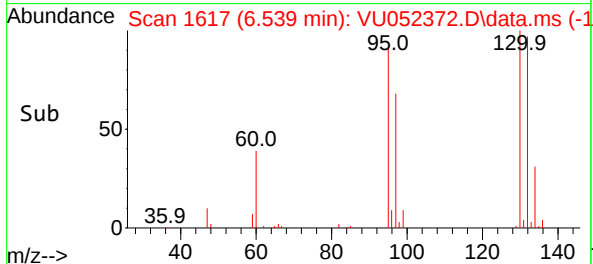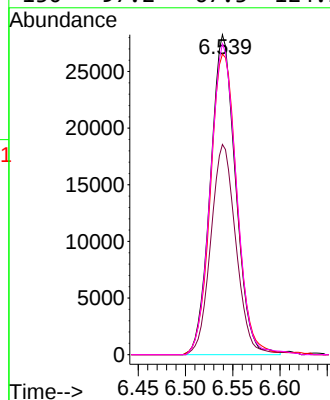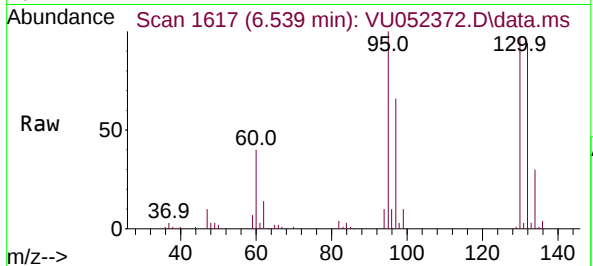

#35
Methylcyclohexane
Concen: 0.914 ug/L
RT: 6.687 min Scan# 1663
Delta R.T. -0.074 min
Lab File: VU052372.D
Acq: 13 Dec 2022 13:15

Tgt Ion: 83 Resp: 26423
Ion Ratio Lower Upper
83 100
55 0.1 60.8 91.2#
98 1.5 35.1 52.7#


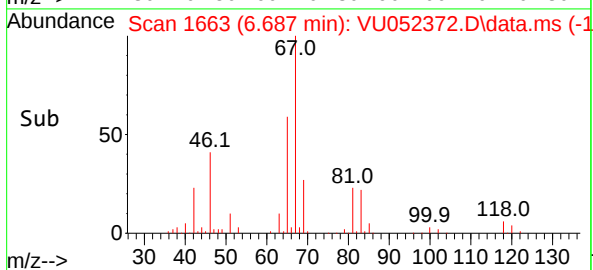
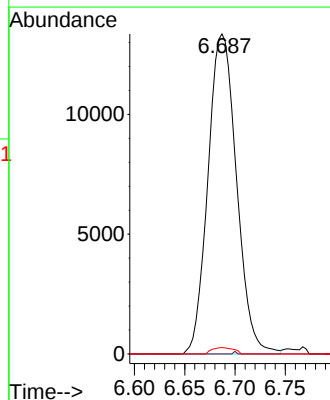
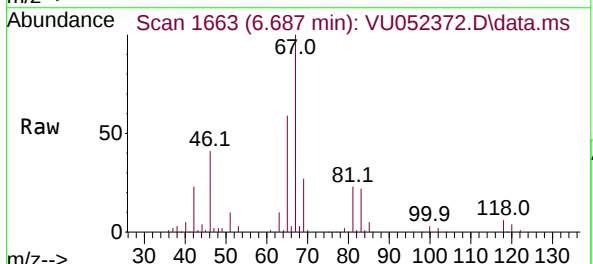


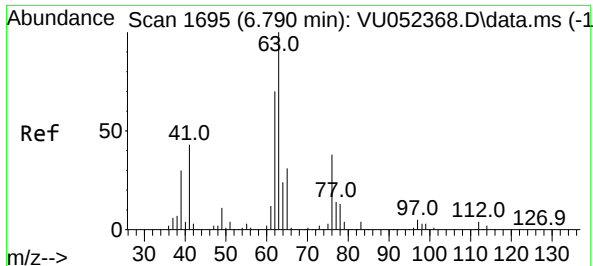

#37
1,2-Dichloropropane
Concen: 0.541 ug/L
RT: 6.687 min Scan# 11
Delta R.T. -0.103 min
Lab File: VU052372.D
Acq: 13 Dec 2022 13:15




Instrument :
MSVOA_U
ClientSampleId :
COL32DL


Tgt Ion: 63 Resp: 11284
Ion Ratio Lower Upper
63 100
112 0.0 3.3 4.9#

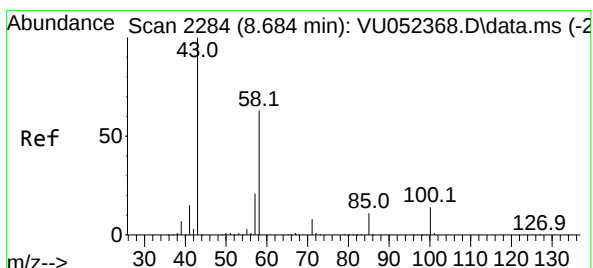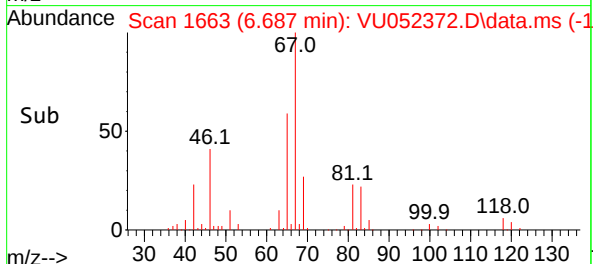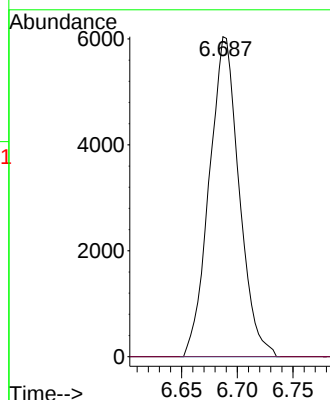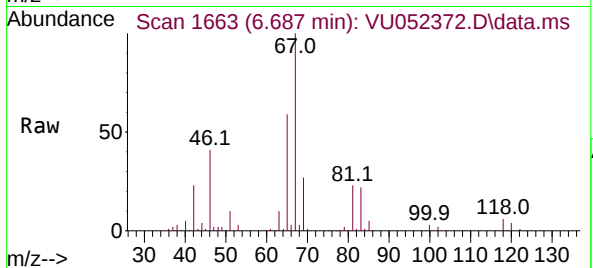

#48
2-Hexanone
Concen: 3.120 ug/L
RT: 8.632 min Scan# 2268
Delta R.T. -0.051 min
Lab File: VU052372.D
Acq: 13 Dec 2022 13:15

Tgt Ion: 43 Resp: 24926
Ion Ratio Lower Upper
43 100
58 42.9 49.4 74.0#
57 36.3 16.3 24.5#
100 3.8 10.4 15.6#

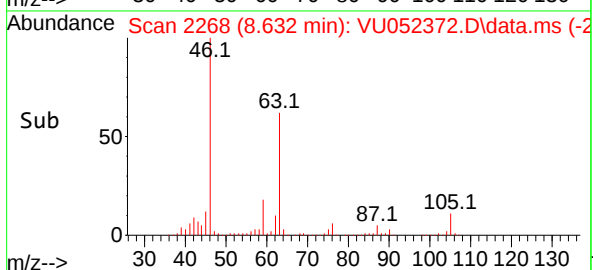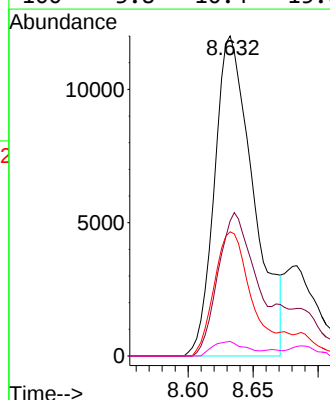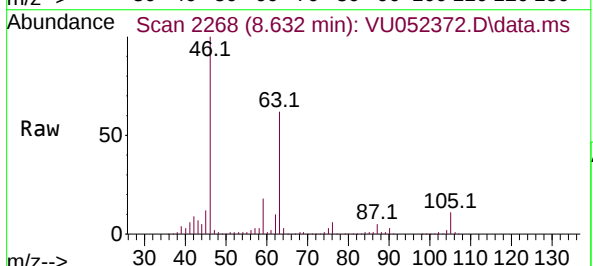

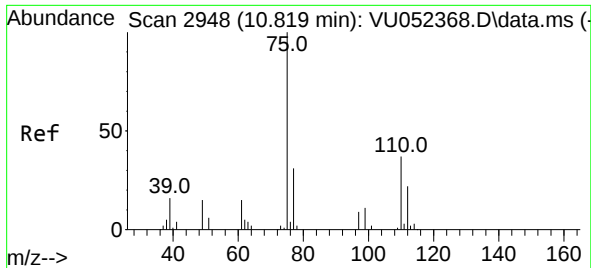

#61

1,2,3-Trichloropropane

Concen: 1.042 ug/L

RT: 11.809 min Scan# 31

Delta R.T. 0.990 min

Lab File: VU052372.D


Acq: 13 Dec 2022 13:15

Instrument :

MSVOA_U

ClientSampleId :

C0L32DL

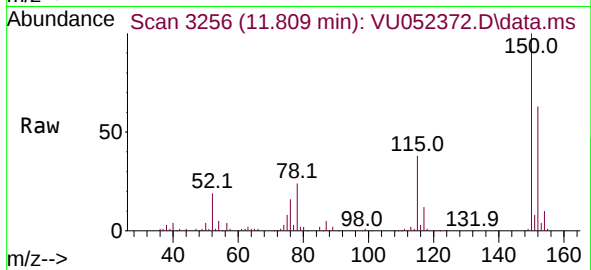

Tgt Ion: 75 Resp: 12965

Ion Ratio Lower Upper

75 100

110 1.6 28.3 42.5#

77 30.8 26.2 39.2

