

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
 Data File : VU052371.D
 Acq On : 13 Dec 2022 12:52
 Operator : JC/MD
 Sample : N6030-02DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL31DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.498	39	49	69	rBV4	11266	36926	3.43%	0.431%
2	1.600	73	81	95	rVB	120447	141047	13.12%	1.646%
3	1.916	170	179	192	rBV	100889	136562	12.70%	1.594%
4	2.568	369	382	402	rVB	199100	327957	30.50%	3.827%
5	3.044	518	530	554	rVB3	23712	49297	4.59%	0.575%
6	4.642	1007	1027	1061	rBV	145506	534104	49.68%	6.233%
7	5.060	1136	1157	1179	rBV2	179255	396179	36.85%	4.623%
8	5.723	1341	1363	1395	rBV2	362563	946271	88.02%	11.043%
9	6.247	1512	1526	1547	rBV	296735	574929	53.48%	6.709%
10	6.539	1603	1617	1638	rBV	294433	562360	52.31%	6.563%
11	6.687	1648	1663	1684	rBV	228543	445530	41.44%	5.199%
12	7.565	1923	1936	1958	rBV	98301	179384	16.69%	2.093%
13	7.896	2025	2039	2060	rBV	409271	721547	67.11%	8.420%
14	8.176	2115	2126	2139	rBV	63116	106972	9.95%	1.248%
15	8.632	2253	2268	2311	rBV3	531117	1075118	100.00%	12.547%
16	9.414	2496	2511	2536	rBV	434733	730998	67.99%	8.531%
17	10.751	2912	2927	2945	rBV	197986	324460	30.18%	3.786%
18	11.809	3243	3256	3275	rBV	385486	636799	59.23%	7.431%
19	12.188	3361	3374	3393	rBV	395044	642531	59.76%	7.498%




Sum of corrected areas: 8568971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052371.D
Acq On : 13 Dec 2022 12:52
Operator : JC/MD
Sample : N6030-02DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

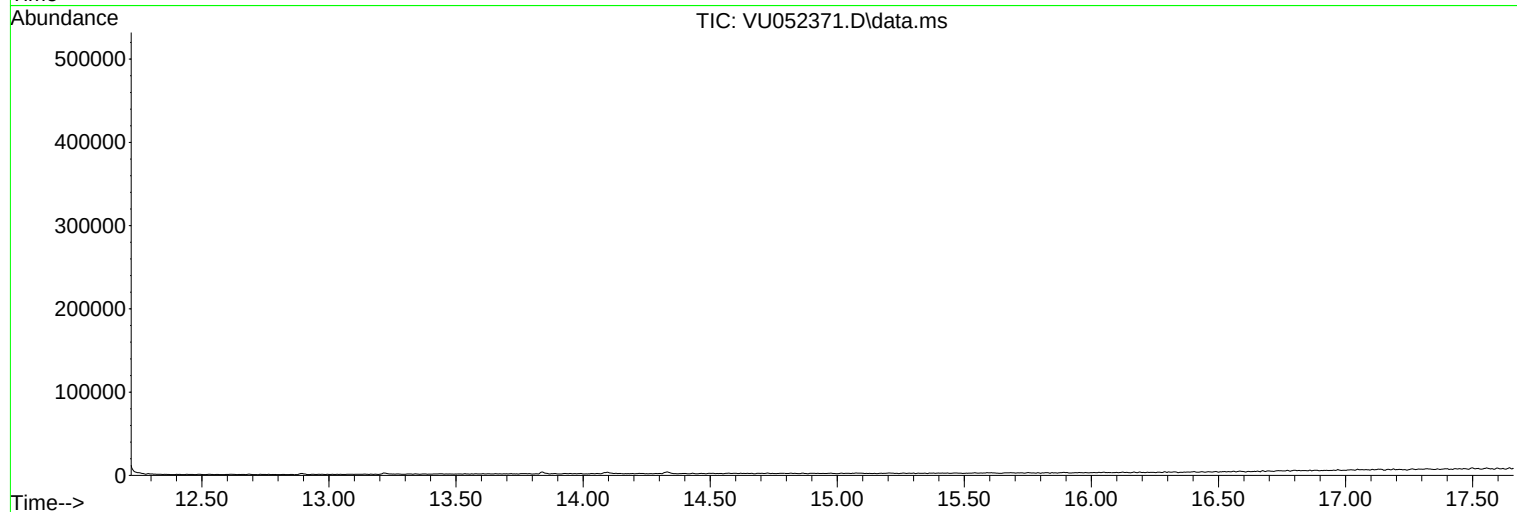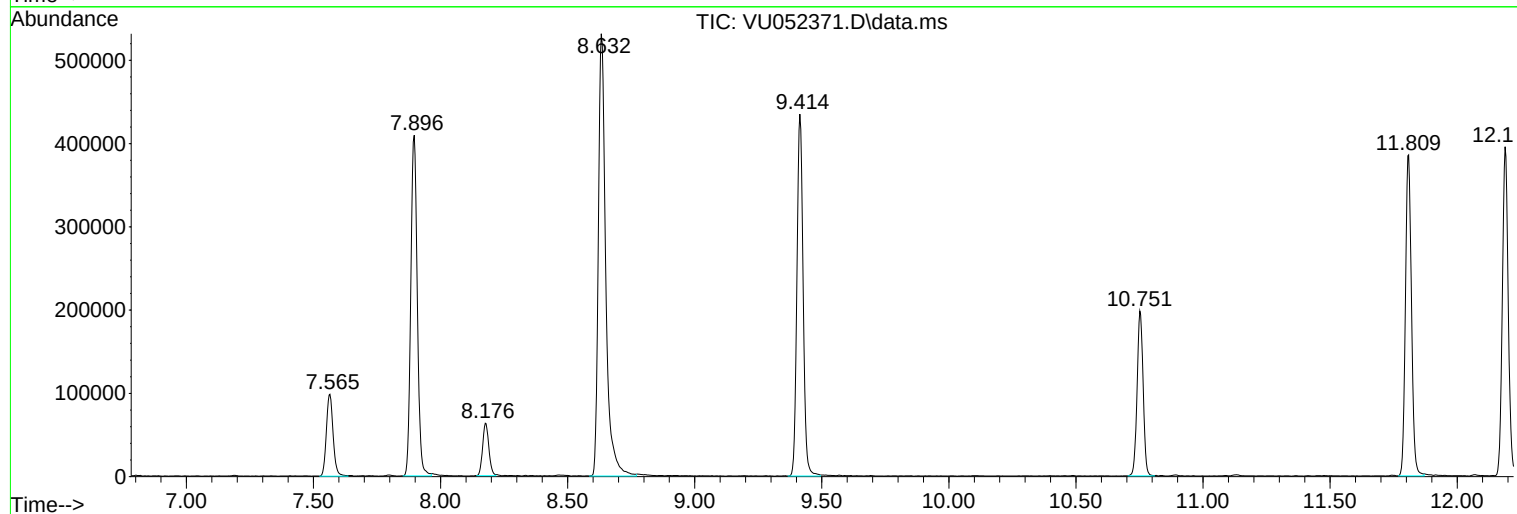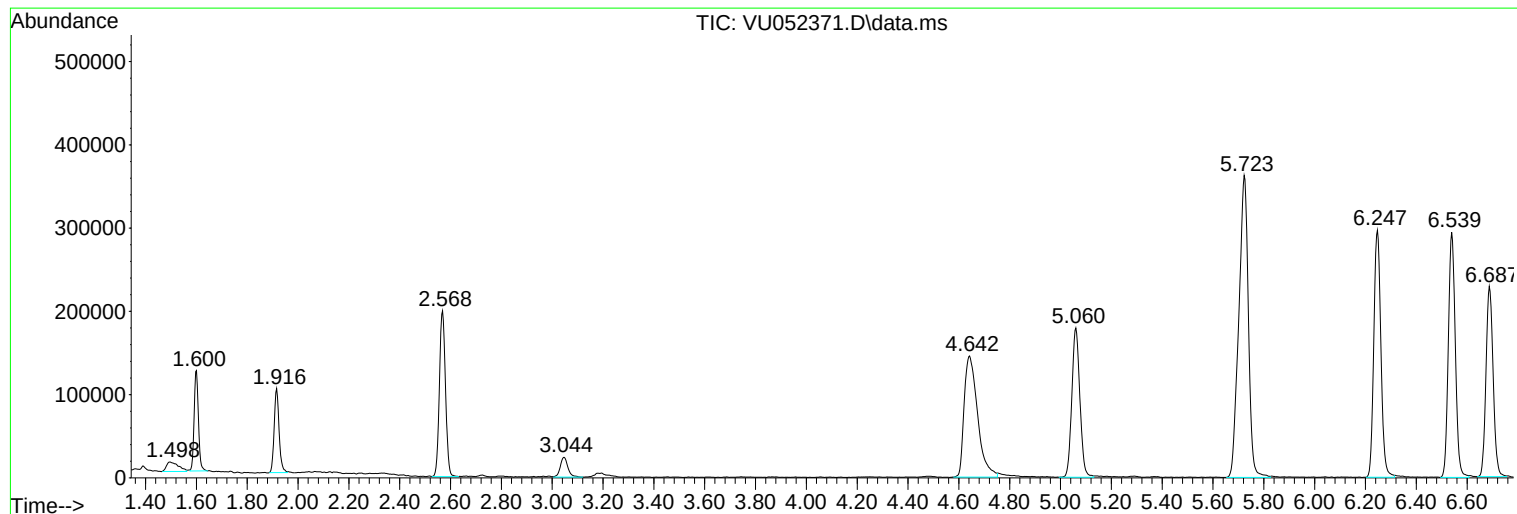

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052371.D
Acq On : 13 Dec 2022 12:52
Operator : JC/MD
Sample : N6030-02DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052371.D
Acq On : 13 Dec 2022 12:52
Operator : JC/MD
Sample : N6030-02DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc