

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
 Data File : VU052372.D
 Acq On : 13 Dec 2022 13:15
 Operator : JC/MD
 Sample : N6030-03DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L32DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	117123	135764	12.25%	1.647%
2	1.915	170	179	196	rBV	104282	138772	12.52%	1.683%
3	2.568	369	382	400	rBV	197940	323545	29.20%	3.924%
4	3.044	520	530	544	rVB2	21364	39130	3.53%	0.475%
5	3.182	560	573	584	rBV3	5435	12914	1.17%	0.157%
6	4.639	1009	1026	1072	rBV	148075	530297	47.85%	6.432%
7	5.060	1137	1157	1181	rBV	177050	394006	35.56%	4.779%
8	5.722	1341	1363	1388	rBV2	362829	945920	85.36%	11.474%
9	6.246	1512	1526	1543	rBV	294419	560781	50.60%	6.802%
10	6.539	1604	1617	1644	rBV	150411	284528	25.68%	3.451%
11	6.687	1648	1663	1690	rBV	229851	450552	40.66%	5.465%
12	7.562	1924	1935	1961	rBV	99203	176676	15.94%	2.143%
13	7.896	2025	2039	2057	rBV	404802	716181	64.63%	8.687%
14	8.176	2114	2126	2148	rBV	64387	109797	9.91%	1.332%
15	8.632	2256	2268	2313	rBV2	552084	1108158	100.00%	13.441%
16	9.414	2496	2511	2534	rBV	429040	717263	64.73%	8.700%
17	10.751	2910	2927	2948	rBV	198135	328714	29.66%	3.987%
18	11.809	3243	3256	3280	rBV	386207	622434	56.17%	7.550%
19	12.188	3361	3374	3398	rBV	396770	648878	58.55%	7.871%




Sum of corrected areas: 8244310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052372.D
Acq On : 13 Dec 2022 13:15
Operator : JC/MD
Sample : N6030-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

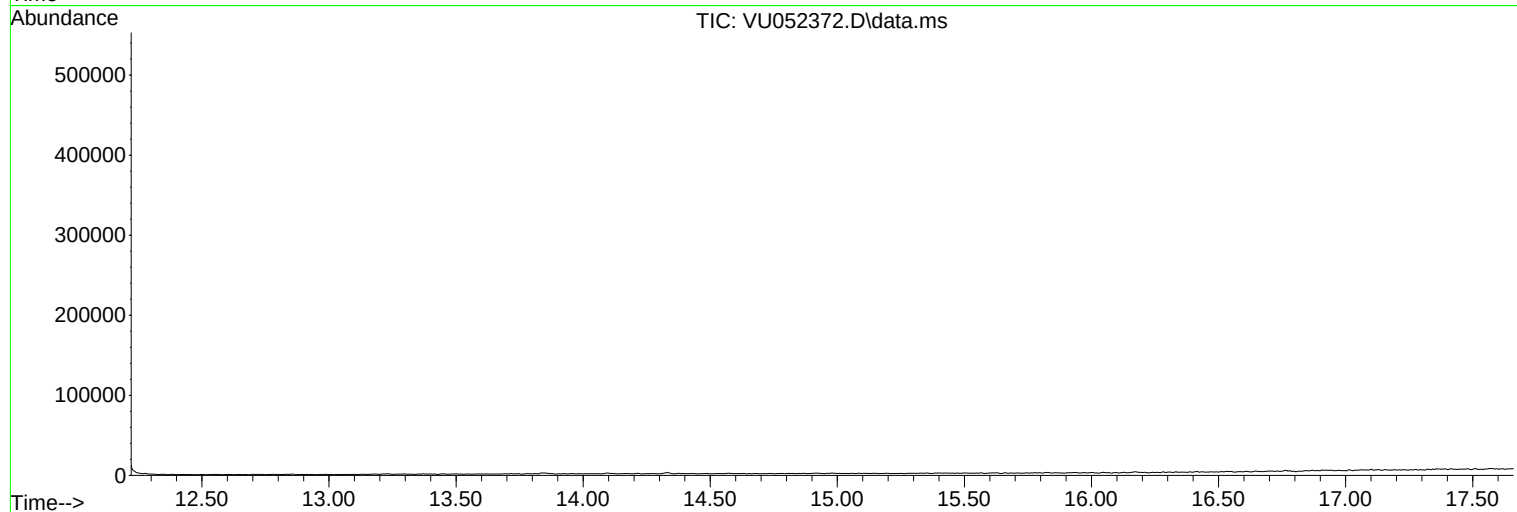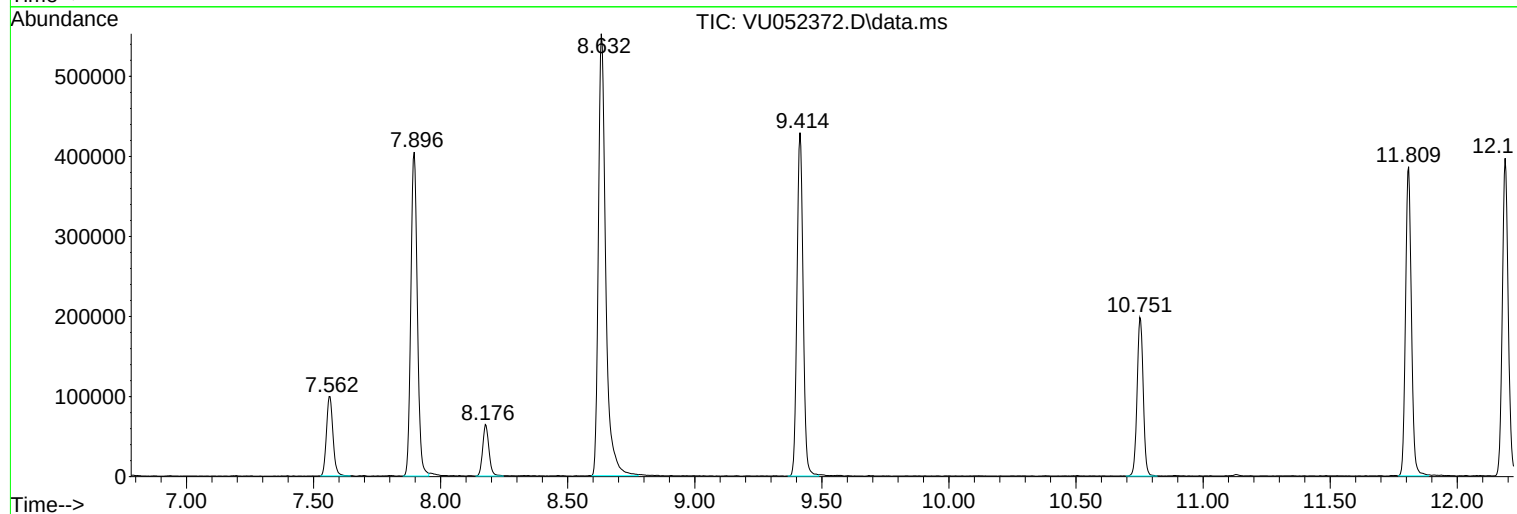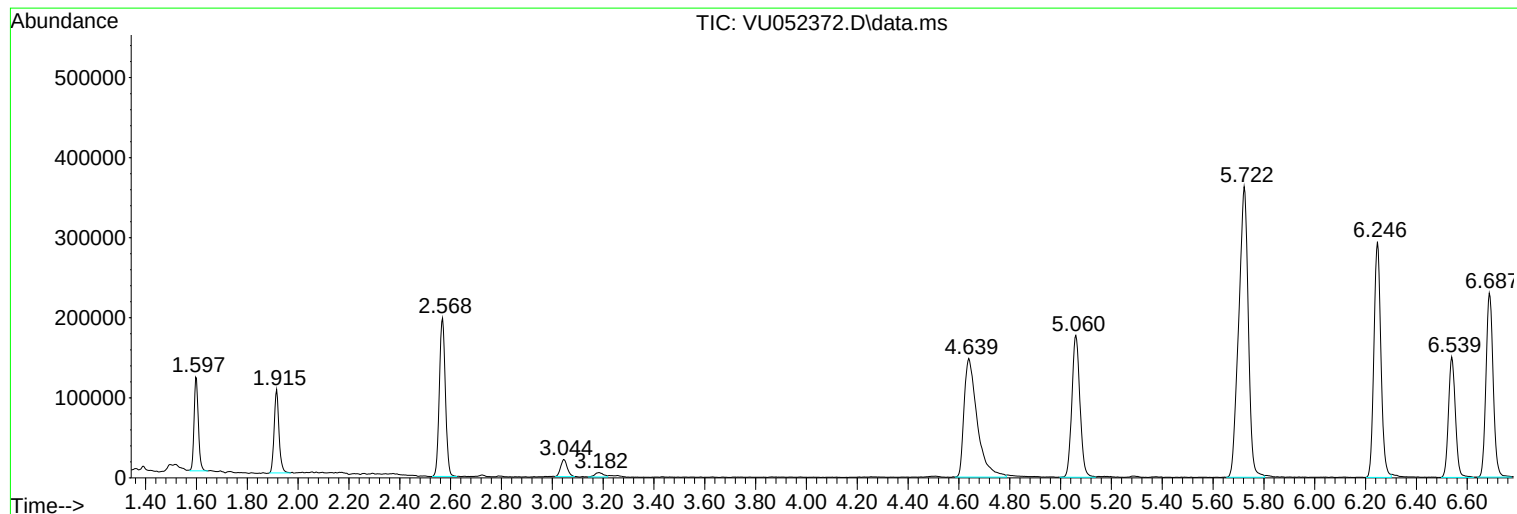

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052372.D
Acq On : 13 Dec 2022 13:15
Operator : JC/MD
Sample : N6030-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052372.D
Acq On : 13 Dec 2022 13:15
Operator : JC/MD
Sample : N6030-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc