

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
 Data File : VU052374.D
 Acq On : 13 Dec 2022 14:02
 Operator : JC/MD
 Sample : N6030-05DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L34DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.498	41	49	53	rBV3	8671	13944	1.31%	0.170%
2	1.601	73	81	95	rVB	113100	132082	12.45%	1.612%
3	1.916	171	179	192	rBV	100338	134098	12.64%	1.637%
4	2.568	370	382	398	rVB	186956	305258	28.77%	3.726%
5	3.047	519	531	544	rBV	51347	99138	9.34%	1.210%
6	4.639	1005	1026	1068	rBV2	137831	490373	46.22%	5.986%
7	5.060	1137	1157	1183	rBV	180052	399008	37.61%	4.870%
8	5.723	1342	1363	1392	rBV2	354304	938562	88.46%	11.456%
9	6.247	1512	1526	1548	rBV	298175	572521	53.96%	6.988%
10	6.539	1603	1617	1640	rBV	143707	276123	26.02%	3.370%
11	6.687	1649	1663	1687	rBV	229446	452319	42.63%	5.521%
12	7.562	1923	1935	1960	rBV	98419	177658	16.74%	2.169%
13	7.896	2026	2039	2059	rBV	405405	709136	66.84%	8.656%
14	8.176	2110	2126	2143	rBV2	61652	107666	10.15%	1.314%
15	8.632	2253	2268	2305	rBV2	529420	1061007	100.00%	12.951%
16	9.414	2498	2511	2534	rBV	435235	733781	69.16%	8.957%
17	10.751	2910	2927	2949	rBV	194427	322393	30.39%	3.935%
18	11.809	3242	3256	3277	rBV	387837	626254	59.02%	7.644%
19	12.189	3361	3374	3406	rBV	387573	641221	60.44%	7.827%




Sum of corrected areas: 8192542

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052374.D
Acq On : 13 Dec 2022 14:02
Operator : JC/MD
Sample : N6030-05DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

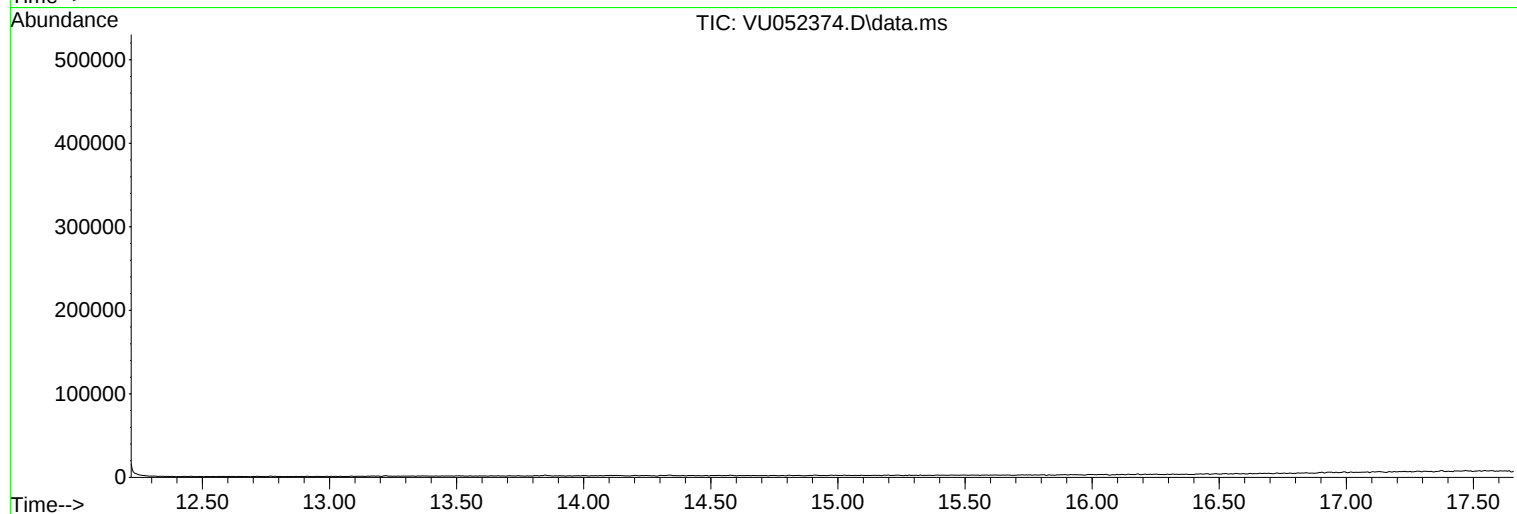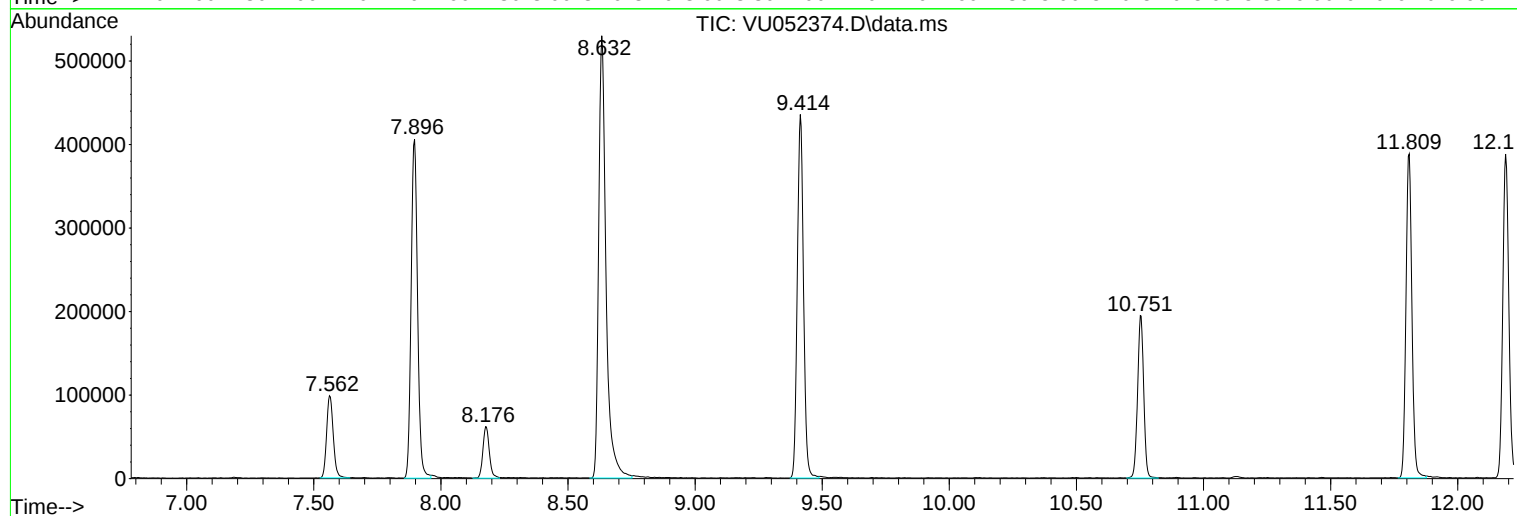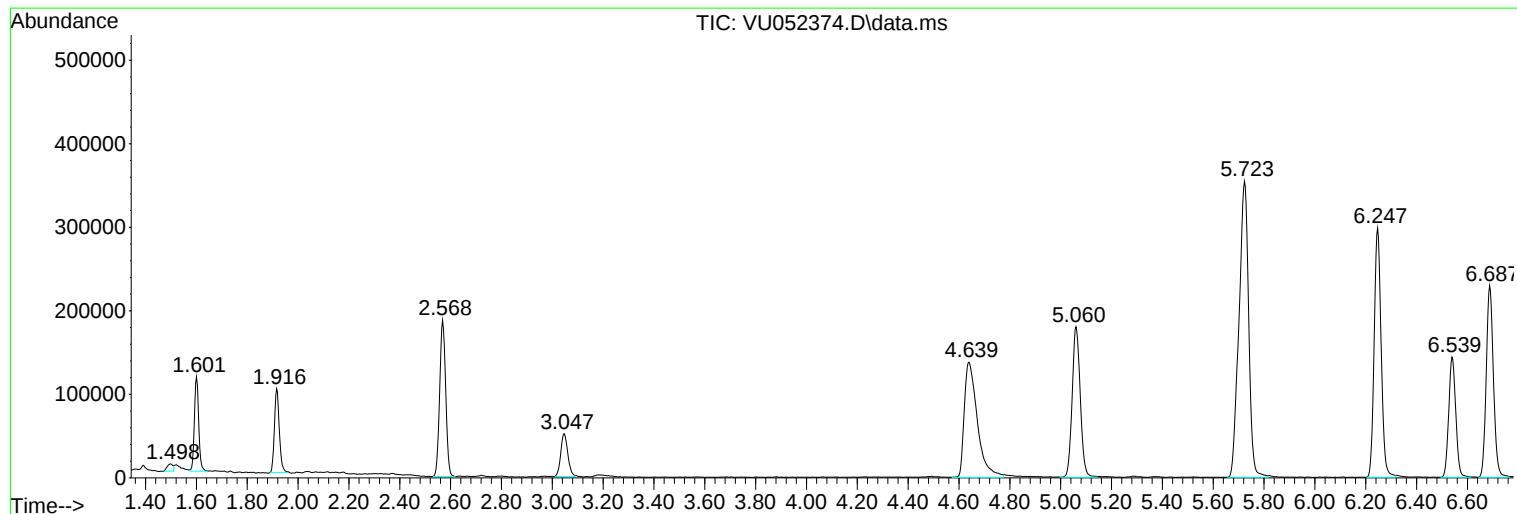

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052374.D
Acq On : 13 Dec 2022 14:02
Operator : JC/MD
Sample : N6030-05DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052374.D
Acq On : 13 Dec 2022 14:02
Operator : JC/MD
Sample : N6030-05DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc