
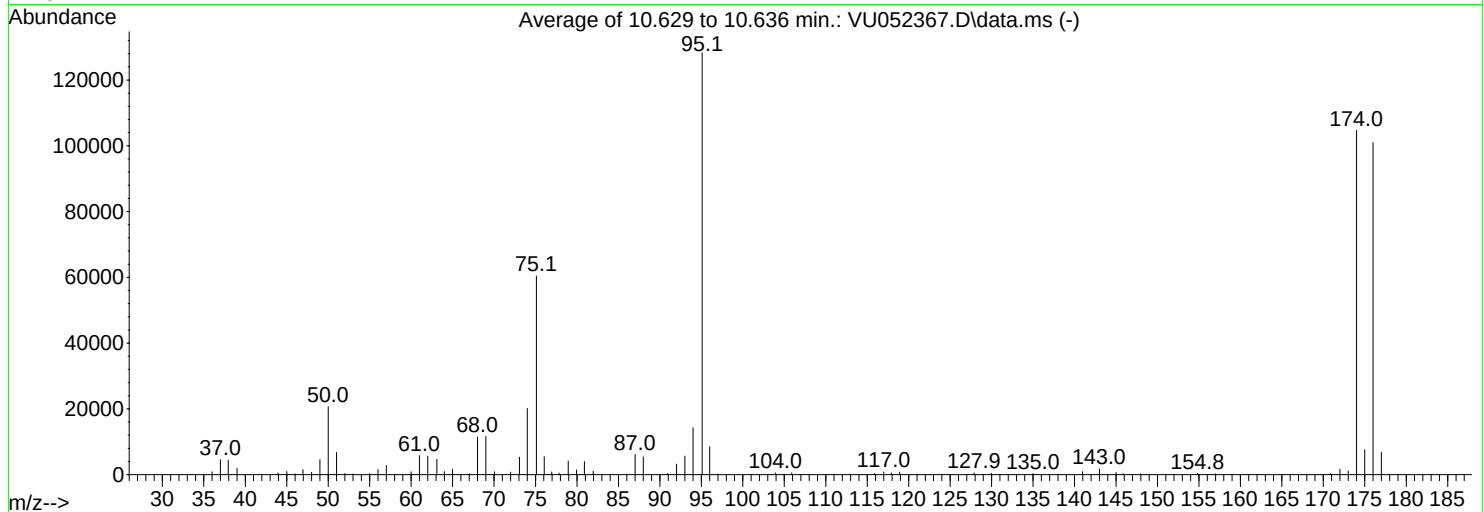


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121322\
Data File : VU052367.D
Acq On : 13 Dec 2022 09:25
Operator : JC/MD
Sample : BFB178
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB178

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 14 03:17:56 2022

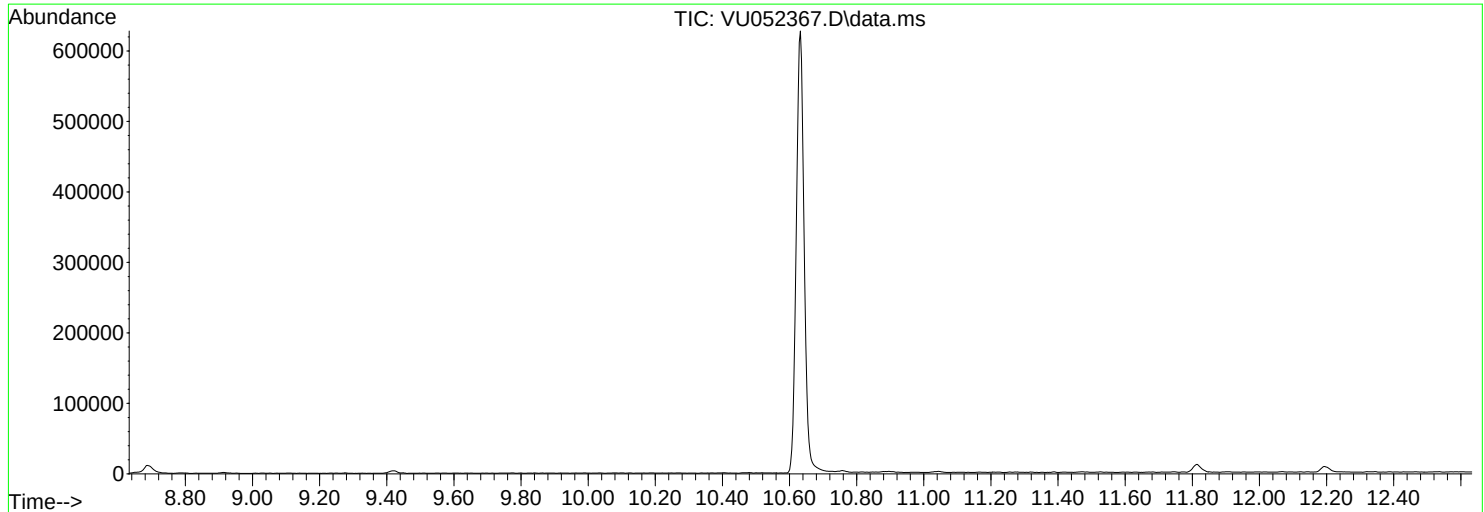

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	20659	PASS
75	95	30	80	47.1	60429	PASS
95	95	100	100	100.0	128264	PASS
96	95	5	9	6.6	8523	PASS
173	174	0.00	2	1.1	1139	PASS
174	95	50	120	81.6	104685	PASS
175	174	5	9	7.2	7572	PASS
176	174	95	101	96.5	101000	PASS
177	176	5	9	6.7	6766	PASS

m/z	Abundance
36.00	271.0
37.80	111.0
40.00	487.0
43.90	416.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178

m/z	Abundance
36.00	1220.0
37.00	4629.0
38.00	4651.0
39.00	2009.0
39.90	568.0
44.00	932.0
45.00	898.0
46.00	320.0
47.00	1782.0
48.00	669.0
49.00	4727.0
50.00	21408.0
51.00	6893.0
52.00	388.0
52.90	156.0
55.00	309.0
56.00	1593.0
57.00	2841.0
58.10	184.0
60.00	1053.0
61.00	6130.0
62.00	5570.0
63.10	4798.0
64.00	914.0
65.00	1541.0
66.00	160.0
67.10	282.0
68.00	11385.0
69.00	11778.0
70.10	826.0
72.00	823.0
73.10	5263.0
74.00	20208.0
75.10	61504.0
76.00	5497.0
77.00	877.0
77.80	555.0
79.00	4187.0
79.90	1549.0
80.90	4180.0
82.00	1111.0
83.00	113.0
86.10	216.0
87.00	5997.0
88.00	5593.0
90.90	477.0
92.00	3028.0
93.00	5530.0
94.00	14494.0
95.10	129896.0
96.00	8462.0
97.00	228.0
104.00	536.0
104.90	192.0
105.90	595.0
106.90	119.0
114.90	116.0
115.90	415.0
117.00	799.0
117.90	583.0
118.90	754.0
126.90	129.0
127.90	484.0
128.90	138.0
129.90	486.0
130.90	176.0
135.00	304.0
136.90	158.0
141.00	917.0
143.00	1822.0
145.00	750.0
145.80	257.0
146.80	110.0
148.00	332.0
154.90	322.0
157.00	195.0
158.90	120.0
160.80	128.0
170.90	339.0
172.00	1806.0
173.00	1029.0
174.00	103552.0
175.00	7909.0
176.00	99024.0
177.00	6965.0
177.90	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178

m/z	Abundance
36.00	1211.0
37.00	4680.0
38.00	4679.0
39.00	1992.0
39.90	500.0
44.00	957.0
45.00	916.0
46.00	259.0
47.00	1625.0
48.00	777.0
49.00	4774.0
50.00	21344.0
51.00	6917.0
52.00	347.0
52.90	178.0
55.00	335.0
56.00	1568.0
57.00	2788.0
58.00	145.0
60.00	897.0
61.00	6069.0
62.00	5879.0
63.10	4877.0
64.00	981.0
65.00	1714.0
66.00	158.0
67.10	286.0
68.00	11797.0
69.00	11894.0
70.10	926.0
72.00	826.0
73.00	5388.0
74.00	20816.0
75.10	62448.0
76.00	5650.0
77.00	814.0
77.80	489.0
79.00	4311.0
79.90	1472.0
80.90	4087.0
81.90	1128.0
83.00	117.0
86.00	191.0
87.00	6386.0
88.00	5572.0
91.00	404.0
92.00	3285.0
93.00	5873.0
94.00	14631.0
95.10	132352.0
96.00	8806.0
96.90	205.0
104.00	546.0
104.90	178.0
105.90	564.0
106.90	101.0
114.90	112.0
115.90	386.0
117.00	810.0
117.90	559.0
118.90	802.0
126.90	125.0
127.90	552.0
128.90	137.0
129.90	433.0
130.90	178.0
135.00	401.0
137.00	157.0
140.90	943.0
143.00	1765.0
145.00	794.0
145.80	292.0
146.80	128.0
148.00	331.0
154.90	386.0
157.00	238.0
158.90	120.0
160.80	128.0
170.90	334.0
172.00	1741.0
173.00	1178.0
174.00	107720.0
175.00	7760.0
176.00	104440.0
177.00	7011.0
177.90	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178

m/z	Abundance
36.00	1083.0
37.00	4220.0
38.00	4238.0
39.00	1807.0
39.90	413.0
44.00	946.0
45.00	940.0
46.00	232.0
46.90	1311.0
48.00	753.0
49.00	4234.0
50.00	19224.0
51.00	6469.0
52.00	314.0
53.00	206.0
55.00	325.0
56.00	1468.0
57.00	2661.0
58.00	100.0
60.00	705.0
61.00	5205.0
62.00	5515.0
63.10	4373.0
64.00	942.0
65.00	1609.0
66.00	114.0
67.00	298.0
68.00	11068.0
69.00	11220.0
70.00	913.0
72.00	735.0
73.00	5269.0
74.00	19368.0
75.10	57336.0
76.10	5181.0
76.90	761.0
77.90	480.0
78.90	3956.0
80.00	1267.0
80.90	3711.0
81.90	1047.0
83.00	107.0
85.90	185.0
87.00	6028.0
88.00	5096.0
91.00	359.0
92.00	3386.0
93.00	5578.0
94.00	13624.0
95.10	122544.0
96.00	8302.0
96.90	207.0
103.90	577.0
105.00	155.0
105.90	458.0
112.90	100.0
115.90	331.0
117.00	772.0
117.90	434.0
118.90	710.0
127.90	558.0
128.90	158.0
130.00	383.0
130.90	147.0
135.00	373.0
137.00	167.0
140.90	942.0
143.00	1671.0
145.00	695.0
145.90	275.0
147.90	287.0
154.80	406.0
157.00	257.0
158.90	102.0
160.80	126.0
170.90	308.0
172.00	1580.0
173.00	1210.0
174.00	102784.0
175.00	7047.0
176.00	99536.0
177.00	6321.0
177.90	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178