

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121418\
 Data File : VU028669.D
 Acq On : 13 Dec 2018 10:48
 Operator : MD/SY
 Sample : J6347-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-A-181210-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.324	351	358	372	rVB3	2676	4942	4.63%	1.743%
2	2.447	384	396	418	rBV	60903	106752	100.00%	37.641%
3	2.620	442	450	459	rVB3	1839	3043	2.85%	1.073%
4	2.836	501	517	533	rBV2	7616	16795	15.73%	5.922%
5	4.250	941	957	975	rBV	9667	26900	25.20%	9.485%
6	4.395	993	1002	1012	rVB2	4160	7910	7.41%	2.789%
7	4.649	1076	1081	1083	rBV3	1334	1254	1.17%	0.442%
8	5.739	1409	1420	1432	rVB	20677	39123	36.65%	13.795%
9	6.835	1757	1761	1769	rVB4	1345	1753	1.64%	0.618%
10	7.630	2001	2008	2016	rBV3	1478	2328	2.18%	0.821%
11	9.372	2543	2550	2558	rBV4	1024	1561	1.46%	0.550%
12	10.308	2832	2841	2854	rVB	16258	23743	22.24%	8.372%
13	11.858	3314	3323	3338	rBV2	19305	30638	28.70%	10.803%
14	13.986	3979	3985	3992	rVB4	1938	2564	2.40%	0.904%
15	14.279	4066	4076	4089	rBV3	1975	3530	3.31%	1.245%
16	15.353	4400	4410	4421	rVB5	5225	7331	6.87%	2.585%
17	15.880	4565	4574	4583	rVB2	2129	3438	3.22%	1.212%


Sum of corrected areas: 283605

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121418\
Data File : VU028669.D
Acq On : 13 Dec 2018 10:48
Operator : MD/SY
Sample : J6347-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-A-181210-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

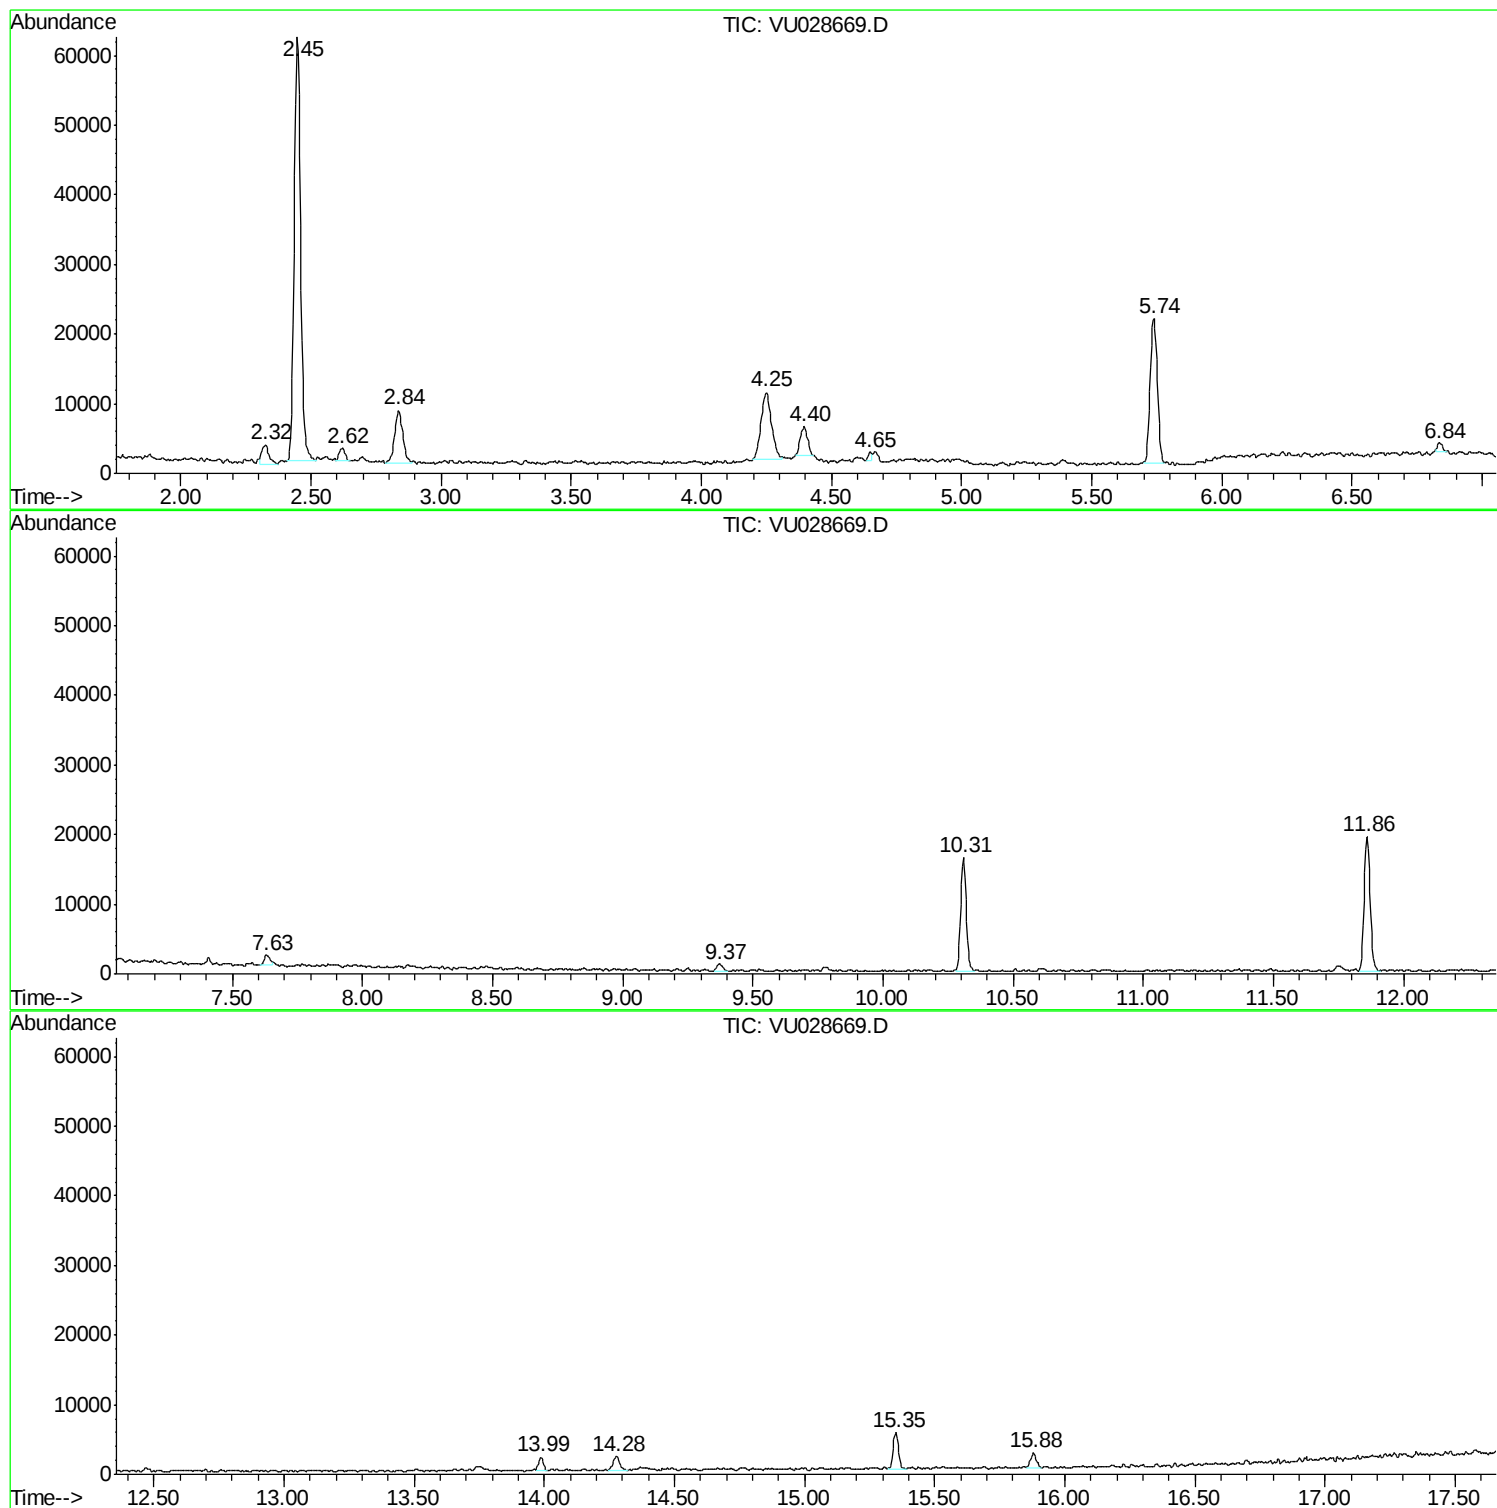

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121418\
Data File : VU028669.D
Acq On : 13 Dec 2018 10:48
Operator : MD/SY
Sample : J6347-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-A-181210-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121418\
Data File : VU028669.D
Acq On : 13 Dec 2018 10:48
Operator : MD/SY
Sample : J6347-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-A-181210-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc