

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121418\
 Data File : VU028670.D
 Acq On : 13 Dec 2018 11:17
 Operator : MD/SY
 Sample : J6377-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-C-181211-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.183	311	314	319	rVB2	479	355	1.08%	0.269%
2	2.250	329	335	337	rBV2	427	381	1.16%	0.289%
3	2.328	354	359	362	rBV2	645	551	1.68%	0.418%
4	2.443	390	395	396	rBV	540	457	1.39%	0.347%
5	2.546	425	427	431	rVV3	353	337	1.02%	0.256%
6	2.620	442	450	458	rBV2	2042	3190	9.70%	2.422%
7	2.839	509	518	528	rVB2	4108	7138	21.71%	5.418%
8	2.942	548	550	559	rVB4	401	437	1.33%	0.332%
9	3.138	607	611	614	rBV2	454	345	1.05%	0.262%
10	3.231	633	640	642	rBV2	523	573	1.74%	0.435%
11	3.347	671	676	683	rBV3	510	759	2.31%	0.576%
12	3.614	757	759	764	rBV	466	407	1.24%	0.309%
13	4.032	886	889	897	rVB	584	590	1.79%	0.448%
14	4.151	923	926	932	rBV2	440	425	1.29%	0.323%
15	4.244	949	955	960	rBV2	730	782	2.38%	0.594%
16	4.395	993	1002	1020	rVB2	3931	8467	25.75%	6.427%
17	4.655	1080	1083	1084	rBV2	605	344	1.05%	0.261%
18	5.376	1303	1307	1314	rBV2	455	509	1.55%	0.386%
19	5.655	1391	1394	1401	rVB2	430	414	1.26%	0.314%
20	5.736	1407	1419	1434	rBV	17059	32879	100.00%	24.958%
21	6.752	1732	1735	1738	rBV3	585	423	1.29%	0.321%
22	7.151	1855	1859	1864	rBV3	391	444	1.35%	0.337%
23	7.478	1958	1961	1969	rVB3	350	346	1.05%	0.263%
24	7.636	2001	2010	2018	rVB3	1813	2751	8.37%	2.088%
25	7.845	2070	2075	2077	rBV2	384	404	1.23%	0.307%
26	8.176	2172	2178	2180	rBV3	557	631	1.92%	0.479%
27	8.430	2254	2257	2261	rVB	547	450	1.37%	0.342%
28	8.884	2391	2398	2400	rBV	413	384	1.17%	0.291%
29	9.369	2542	2549	2561	rVB3	2322	3230	9.82%	2.452%
30	9.777	2667	2676	2682	rBV3	709	911	2.77%	0.692%
31	10.215	2803	2812	2818	rVB	215	352	1.07%	0.267%
32	10.308	2833	2841	2854	rVB4	12003	18485	56.22%	14.032%
33	10.736	2968	2974	2981	rVB	209	344	1.05%	0.261%
34	11.752	3283	3290	3296	rVB2	623	563	1.71%	0.427%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121418\
Data File : VU028670.D
Acq On : 13 Dec 2018 11:17
Operator : MD/SY
Sample : J6377-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-C-181211-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

35	11.861	3311	3324	3339	rBV2	15872	24210	73.63%	18.378%
36	13.745	3905	3910	3911	rBV	364	336	1.02%	0.255%
37	13.874	3945	3950	3959	rBV	345	454	1.38%	0.345%
38	13.986	3976	3985	3993	rBV4	2815	4092	12.45%	3.106%
39	14.189	4044	4048	4055	rBV2	358	348	1.06%	0.264%
40	14.279	4067	4076	4090	rVB3	1557	2985	9.08%	2.266%
41	14.379	4101	4107	4111	rBV	302	420	1.28%	0.319%
42	15.086	4318	4327	4330	rBV	245	423	1.29%	0.321%
43	15.292	4384	4391	4396	rBV2	254	344	1.05%	0.261%
44	15.353	4405	4410	4413	rBV2	488	515	1.57%	0.391%
45	15.449	4435	4440	4447	rVB2	298	413	1.26%	0.314%
46	15.880	4565	4574	4586	rBV2	2395	3912	11.90%	2.970%
47	16.375	4721	4728	4730	rBV3	516	510	1.55%	0.387%
48	16.922	4894	4898	4903	rBV4	469	562	1.71%	0.427%
49	17.079	4943	4947	4951	rBV3	611	594	1.81%	0.451%
50	17.263	5001	5004	5007	rVB2	662	435	1.32%	0.330%
51	17.288	5007	5012	5015	rBV5	824	795	2.42%	0.603%
52	17.436	5055	5058	5061	rBV3	676	497	1.51%	0.377%
53	17.594	5105	5107	5112	rBV4	558	448	1.36%	0.340%
54	17.620	5112	5115	5116	rBV3	607	384	1.17%	0.291%


Sum of corrected areas: 131735

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121418\
Data File : VU028670.D
Acq On : 13 Dec 2018 11:17
Operator : MD/SY
Sample : J6377-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-C-181211-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

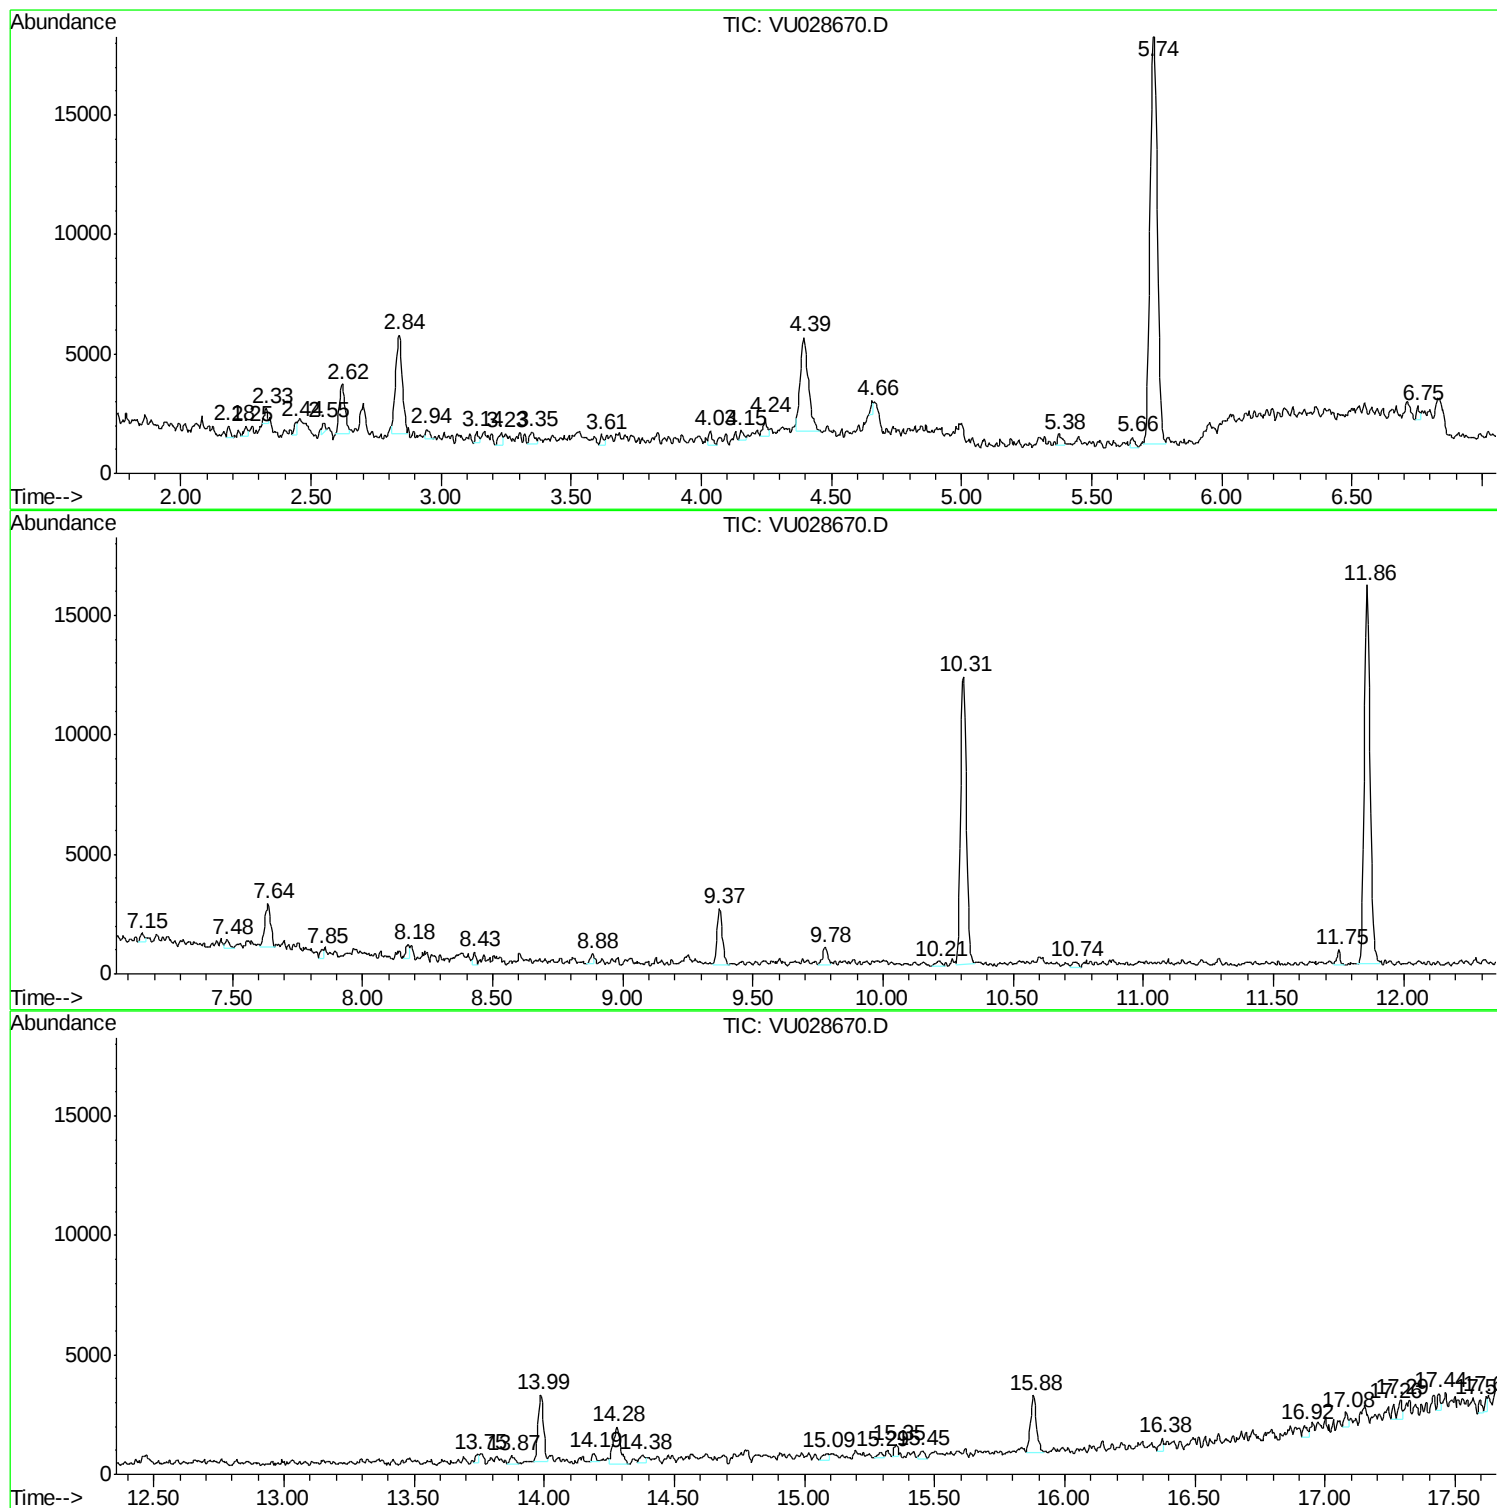

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121418\
Data File : VU028670.D
Acq On : 13 Dec 2018 11:17
Operator : MD/SY
Sample : J6377-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-C-181211-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121418\
Data File : VU028670.D
Acq On : 13 Dec 2018 11:17
Operator : MD/SY
Sample : J6377-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-C-181211-01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc