

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121418\
 Data File : VU028672.D
 Acq On : 13 Dec 2018 12:15
 Operator : MD/SY
 Sample : J6347-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 P001-TW001-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.324	347	358	370	rVB5	1508	2971	4.82%	1.765%
2	2.453	393	398	401	rVB5	841	821	1.33%	0.488%
3	2.617	438	449	461	rBV3	2234	4467	7.24%	2.654%
4	2.694	466	473	474	rBV	1950	1607	2.61%	0.955%
5	2.829	511	515	521	rBV5	1071	1443	2.34%	0.857%
6	4.257	944	959	965	rBV4	1226	3151	5.11%	1.872%
7	4.392	990	1001	1017	rVB	8908	19219	31.16%	11.420%
8	4.688	1088	1093	1097	rBV	610	624	1.01%	0.371%
9	5.739	1406	1420	1435	rBV	15921	30115	48.82%	17.894%
10	6.180	1544	1557	1570	rBV2	32764	61681	100.00%	36.651%
11	10.308	2832	2841	2854	rBV3	10398	16049	26.02%	9.536%
12	11.861	3310	3324	3340	rBV3	13569	21427	34.74%	12.732%
13	14.276	4068	4075	4076	rBV2	943	947	1.54%	0.563%
14	15.880	4564	4574	4584	rVB2	2286	3772	6.12%	2.241%


Sum of corrected areas: 168294

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121418\
Data File : VU028672.D
Acq On : 13 Dec 2018 12:15
Operator : MD/SY
Sample : J6347-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW001-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

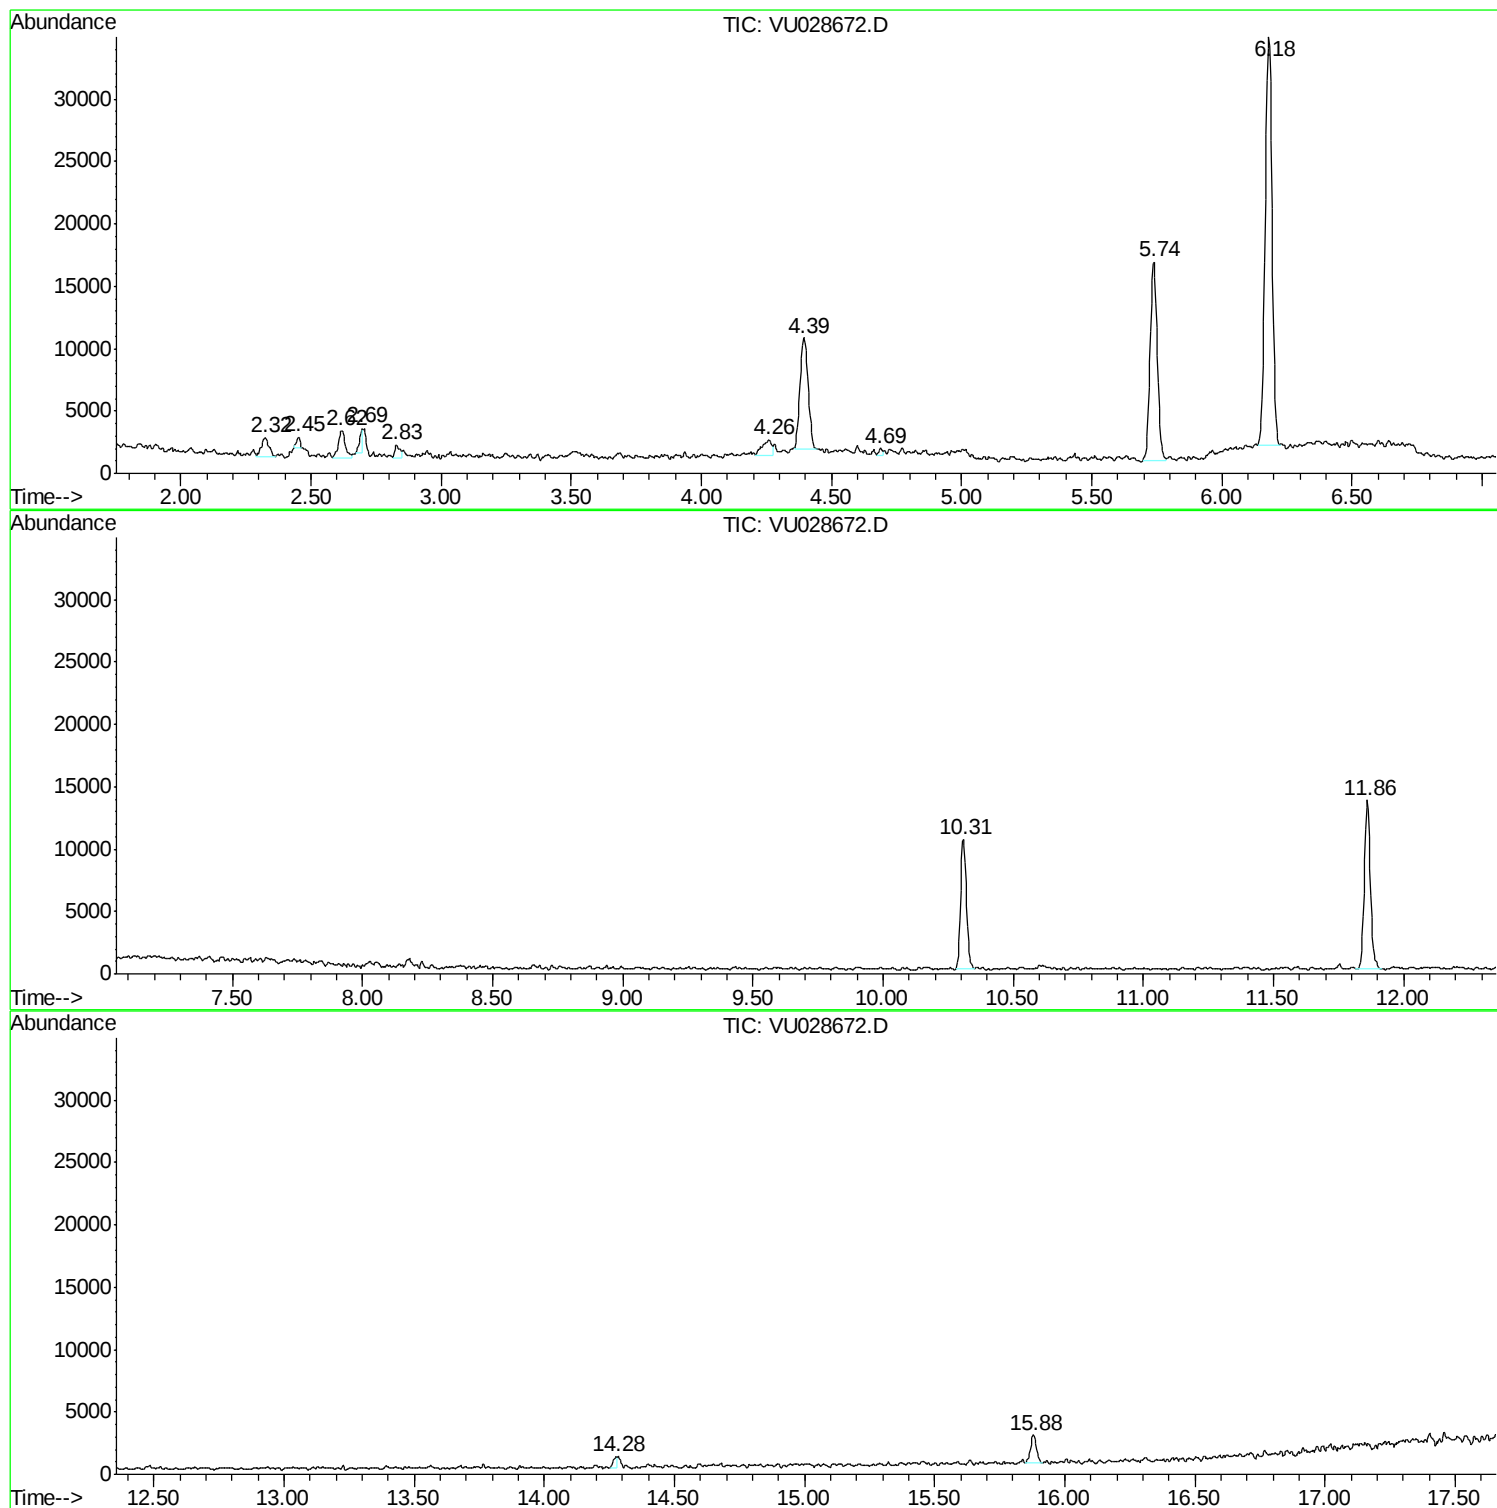

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121418\
Data File : VU028672.D
Acq On : 13 Dec 2018 12:15
Operator : MD/SY
Sample : J6347-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW001-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121418\
Data File : VU028672.D
Acq On : 13 Dec 2018 12:15
Operator : MD/SY
Sample : J6347-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW001-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc