

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121418\
 Data File : VU028673.D
 Acq On : 13 Dec 2018 12:43
 Operator : MD/SY
 Sample : J6347-18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 P001-TW002-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U112618DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.186	311	315	317	rBV	469	346	1.12%	0.359%
2	2.222	322	326	330	rBV2	329	347	1.12%	0.360%
3	2.318	351	356	363	rBV2	1288	1429	4.62%	1.483%
4	2.443	392	395	396	rBV2	601	326	1.05%	0.338%
5	2.501	409	413	418	rBV4	496	473	1.53%	0.491%
6	2.582	432	438	440	rBV2	463	429	1.39%	0.445%
7	2.617	444	449	457	rVB5	1199	2037	6.58%	2.115%
8	2.701	466	475	488	rVB3	3776	6675	21.58%	6.929%
9	2.829	510	515	519	rBV2	512	522	1.69%	0.542%
10	3.090	593	596	599	rBV2	505	372	1.20%	0.386%
11	3.524	727	731	733	rBV	345	327	1.06%	0.339%
12	4.398	995	1003	1010	rBV3	1236	2109	6.82%	2.189%
13	5.739	1408	1420	1431	rBV3	16031	30935	100.00%	32.113%
14	5.964	1487	1490	1493	rBV2	415	375	1.21%	0.389%
15	6.672	1707	1710	1713	rBV2	570	337	1.09%	0.350%
16	7.154	1857	1860	1863	rBV3	435	370	1.20%	0.384%
17	7.244	1885	1888	1895	rVB3	369	433	1.40%	0.449%
18	7.311	1904	1909	1912	rBV3	298	338	1.09%	0.351%
19	7.556	1983	1985	1992	rVB4	539	561	1.81%	0.582%
20	7.636	2004	2010	2016	rBV4	704	868	2.81%	0.901%
21	7.829	2068	2070	2075	rVB3	463	353	1.14%	0.366%
22	7.887	2082	2088	2092	rBV	263	321	1.04%	0.333%
23	8.170	2168	2176	2177	rBV3	566	587	1.90%	0.609%
24	8.189	2180	2182	2186	rVV	469	394	1.27%	0.409%
25	10.308	2833	2841	2853	rBV	10095	15706	50.77%	16.304%
26	10.604	2925	2933	2934	rBV	435	401	1.30%	0.416%
27	11.224	3122	3126	3131	rBV	352	375	1.21%	0.389%
28	11.752	3285	3290	3295	rBV3	358	490	1.58%	0.509%
29	11.861	3315	3324	3336	rBV2	13243	20594	66.57%	21.378%
30	12.308	3457	3463	3466	rBV2	345	394	1.27%	0.409%
31	14.279	4074	4076	4083	rVB2	768	762	2.46%	0.791%
32	15.800	4545	4549	4552	rBV2	366	320	1.03%	0.332%
33	15.877	4564	4573	4582	rBV3	2208	3696	11.95%	3.837%
34	16.745	4840	4843	4845	rBV3	559	325	1.05%	0.337%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121418\
Data File : VU028673.D
Acq On : 13 Dec 2018 12:43
Operator : MD/SY
Sample : J6347-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW002-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

35	16.935	4899	4902	4907	rbV4	714	709	2.29%	0.736%
36	17.054	4937	4939	4943	rbV2	550	389	1.26%	0.404%
37	17.147	4961	4968	4973	rbV4	551	906	2.93%	0.941%


Sum of corrected areas: 96331

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121418\
Data File : VU028673.D
Acq On : 13 Dec 2018 12:43
Operator : MD/SY
Sample : J6347-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW002-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

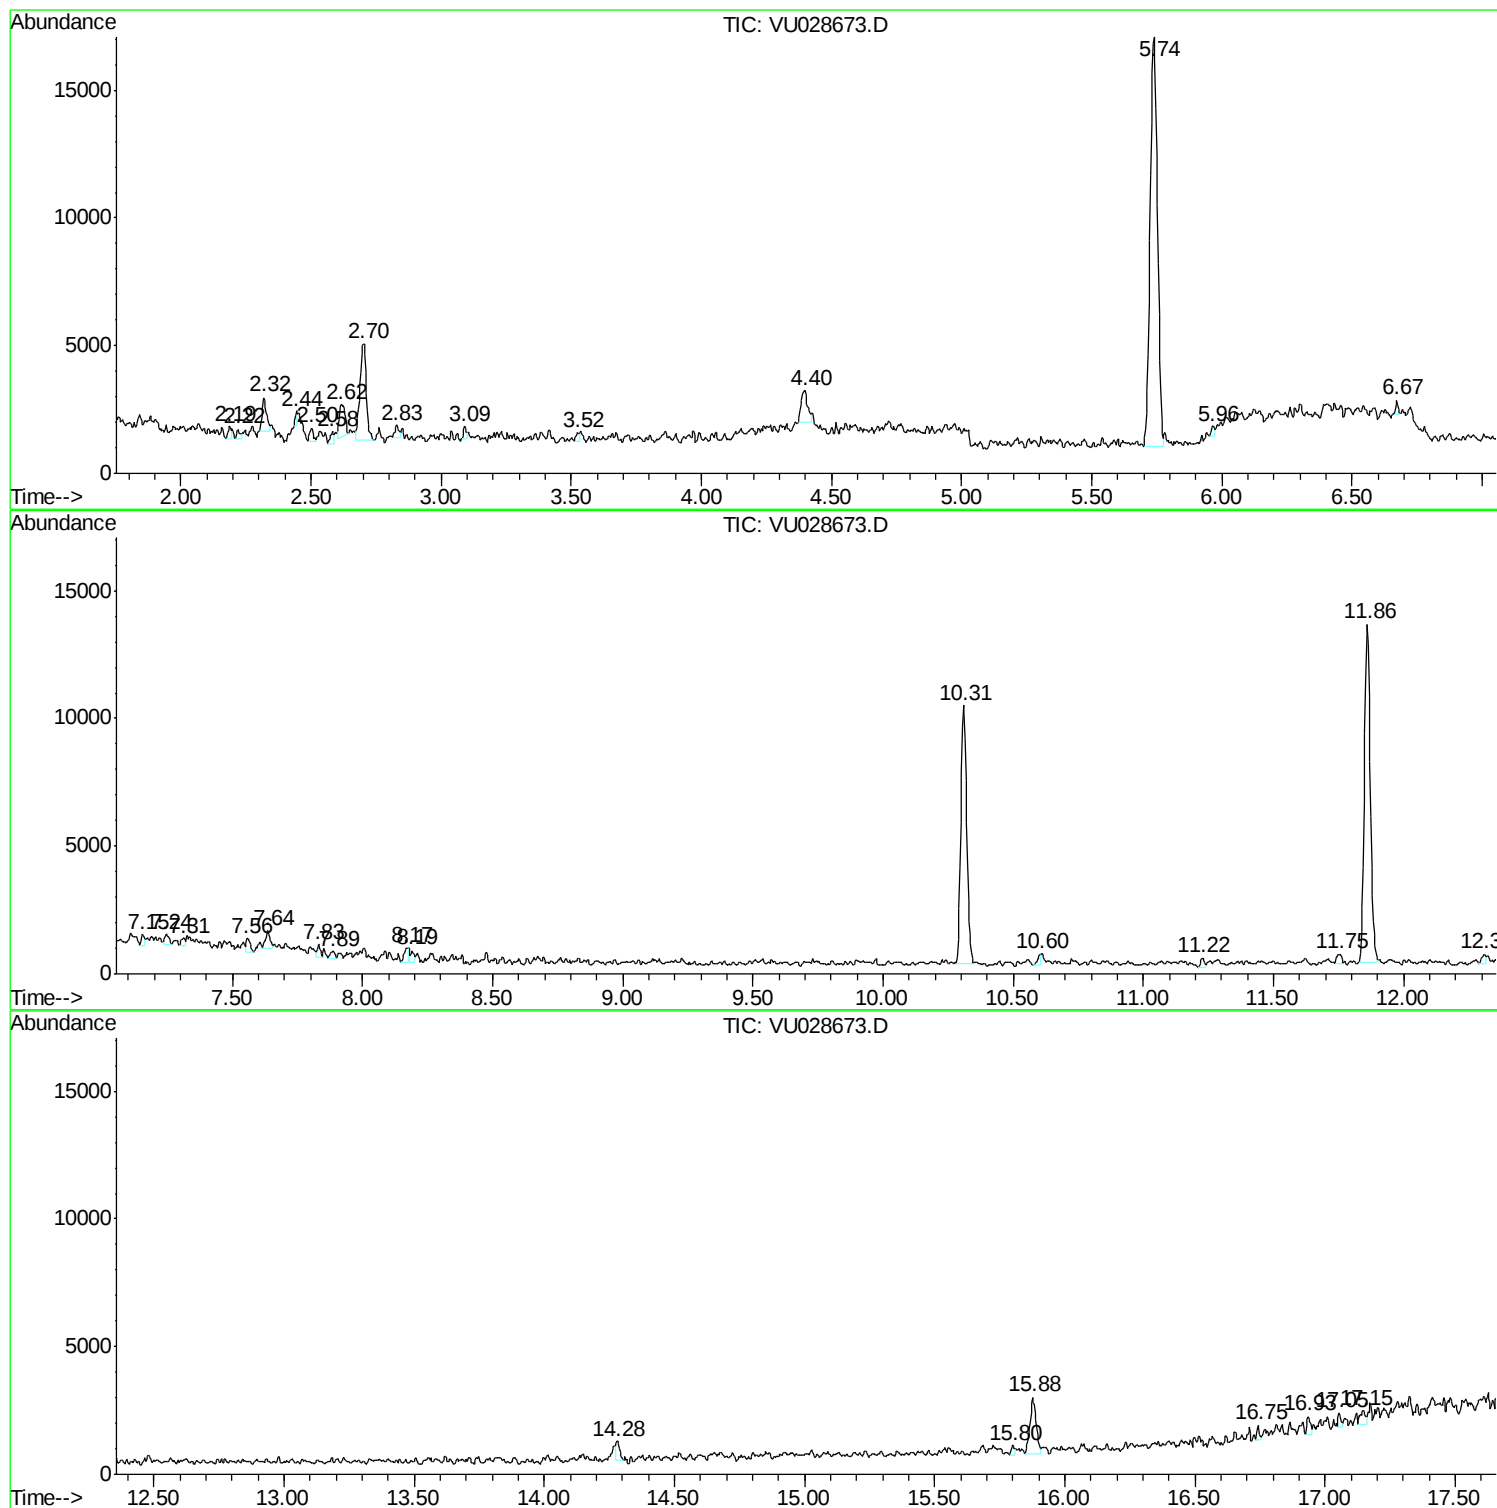

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121418\
Data File : VU028673.D
Acq On : 13 Dec 2018 12:43
Operator : MD/SY
Sample : J6347-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW002-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121418\
Data File : VU028673.D
Acq On : 13 Dec 2018 12:43
Operator : MD/SY
Sample : J6347-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW002-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc