

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121418\
 Data File : VU028675.D
 Acq On : 13 Dec 2018 13:41
 Operator : MD/SY
 Sample : J6347-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 P001-TW001-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.321	351	357	369	rVB2	1424	2549	4.22%	1.530%
2	2.450	389	397	401	rBV3	607	1064	1.76%	0.639%
3	2.617	440	449	460	rBV3	2068	4007	6.63%	2.406%
4	2.701	468	475	488	rVB4	2172	3327	5.51%	1.998%
5	2.836	510	517	518	rBV2	889	972	1.61%	0.584%
6	4.395	989	1002	1018	rBV2	7743	17287	28.62%	10.380%
7	5.736	1407	1419	1436	rBV	15784	30228	50.05%	18.150%
8	6.180	1545	1557	1571	rBV3	33147	60397	100.00%	36.264%
9	8.176	2172	2178	2181	rBV3	593	723	1.20%	0.434%
10	10.308	2829	2841	2852	rBV	11004	15996	26.48%	9.604%
11	11.861	3314	3324	3335	rBV2	13752	21253	35.19%	12.761%
12	14.276	4070	4075	4085	rVB3	1088	1744	2.89%	1.047%
13	14.967	4286	4290	4298	rBV2	403	624	1.03%	0.375%
14	15.880	4563	4574	4585	rBV	1942	3518	5.82%	2.112%
15	16.893	4885	4889	4893	rVB3	1121	883	1.46%	0.530%
16	17.031	4925	4932	4937	rBV5	891	1315	2.18%	0.790%
17	17.060	4937	4941	4946	rVB3	609	661	1.09%	0.397%


Sum of corrected areas: 166548

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121418\
Data File : VU028675.D
Acq On : 13 Dec 2018 13:41
Operator : MD/SY
Sample : J6347-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW001-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

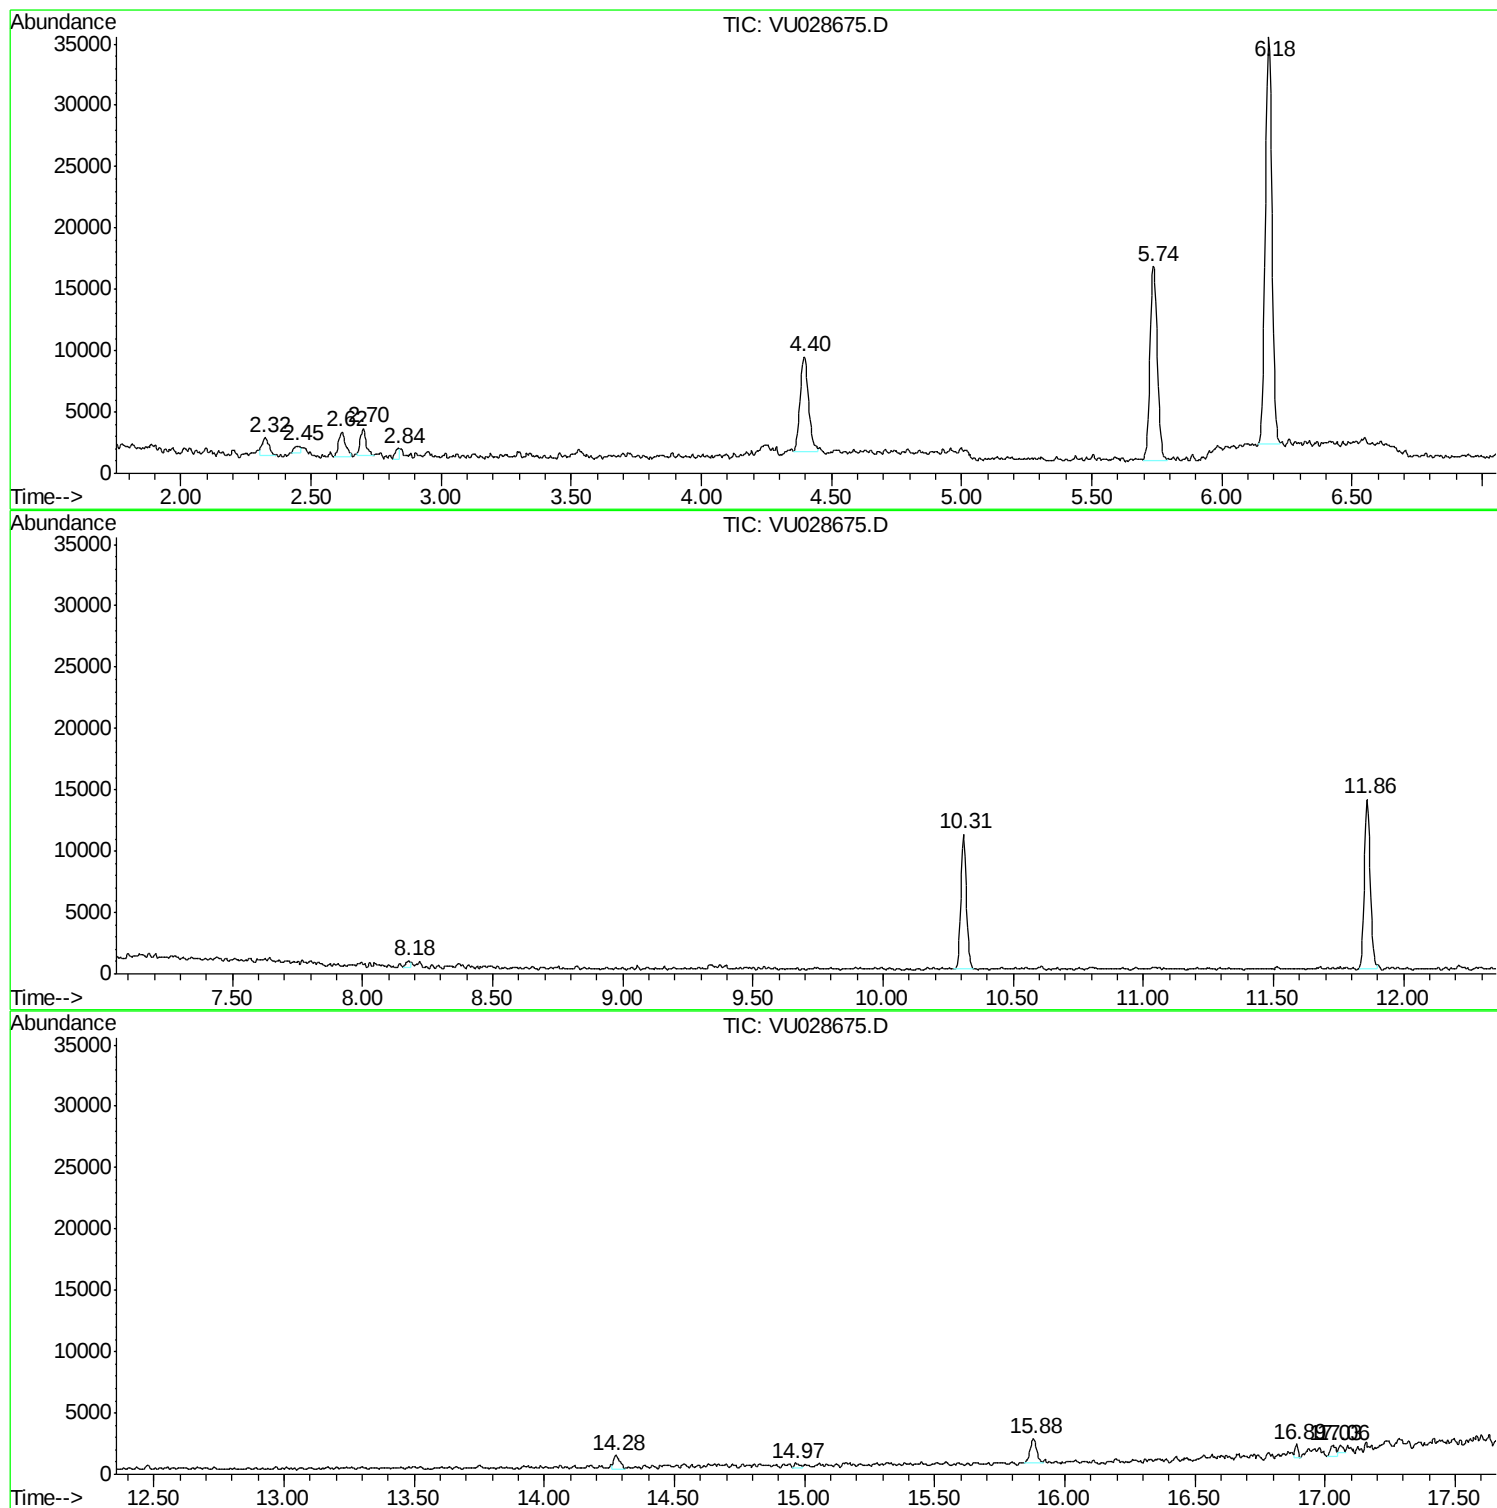

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121418\
Data File : VU028675.D
Acq On : 13 Dec 2018 13:41
Operator : MD/SY
Sample : J6347-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW001-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121418\
Data File : VU028675.D
Acq On : 13 Dec 2018 13:41
Operator : MD/SY
Sample : J6347-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P001-TW001-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc